

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036378.D
 Acq On : 22 Aug 2022 22:57
 Operator : CG/JU
 Sample : PB147176BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK176

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	31	rVB	84160	120783	2.18%	0.186%
2	3.628	90	92	111	rBV	985335	1577173	28.46%	2.431%
3	3.951	143	147	152	rVB	22533	30046	0.54%	0.046%
4	6.969	654	660	677	rBV	1146534	1891159	34.13%	2.915%
5	7.134	682	688	699	rVB	1011310	1564219	28.23%	2.411%
6	7.322	713	720	734	rBV	1173484	1887599	34.06%	2.909%
7	7.792	793	800	808	rBV	1047008	1613617	29.12%	2.487%
8	8.516	912	923	941	rBV	1344340	2275586	41.06%	3.507%
9	8.963	991	999	1010	rBV	1134188	1838764	33.18%	2.834%
10	9.680	1112	1121	1137	rBV	857426	1439644	25.98%	2.219%
11	10.222	1206	1213	1232	rBV	1200744	2185847	39.44%	3.369%
12	10.592	1266	1276	1289	rBV	1463289	2387976	43.09%	3.680%
13	10.739	1294	1301	1326	rBV	1223229	2382692	43.00%	3.672%
14	12.210	1545	1551	1556	rBV2	16072	31005	0.56%	0.048%
15	13.416	1752	1756	1763	rVB8	4087	7108	0.13%	0.011%
16	13.857	1824	1831	1845	rBV	2263458	3069746	55.39%	4.731%
17	14.133	1871	1878	1893	rBV	2665944	3945803	71.20%	6.081%
18	14.433	1923	1929	1942	rBV	2041859	2990387	53.96%	4.609%
19	14.663	1962	1968	1991	rBV	626643	1385244	25.00%	2.135%
20	15.427	2091	2098	2112	rBV	3508342	4833976	87.23%	7.450%
21	15.562	2115	2121	2136	rBV	708554	1149884	20.75%	1.772%
22	15.668	2136	2139	2145	rVB3	19661	31428	0.57%	0.048%
23	16.862	2338	2342	2345	rBV6	3110	5997	0.11%	0.009%
24	16.968	2355	2360	2366	rVB5	5215	10035	0.18%	0.015%
25	17.180	2390	2396	2406	rBV	2449665	3263926	58.90%	5.031%
26	17.280	2406	2413	2427	rVV	3661830	5047921	91.09%	7.780%
27	19.003	2704	2706	2709	rBV4	4502	5568	0.10%	0.009%
28	19.139	2725	2729	2735	rBV3	37872	53479	0.97%	0.082%
29	19.209	2737	2741	2746	rVV2	35931	47055	0.85%	0.073%
30	19.574	2797	2803	2815	rBV	4331563	5541728	100.00%	8.541%
31	20.574	2970	2973	2978	rBV2	61452	71878	1.30%	0.111%
32	21.362	3102	3107	3117	rBV	2716972	3398993	61.33%	5.239%
33	23.538	3470	3477	3491	rBV2	2812547	5416555	97.74%	8.348%
34	23.685	3496	3502	3514	rVB2	1680317	3379332	60.98%	5.208%

Sum of corrected areas: 64882153

Instrument :

BNA_M

ClientSampleId :




SBLK176

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036378.D
Acq On : 22 Aug 2022 22:57
Operator : CG/JU
Sample : PB147176BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK176

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

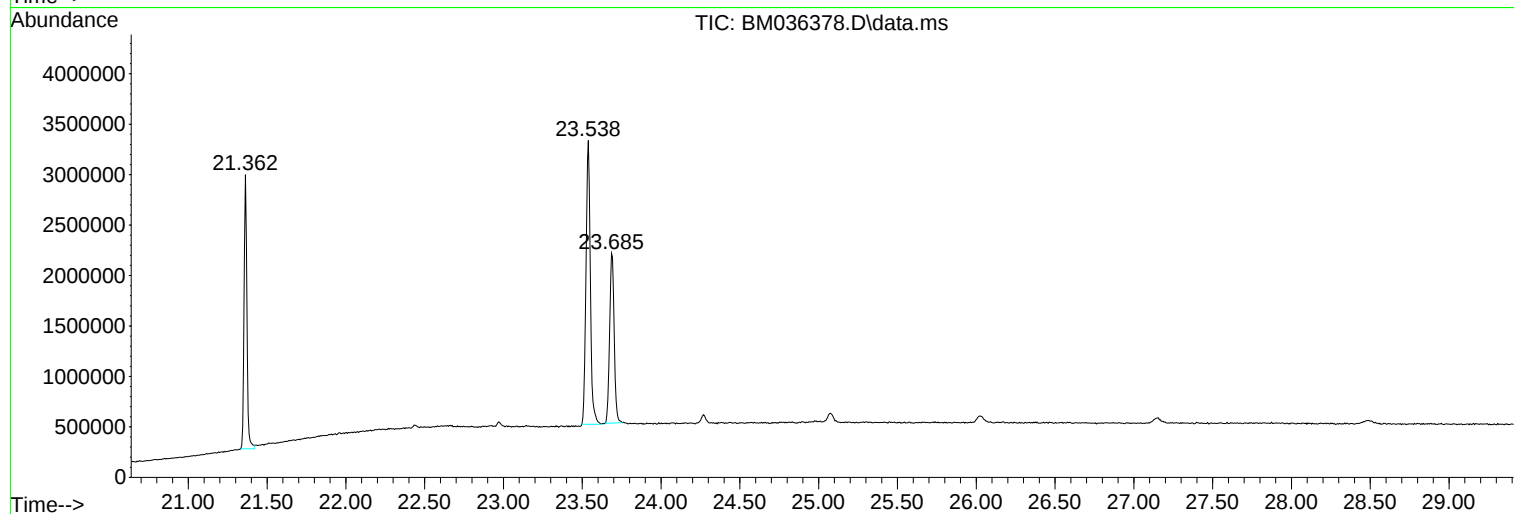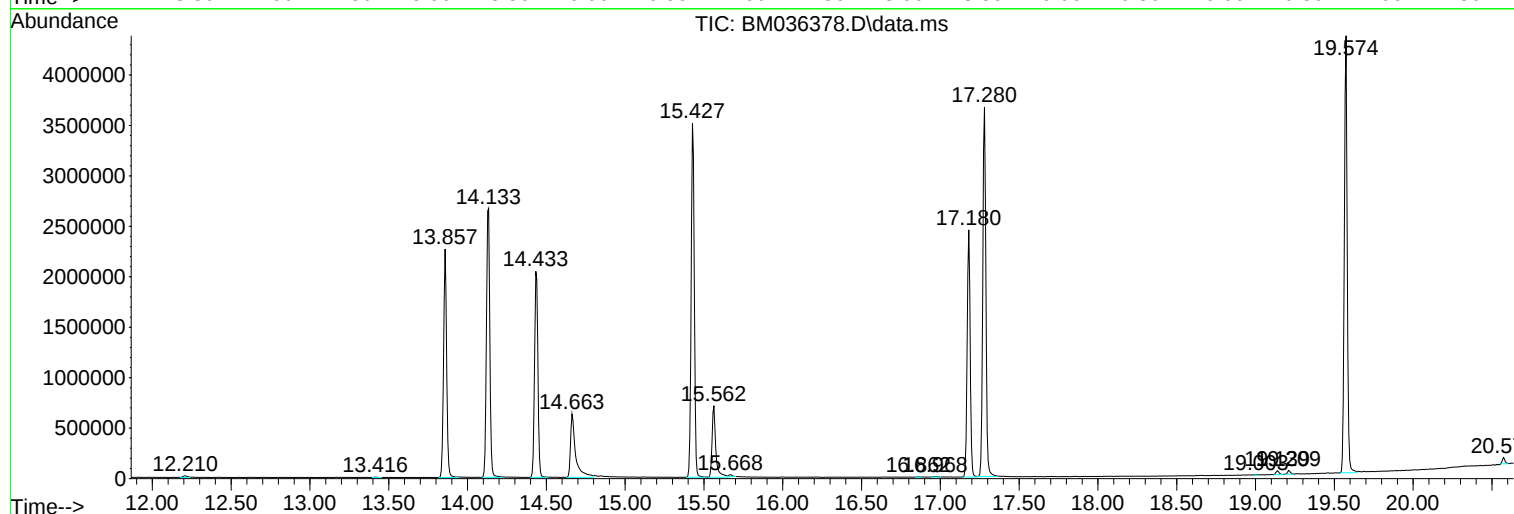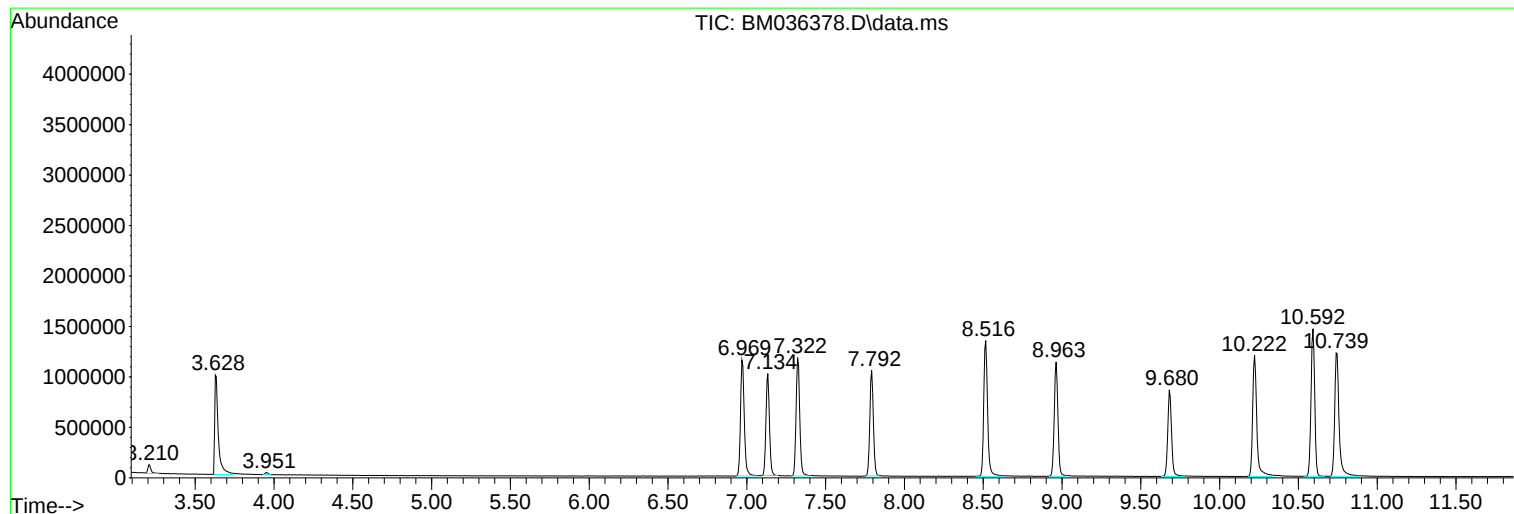

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036378.D
Acq On : 22 Aug 2022 22:57
Operator : CG/JU
Sample : PB147176BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK176

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036378.D
Acq On : 22 Aug 2022 22:57
Operator : CG/JU
Sample : PB147176BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK176

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc