

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036382.D
 Acq On : 23 Aug 2022 09:11
 Operator : CG/JU
 Sample : N4231-06DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0KN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	9	13	22	rBV	866121	1269656	33.83%	5.220%
2	3.240	22	26	35	rVB	169957	231878	6.18%	0.953%
3	3.663	96	98	104	rBV2	20148	37833	1.01%	0.156%
4	3.946	142	146	151	rVB	15723	21373	0.57%	0.088%
5	4.069	163	167	172	rVB5	6334	9370	0.25%	0.039%
6	4.475	230	236	252	rBV	2630160	3752844	100.00%	15.430%
7	5.222	358	363	367	rVB	8128	11354	0.30%	0.047%
8	6.904	645	649	653	rBB6	3094	4499	0.12%	0.018%
9	6.981	657	662	671	rBV3	15392	36910	0.98%	0.152%
10	7.128	681	687	701	rBV	115798	203278	5.42%	0.836%
11	7.322	714	720	732	rBV	83544	167928	4.47%	0.690%
12	7.463	742	744	751	rVB8	4421	4690	0.12%	0.019%
13	7.787	792	799	812	rBV	836465	1336823	35.62%	5.496%
14	8.522	919	924	937	rBV	57531	135140	3.60%	0.556%
15	8.963	992	999	1012	rBV	108745	216178	5.76%	0.889%
16	9.345	1062	1064	1069	rVB6	2641	4405	0.12%	0.018%
17	9.687	1115	1122	1131	rBV	71058	140660	3.75%	0.578%
18	10.234	1210	1215	1235	rBV	60185	204363	5.45%	0.840%
19	10.586	1267	1275	1287	rBV	1233505	2093413	55.78%	8.607%
20	10.757	1297	1304	1322	rBV2	76082	221445	5.90%	0.910%
21	11.833	1482	1487	1495	rVB9	2920	7156	0.19%	0.029%
22	13.857	1823	1831	1848	rBV	274679	449126	11.97%	1.847%
23	14.127	1871	1877	1890	rBV	345432	576410	15.36%	2.370%
24	14.433	1921	1929	1943	rBV	2028196	2888086	76.96%	11.875%
25	14.774	1981	1987	1990	rBV8	2873	6343	0.17%	0.026%
26	15.427	2092	2098	2111	rBV	441365	677320	18.05%	2.785%
27	15.574	2118	2123	2134	rBV3	27136	71721	1.91%	0.295%
28	16.639	2300	2304	2308	rVB6	3326	4300	0.11%	0.018%
29	16.968	2356	2360	2365	rVB2	4030	6096	0.16%	0.025%
30	17.174	2389	2395	2407	rVV	2111703	3055368	81.41%	12.562%
31	17.280	2407	2413	2427	rVV	423335	689182	18.36%	2.834%
32	17.710	2482	2486	2493	rVB9	3723	7371	0.20%	0.030%
33	18.098	2549	2552	2553	rBV3	4220	3976	0.11%	0.016%
34	19.574	2797	2803	2813	rBV	444619	656771	17.50%	2.700%
35	20.574	2970	2973	2979	rBV3	44810	60733	1.62%	0.250%
36	21.362	3102	3107	3116	rBV	1875340	2426313	64.65%	9.976%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036382.D
Acq On : 23 Aug 2022 09:11
Operator : CG/JU
Sample : N4231-06DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	23.539	3473	3477	3482	rBV	212575	356587	9.50%	1.466%
38	23.686	3497	3502	3519	rVB2	1103590	2274601	60.61%	9.352%




Sum of corrected areas: 24321500

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036382.D
Acq On : 23 Aug 2022 09:11
Operator : CG/JU
Sample : N4231-06DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

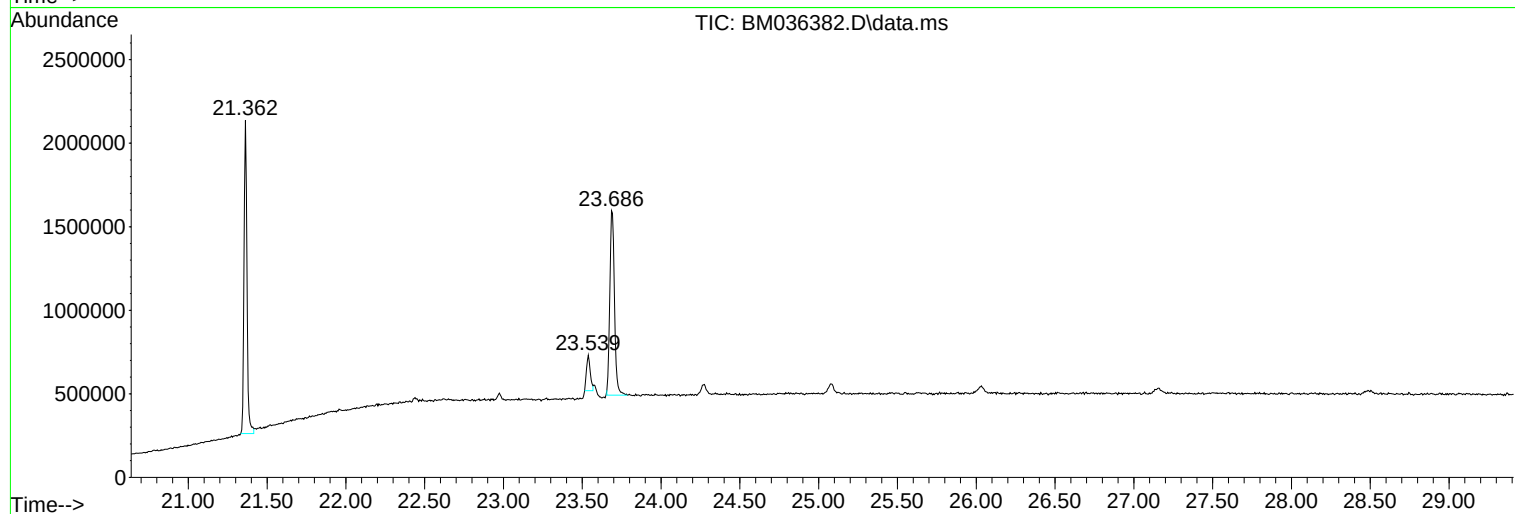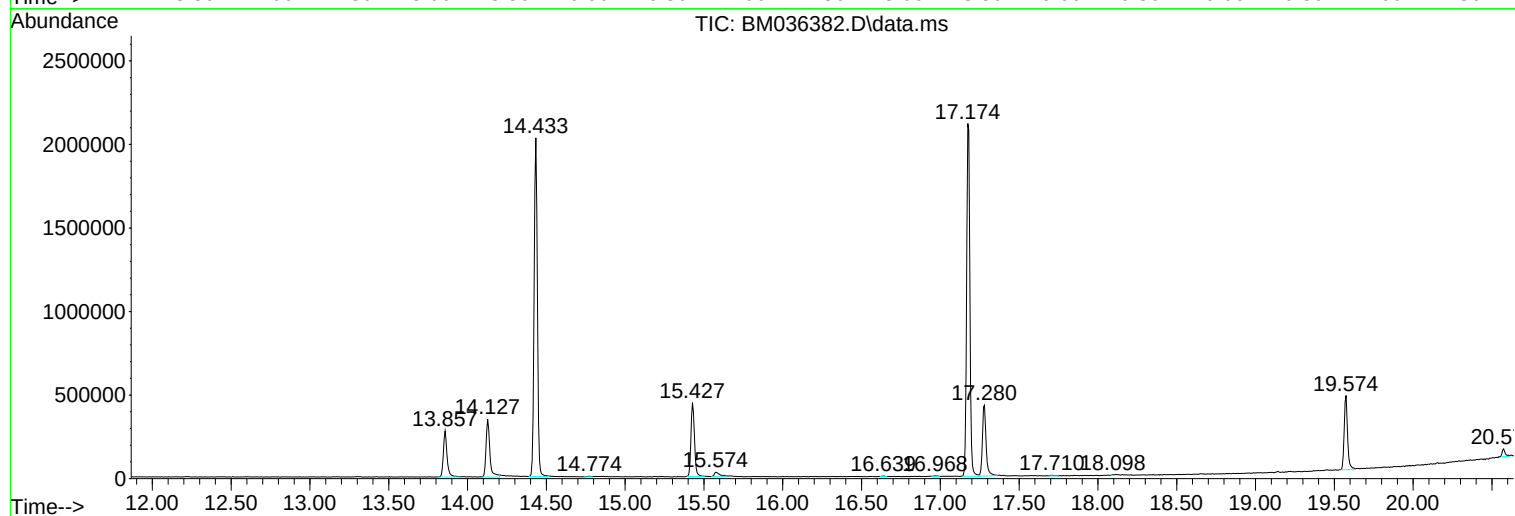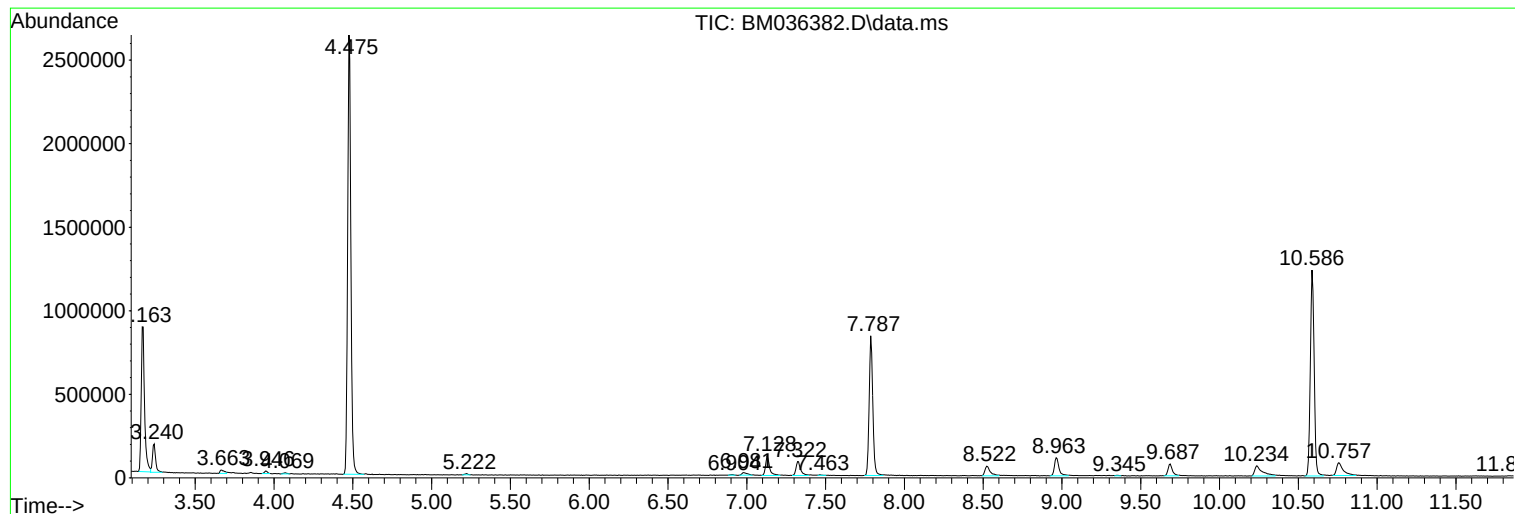

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036382.D
Acq On : 23 Aug 2022 09:11
Operator : CG/JU
Sample : N4231-06DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036382.D
Acq On : 23 Aug 2022 09:11
Operator : CG/JU
Sample : N4231-06DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0KN4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------