

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036386.D
 Acq On : 23 Aug 2022 12:04
 Operator : CG/JU
 Sample : PB147178BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK178

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	26	rVB	67664	91158	1.73%	0.150%
2	3.628	88	92	114	rBV	851953	1419600	26.94%	2.339%
3	3.946	143	146	151	rBV	18164	24508	0.47%	0.040%
4	6.963	651	659	676	rBV	1039501	1711736	32.49%	2.821%
5	7.128	680	687	696	rBV	934063	1439942	27.33%	2.373%
6	7.316	712	719	741	rBV	1047893	1692770	32.13%	2.789%
7	7.786	792	799	813	rBV	874814	1372381	26.05%	2.261%
8	8.510	915	922	937	rBV	1301545	2157239	40.94%	3.555%
9	8.957	990	998	1011	rBV	1101738	1762780	33.45%	2.905%
10	9.675	1112	1120	1134	rBV	803793	1385520	26.29%	2.283%
11	10.216	1205	1212	1231	rBV	1183266	2133998	40.50%	3.516%
12	10.586	1267	1275	1287	rBV	1352099	2207755	41.90%	3.638%
13	10.739	1292	1301	1329	rBV	1240619	2392785	45.41%	3.943%
14	12.198	1542	1549	1559	rBV2	15905	41098	0.78%	0.068%
15	13.416	1750	1756	1760	rBV5	4512	7084	0.13%	0.012%
16	13.857	1824	1831	1846	rBV	2338758	3330274	63.20%	5.488%
17	14.127	1869	1877	1893	rBV	2975385	4141794	78.60%	6.825%
18	14.433	1922	1929	1939	rBV	2168815	3006836	57.06%	4.955%
19	14.663	1960	1968	1994	rBV	572686	1360514	25.82%	2.242%
20	15.427	2088	2098	2112	rBV	3818705	5209976	98.88%	8.585%
21	15.557	2114	2120	2136	rVV	725788	1172736	22.26%	1.932%
22	15.668	2136	2139	2147	rVB3	20340	35471	0.67%	0.058%
23	15.992	2190	2194	2199	rBV7	3922	7463	0.14%	0.012%
24	16.209	2228	2231	2234	rVB5	4703	5557	0.11%	0.009%
25	16.639	2300	2304	2309	rVB4	6628	9954	0.19%	0.016%
26	16.974	2357	2361	2366	rVB7	4225	5621	0.11%	0.009%
27	17.174	2389	2395	2405	rBV	2326494	3275148	62.16%	5.397%
28	17.274	2406	2412	2430	rVB	3694070	5269201	100.00%	8.683%
29	17.709	2483	2486	2490	rVB6	5934	8322	0.16%	0.014%
30	18.656	2644	2647	2652	rVB6	6387	8843	0.17%	0.015%
31	19.139	2724	2729	2734	rBV	34784	51742	0.98%	0.085%
32	19.209	2737	2741	2748	rVV3	29380	45830	0.87%	0.076%
33	19.574	2797	2803	2814	rBV	3795916	5099897	96.79%	8.404%
34	20.574	2969	2973	2977	rBV	139479	166754	3.16%	0.275%
35	21.362	3102	3107	3117	rBV	1925624	2519358	47.81%	4.151%
36	23.538	3470	3477	3491	rBV	2031191	3904806	74.11%	6.434%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036386.D
Acq On : 23 Aug 2022 12:04
Operator : CG/JU
Sample : PB147178BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	23.685	3497	3502	3514	rVB2	1123556	2210242	41.95%	3.642%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 60686693

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036386.D
Acq On : 23 Aug 2022 12:04
Operator : CG/JU
Sample : PB147178BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

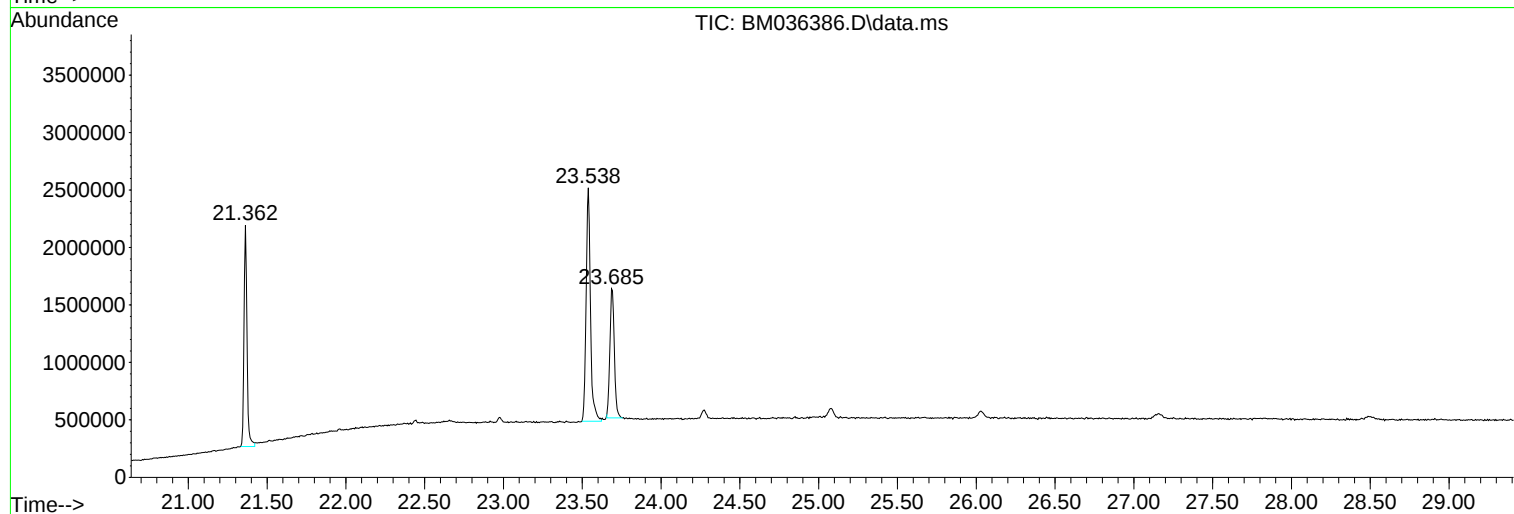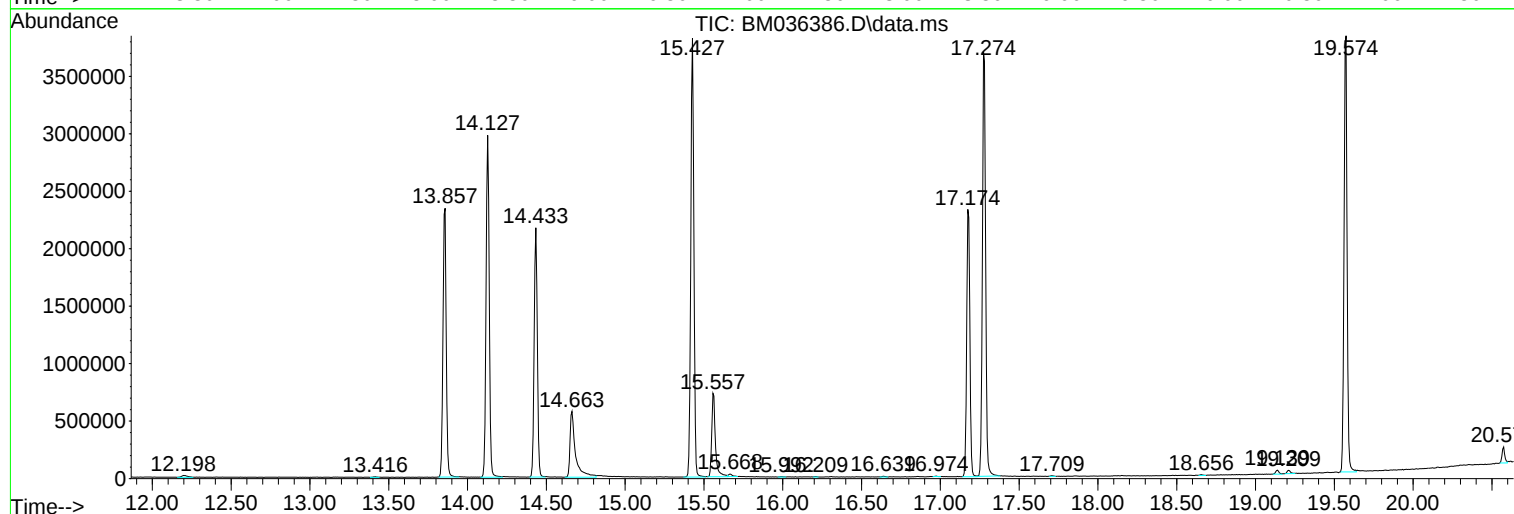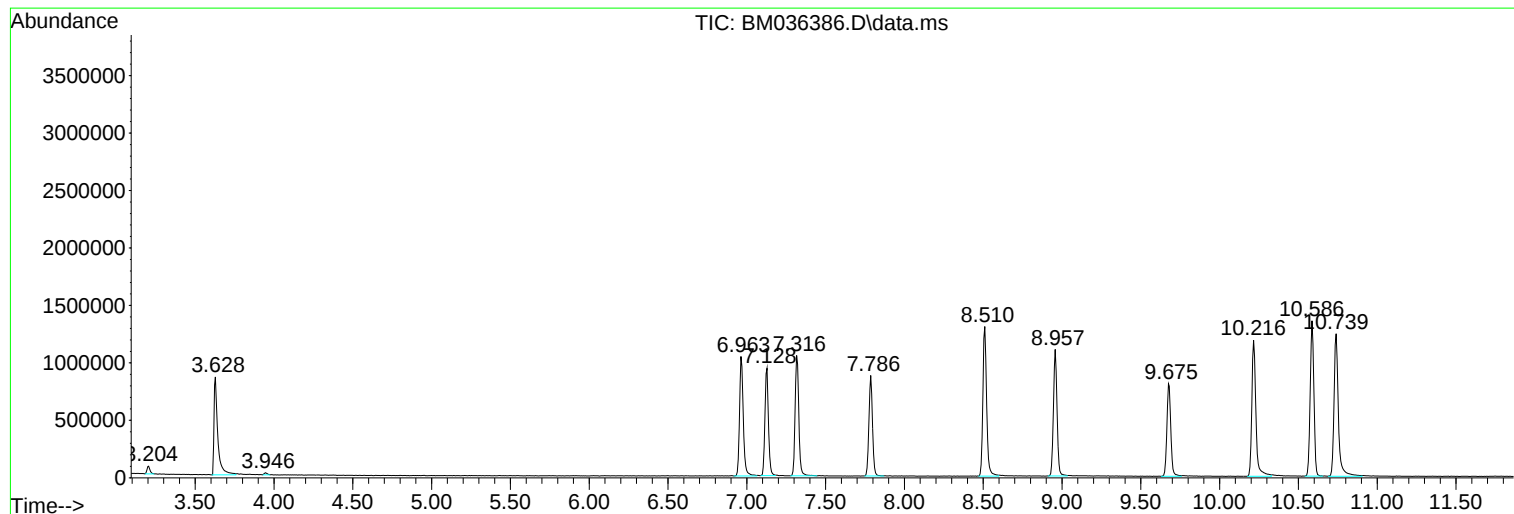

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036386.D
Acq On : 23 Aug 2022 12:04
Operator : CG/JU
Sample : PB147178BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036386.D
Acq On : 23 Aug 2022 12:04
Operator : CG/JU
Sample : PB147178BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK178

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------