

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036387.D
 Acq On : 23 Aug 2022 12:41
 Operator : CG/JU
 Sample : N4251-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	26	rVB	56560	71054	1.49%	0.146%
2	3.640	92	94	112	rBV	129698	237171	4.96%	0.486%
3	3.852	125	130	137	rVB	34722	57436	1.20%	0.118%
4	3.952	143	147	151	rVB	19392	25927	0.54%	0.053%
5	4.393	219	222	227	rVB	10782	15550	0.33%	0.032%
6	4.481	233	237	240	rVB4	10112	13338	0.28%	0.027%
7	5.793	455	460	464	rBV8	3439	5451	0.11%	0.011%
8	6.904	643	649	654	rBV6	4576	9401	0.20%	0.019%
9	6.969	655	660	674	rBV	173079	323490	6.76%	0.663%
10	7.128	681	687	700	rBV	841859	1321015	27.62%	2.707%
11	7.322	713	720	729	rBV	738388	1175729	24.58%	2.409%
12	7.398	731	733	739	rVB6	9619	13705	0.29%	0.028%
13	7.792	792	800	811	rBV	794004	1315781	27.51%	2.696%
14	8.516	916	923	937	rBV	544068	956802	20.01%	1.961%
15	8.963	991	999	1016	rBV	964815	1614296	33.75%	3.308%
16	9.345	1061	1064	1069	rVB6	5291	8465	0.18%	0.017%
17	9.681	1114	1121	1138	rBV	711625	1195055	24.99%	2.449%
18	10.222	1206	1213	1231	rBV	902343	1677377	35.07%	3.437%
19	10.592	1268	1276	1287	rBV	1255823	2055367	42.98%	4.212%
20	10.739	1294	1301	1320	rBV	806814	1606874	33.60%	3.293%
21	12.210	1544	1551	1558	rBV5	11547	26676	0.56%	0.055%
22	13.857	1824	1831	1845	rBV	2017395	2816167	58.88%	5.771%
23	14.127	1870	1877	1889	rBV	2484263	3512502	73.44%	7.198%
24	14.204	1889	1890	1895	rVB5	3962	5239	0.11%	0.011%
25	14.433	1922	1929	1939	rBV	1910889	2677564	55.98%	5.487%
26	14.692	1968	1973	1982	rBV3	36637	115033	2.41%	0.236%
27	14.851	1997	2000	2003	rVB3	4666	5219	0.11%	0.011%
28	14.892	2003	2007	2011	rVB6	5026	8257	0.17%	0.017%
29	15.427	2089	2098	2111	rBV	3228779	4349353	90.94%	8.912%
30	15.563	2115	2121	2135	rVV	555648	923095	19.30%	1.892%
31	15.668	2136	2139	2145	rVB3	16727	29694	0.62%	0.061%
32	16.968	2353	2360	2363	rBV7	3824	6874	0.14%	0.014%
33	17.180	2389	2396	2406	rBV	1894030	2640190	55.20%	5.410%
34	17.280	2406	2413	2430	rVV	3289656	4782684	100.00%	9.800%
35	18.109	2549	2554	2556	rBV6	5536	9241	0.19%	0.019%
36	19.139	2725	2729	2733	rBV2	26072	34947	0.73%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036387.D
Acq On : 23 Aug 2022 12:41
Operator : CG/JU
Sample : N4251-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN74

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	19.209	2737	2741	2745	rBV	29930	36567	0.76%	0.075%
38	19.574	2797	2803	2818	rBV	3650074	4658988	97.41%	9.547%
39	20.574	2970	2973	2977	rBV2	52957	61806	1.29%	0.127%
40	21.362	3102	3107	3117	rBV	1748362	2202832	46.06%	4.514%
41	23.539	3470	3477	3490	rBV2	2057175	4089215	85.50%	8.379%
42	23.686	3496	3502	3513	rVB2	1052277	2110051	44.12%	4.324%




Sum of corrected areas: 48801478

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036387.D
Acq On : 23 Aug 2022 12:41
Operator : CG/JU
Sample : N4251-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

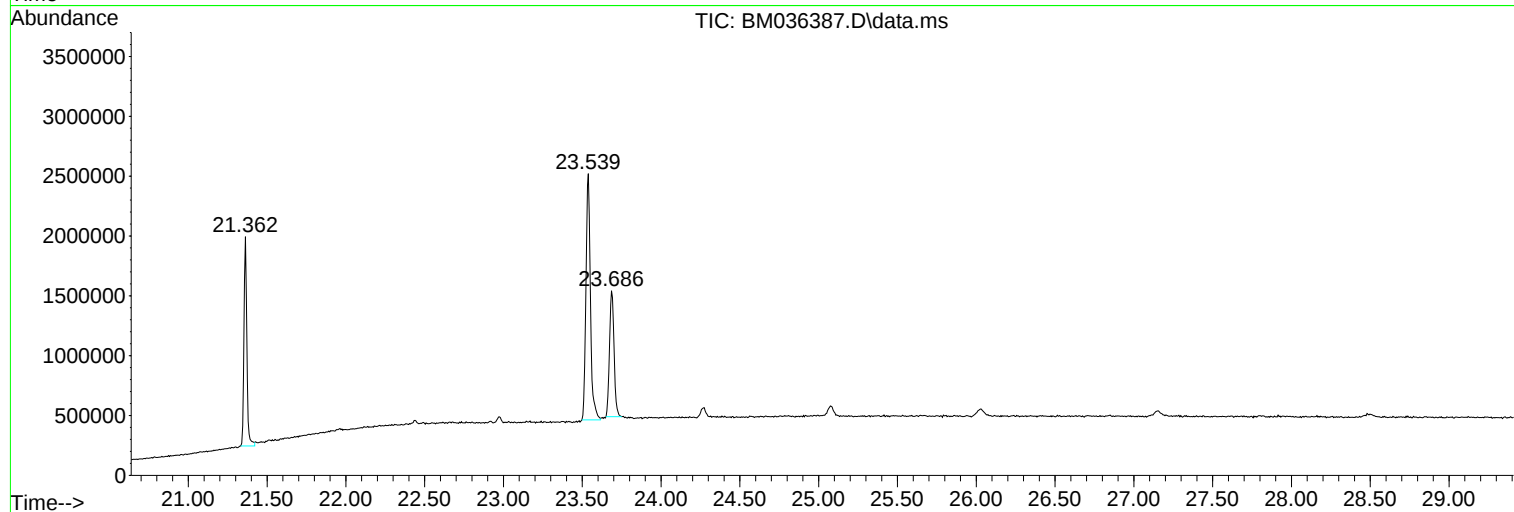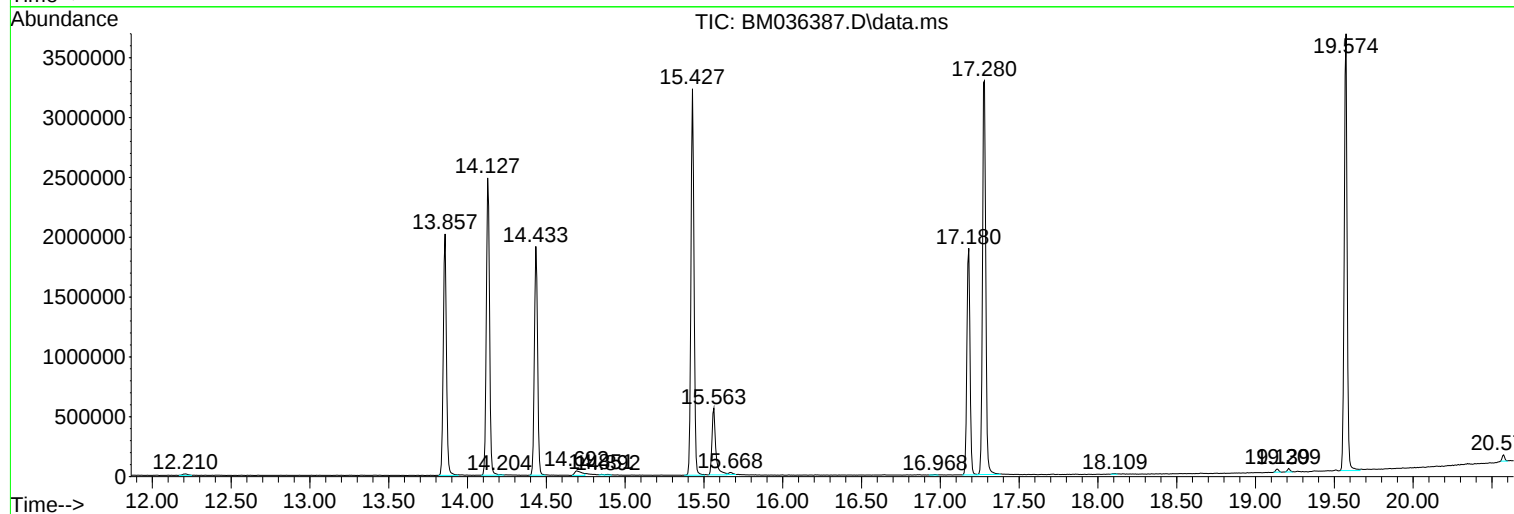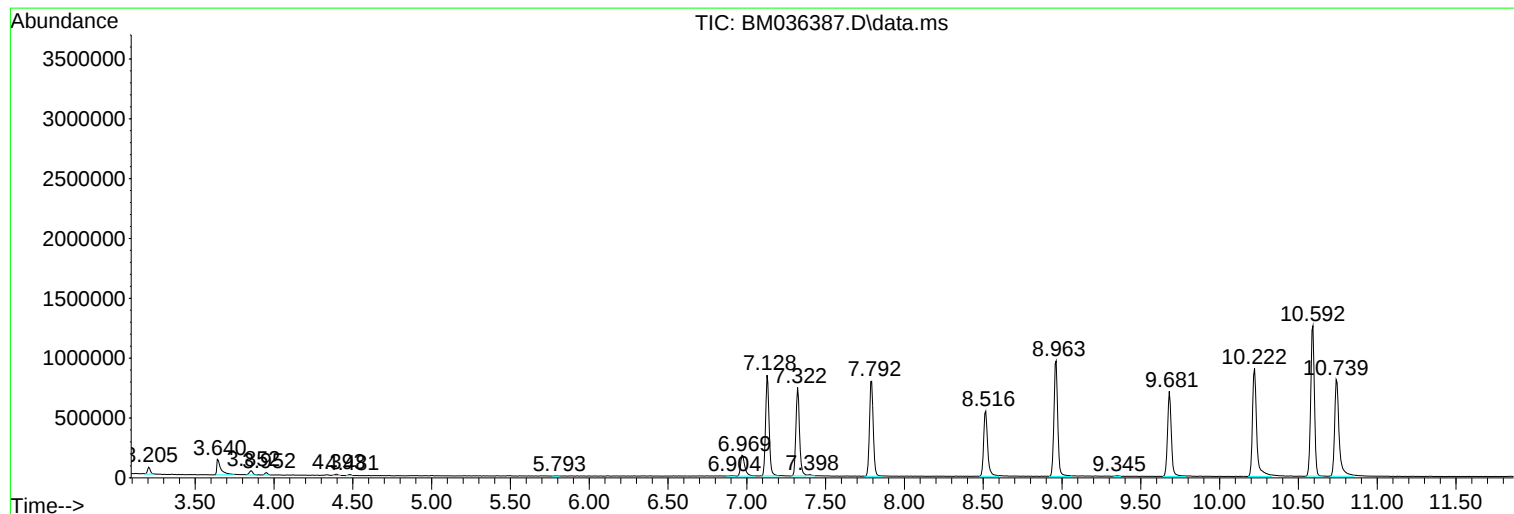

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036387.D
Acq On : 23 Aug 2022 12:41
Operator : CG/JU
Sample : N4251-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036387.D
Acq On : 23 Aug 2022 12:41
Operator : CG/JU
Sample : N4251-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN74

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc