

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
 Data File : BM036392.D
 Acq On : 23 Aug 2022 16:22
 Operator : CG/JU
 Sample : PB147163BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	16	20	29	rVB	84061	109344	2.24%	0.185%
2	3.628	89	92	114	rBV	1025529	1563909	32.07%	2.640%
3	3.951	143	147	154	rVB	19662	26223	0.54%	0.044%
4	6.969	653	660	673	rBV	1201135	1940190	39.78%	3.275%
5	7.134	681	688	701	rBV	1020791	1625089	33.32%	2.743%
6	7.322	713	720	734	rBV	1213517	1912505	39.22%	3.229%
7	7.792	793	800	817	rBV	872620	1394453	28.59%	2.354%
8	7.975	829	831	836	rBV6	3511	5590	0.11%	0.009%
9	8.516	915	923	943	rBV	1381709	2390525	49.02%	4.036%
10	8.963	991	999	1015	rBV	1177832	1955175	40.09%	3.301%
11	9.680	1114	1121	1134	rBV	930374	1533848	31.45%	2.589%
12	10.222	1206	1213	1237	rBV	1240202	2297353	47.11%	3.878%
13	10.592	1268	1276	1286	rBV	1273735	2097246	43.00%	3.541%
14	10.745	1294	1302	1330	rBV	1285511	2505866	51.38%	4.230%
15	12.210	1545	1551	1560	rBV2	16947	40446	0.83%	0.068%
16	13.416	1753	1756	1761	rVB6	4447	6616	0.14%	0.011%
17	13.857	1824	1831	1845	rBV	2359419	3261873	66.88%	5.507%
18	14.133	1871	1878	1890	rBV	2787439	4077018	83.60%	6.883%
19	14.433	1923	1929	1941	rBV	1758334	2585424	53.01%	4.365%
20	14.663	1959	1968	1997	rBV	520041	1303561	26.73%	2.201%
21	14.851	1997	2000	2006	rVB8	6650	12150	0.25%	0.021%
22	15.427	2091	2098	2113	rBV	3422902	4876873	100.00%	8.233%
23	15.562	2115	2121	2135	rVV	704085	1100988	22.58%	1.859%
24	15.668	2135	2139	2145	rVB3	18303	33084	0.68%	0.056%
25	16.209	2227	2231	2235	rBV7	5421	7363	0.15%	0.012%
26	16.862	2339	2342	2346	rBV5	3794	6155	0.13%	0.010%
27	17.180	2390	2396	2405	rBV	1897656	2529812	51.87%	4.271%
28	17.280	2406	2413	2432	rVV	3359159	4696661	96.30%	7.929%
29	19.139	2725	2729	2733	rBV3	32272	46928	0.96%	0.079%
30	19.209	2738	2741	2747	rVV	26843	38977	0.80%	0.066%
31	19.574	2797	2803	2816	rBV	3654062	4650420	95.36%	7.851%
32	20.574	2970	2973	2977	rBV2	69332	81243	1.67%	0.137%
33	21.362	3102	3107	3116	rBV	1596006	2222185	45.57%	3.751%
34	23.538	3470	3477	3491	rBV2	2118390	4215621	86.44%	7.117%
35	23.691	3497	3503	3514	rVB2	1029196	2085106	42.75%	3.520%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036392.D
Acq On : 23 Aug 2022 16:22
Operator : CG/JU
Sample : PB147163BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 59235820

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036392.D
Acq On : 23 Aug 2022 16:22
Operator : CG/JU
Sample : PB147163BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

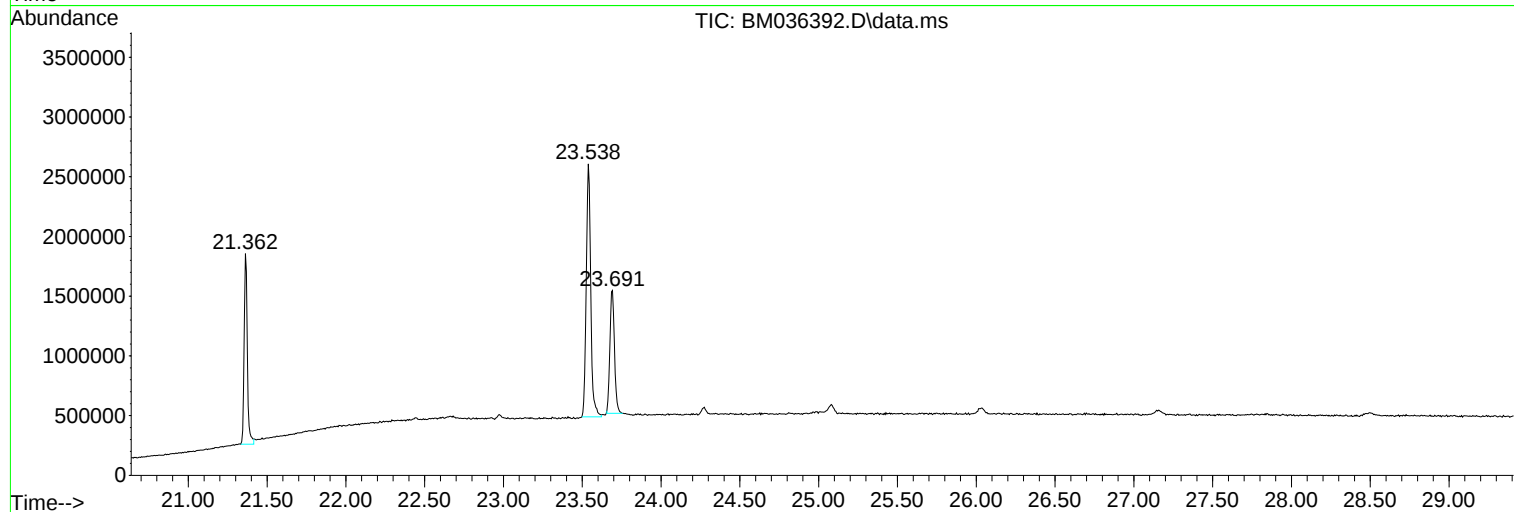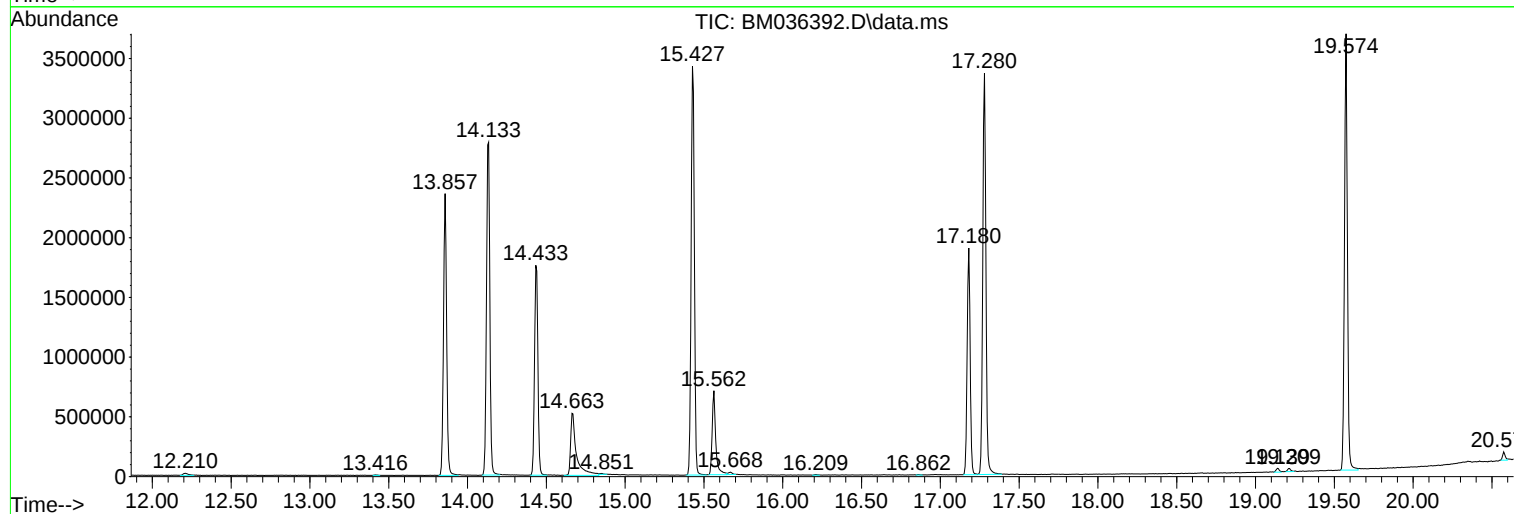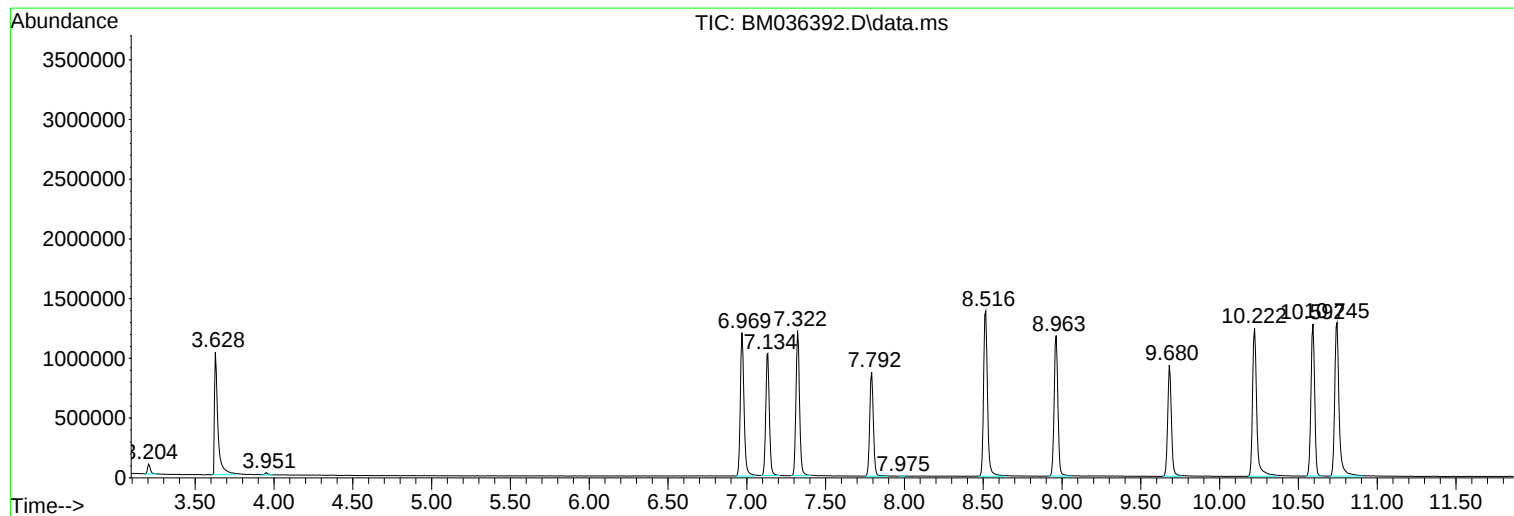

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036392.D
Acq On : 23 Aug 2022 16:22
Operator : CG/JU
Sample : PB147163BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082222\
Data File : BM036392.D
Acq On : 23 Aug 2022 16:22
Operator : CG/JU
Sample : PB147163BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc