

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
 Data File : BM047313.D
 Acq On : 22 Aug 2024 12:32
 Operator : RC/JU
 Sample : PB162757BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB162757BL

Quant Time: Aug 22 13:30:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 11 23:47:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.351	152	292730	20.000	ng	-0.02
21) Naphthalene-d8	10.104	136	1111486	20.000	ng	-0.03
39) Acenaphthene-d10	14.010	164	771992	20.000	ng	-0.02
64) Phenanthrene-d10	16.774	188	1724658	20.000	ng	-0.02
76) Chrysene-d12	21.015	240	1583438	20.000	ng	-0.02
86) Perylene-d12	23.709	264	1534865	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.010	112	1962459	119.790	ng	-0.01
7) Phenol-d6	6.569	99	2501470	110.813	ng	-0.02
23) Nitrobenzene-d5	8.504	82	1655941	75.019	ng	-0.02
42) 2,4,6-Tribromophenol	15.527	330	1174894	131.253	ng	-0.01
45) 2-Fluorobiphenyl	12.621	172	3958679	79.099	ng	-0.02
79) Terphenyl-d14	19.445	244	7120475	96.357	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.504	77	198	Below Cal	Qvalue #	3

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047313.D
Acq On : 22 Aug 2024 12:32
Operator : RC/JU
Sample : PB162757BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162757BL


Quant Time: Aug 22 13:30:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

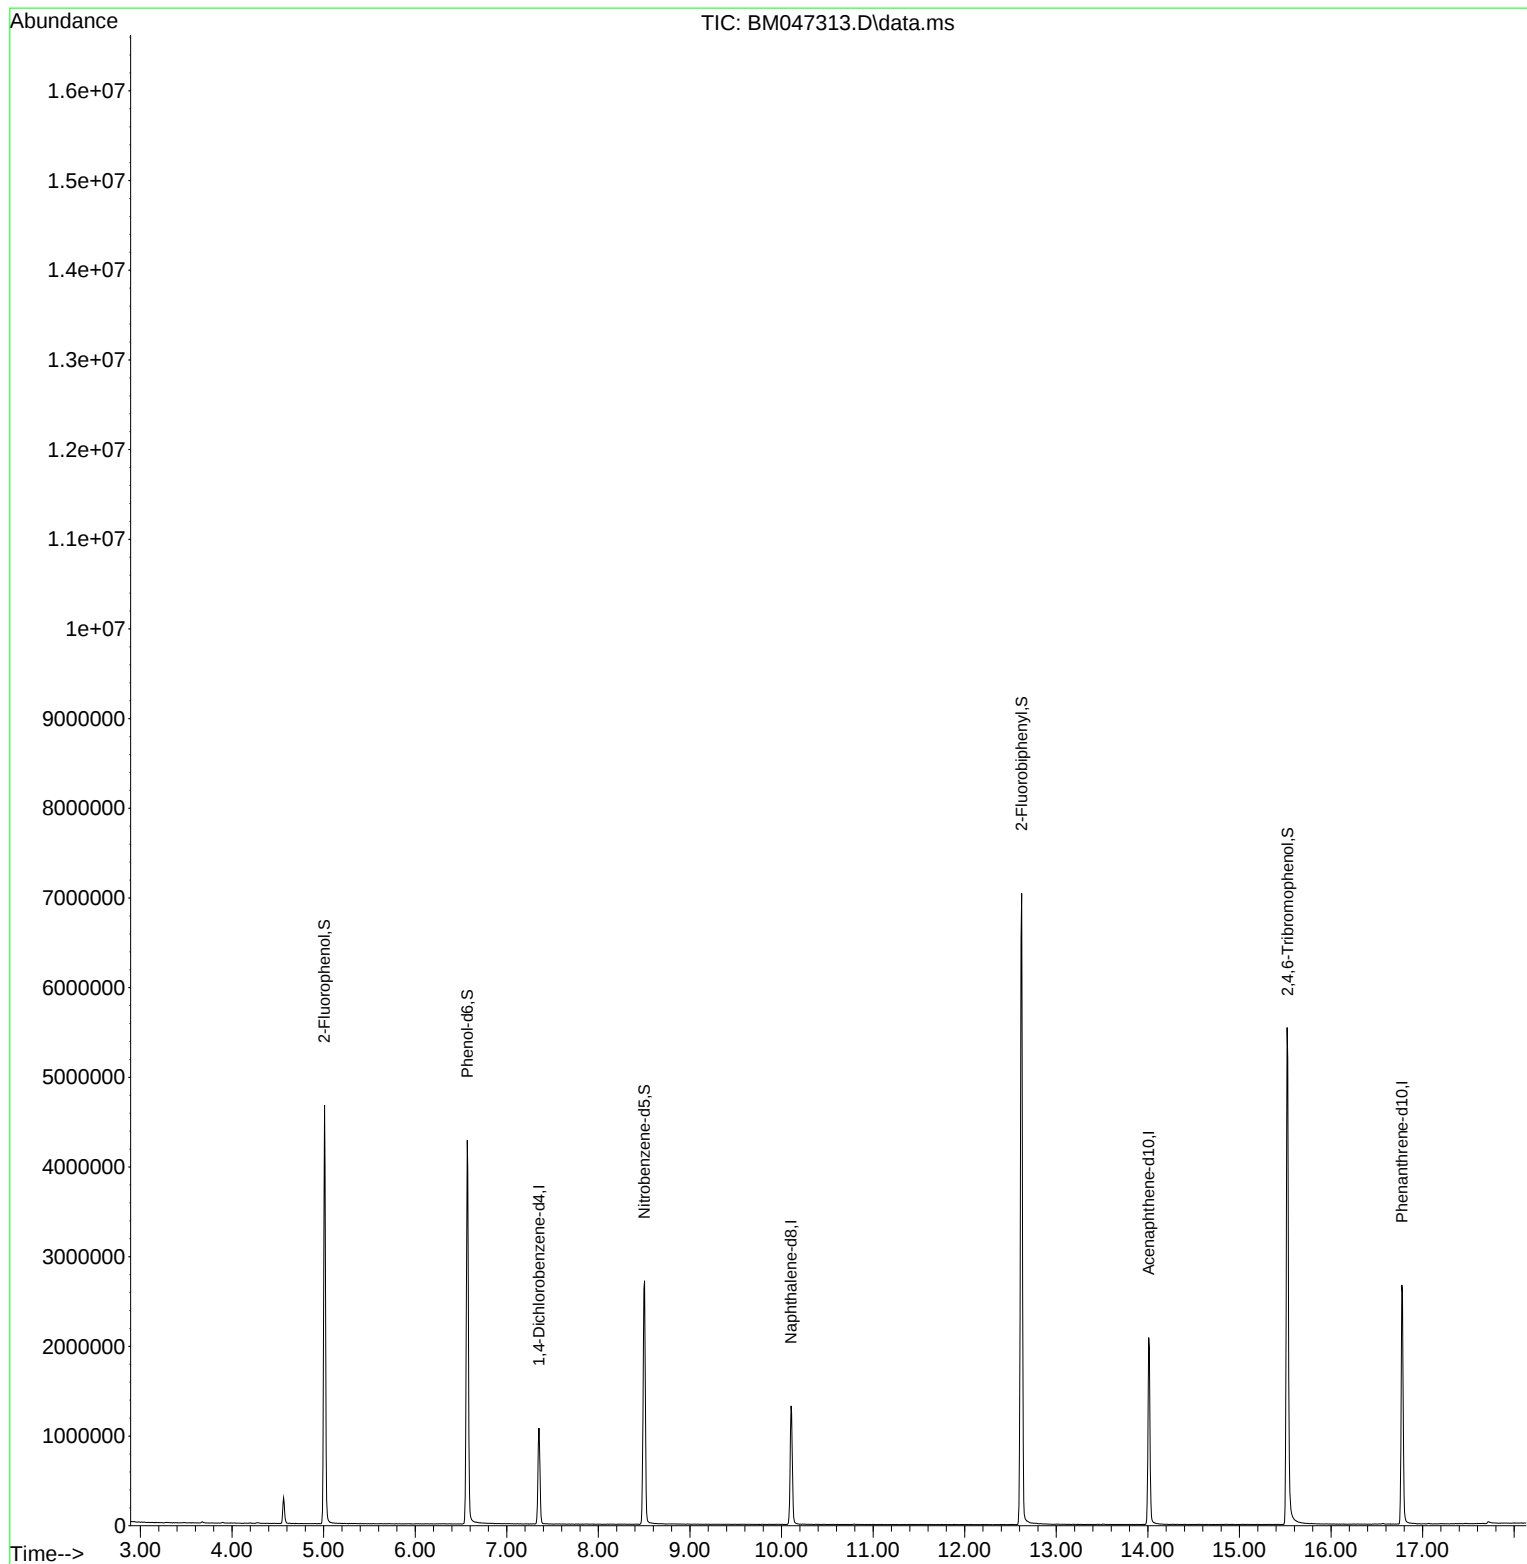


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047313.D
Acq On : 22 Aug 2024 12:32
Operator : RC/JU
Sample : PB162757BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162757BL

Quant Time: Aug 22 13:30:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

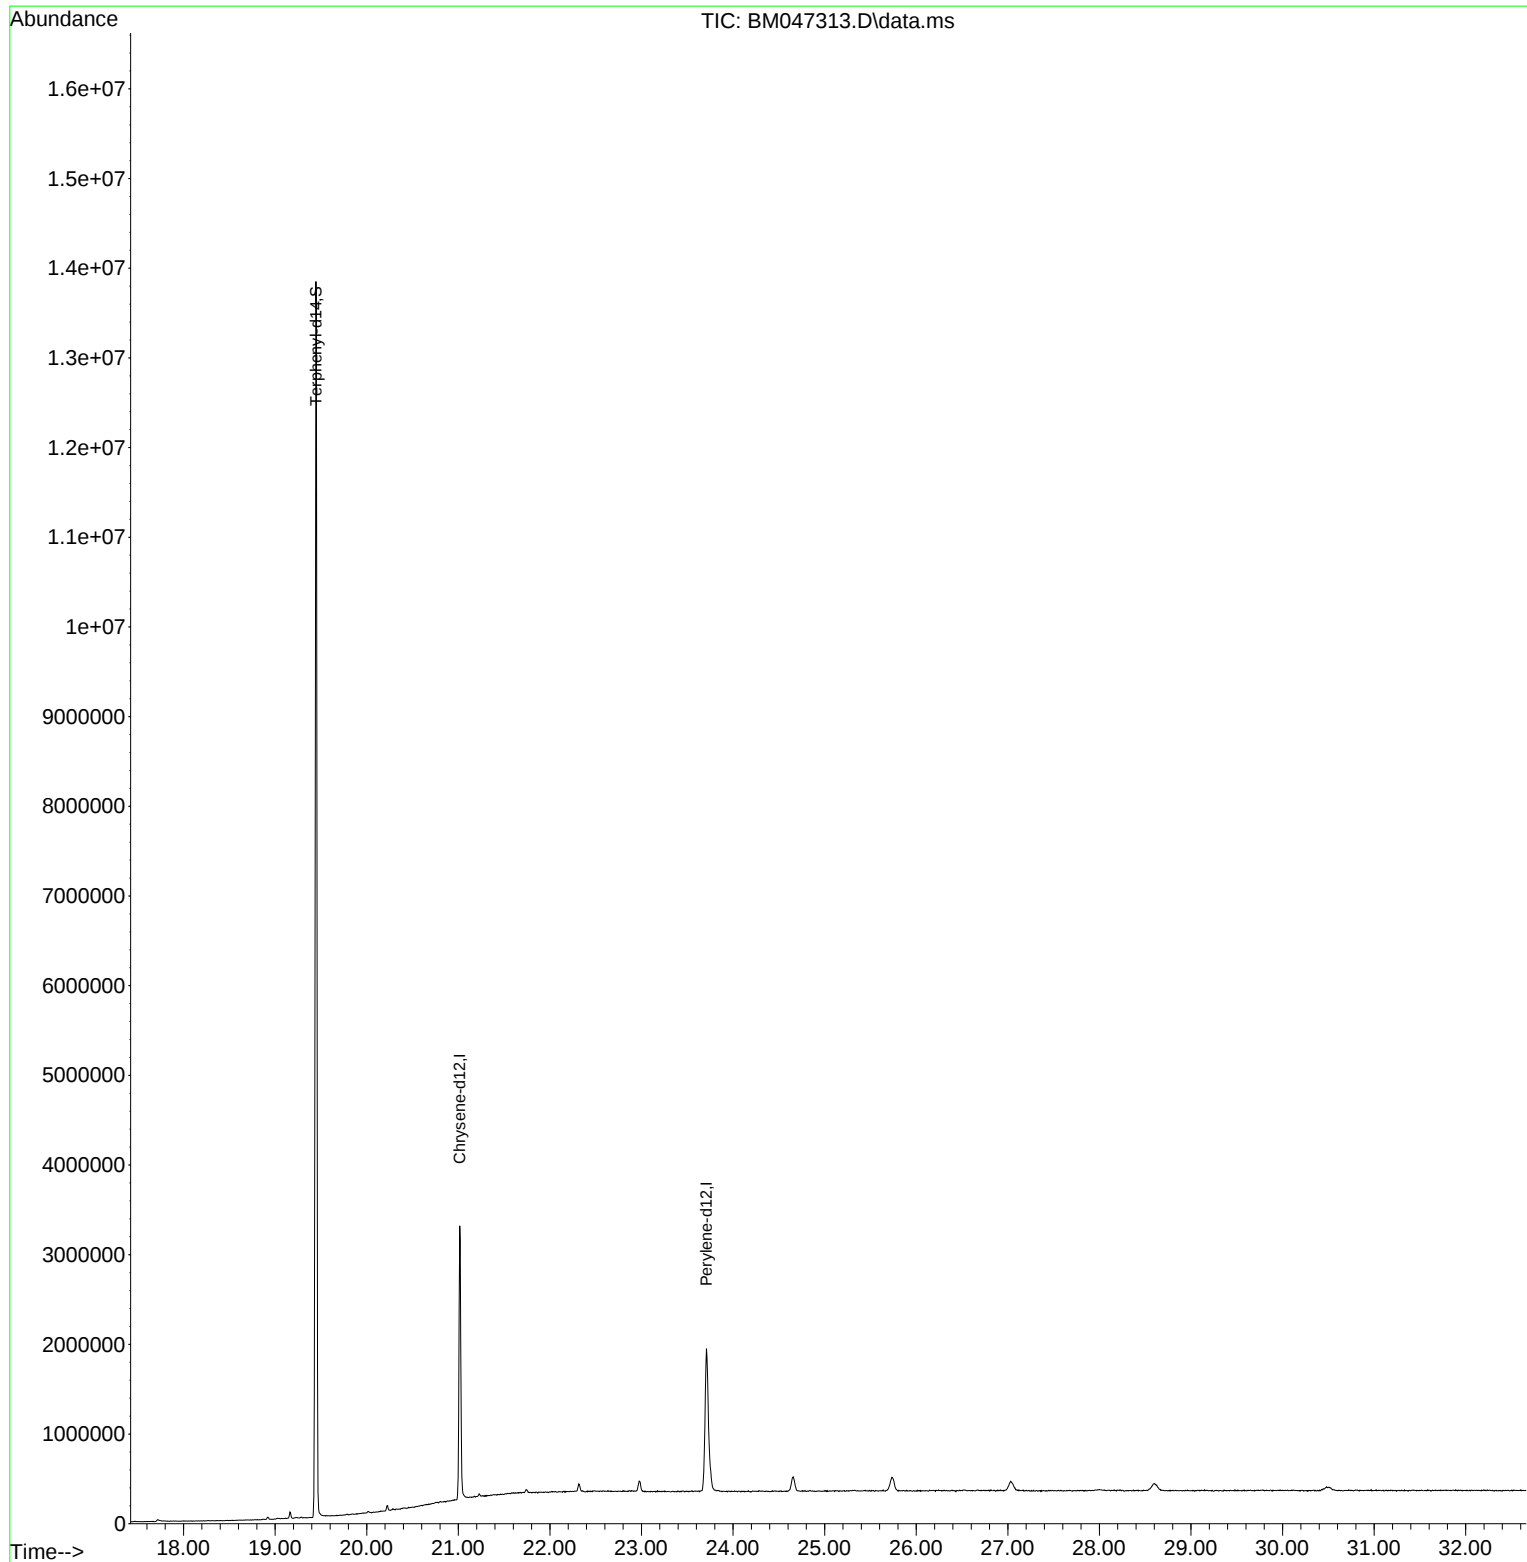

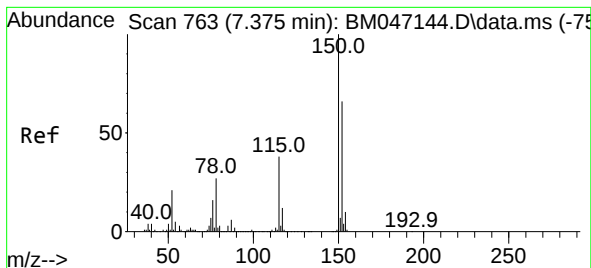

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 7.351 min Scan# 71

Delta R.T. -0.024 min

Lab File: BM047313.D

Acq: 22 Aug 2024 12:32

Instrument :

BNA_M

ClientSampleId :

PB162757BL





Tgt Ion:152 Resp: 292730

Ion Ratio Lower Upper

152 100

150 157.4 120.5 180.7

115 54.1 45.5 68.3

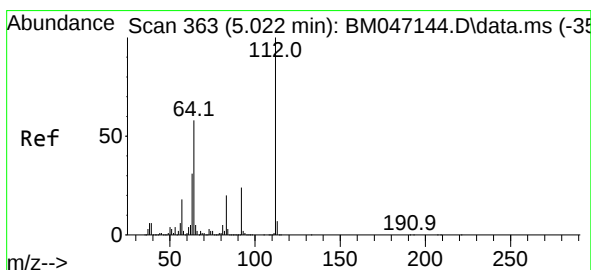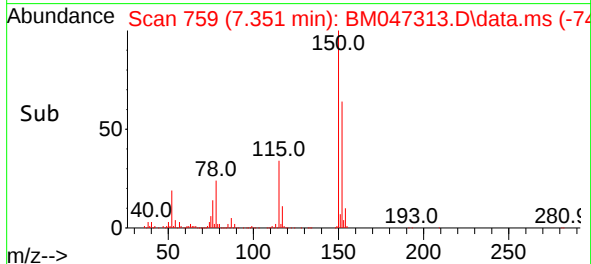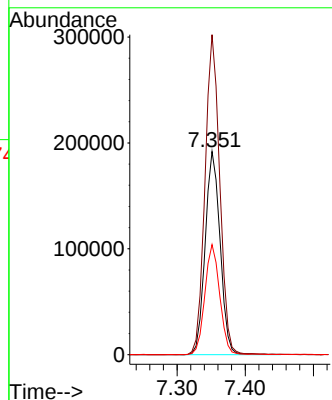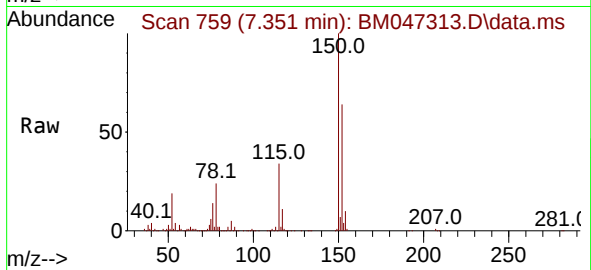

#5

2-Fluorophenol

Concen: 119.790 ng

RT: 5.010 min Scan# 361

Delta R.T. -0.012 min

Lab File: BM047313.D

Acq: 22 Aug 2024 12:32




Tgt Ion:112 Resp: 1962459


Ion Ratio Lower Upper

112 100

64 56.7 46.7 70.1

63 29.8 24.8 37.2


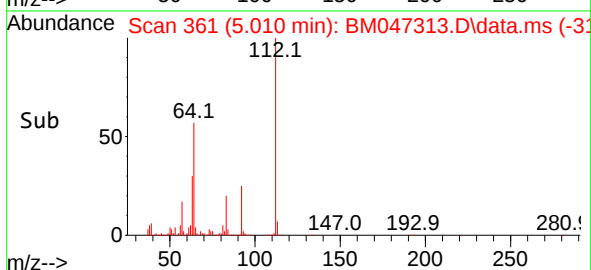
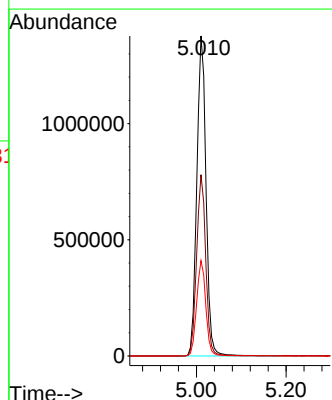
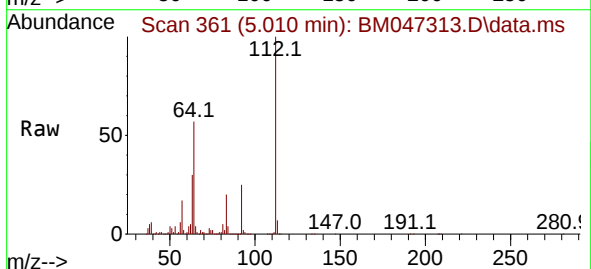


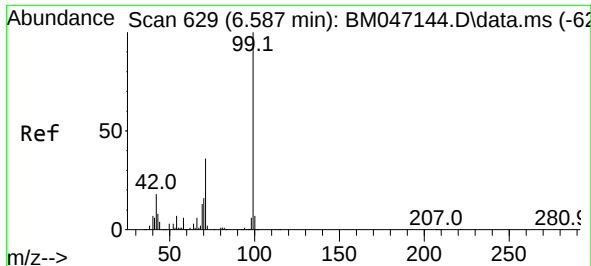

#7
Phenol-d6
Concen: 110.813 ng
RT: 6.569 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM047313.D
Acq: 22 Aug 2024 12:32




Instrument :
BNA_M
ClientSampleId :
PB162757BL

Tgt Ion: 99 Resp: 2501470
Ion Ratio Lower Upper
99 100
42 16.4 14.1 21.1
71 35.2 28.5 42.7

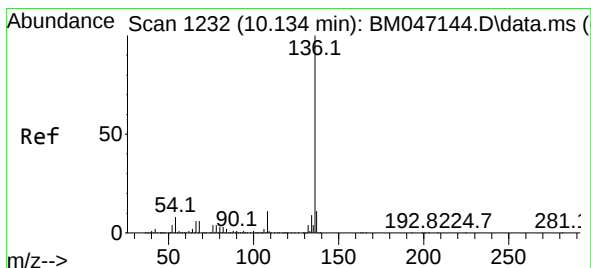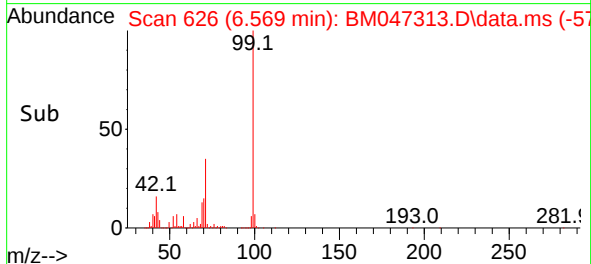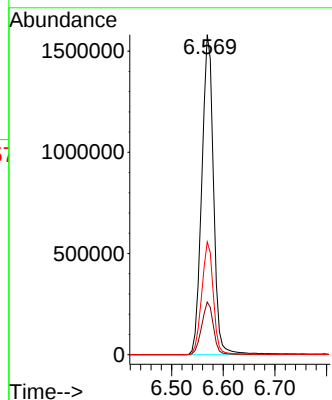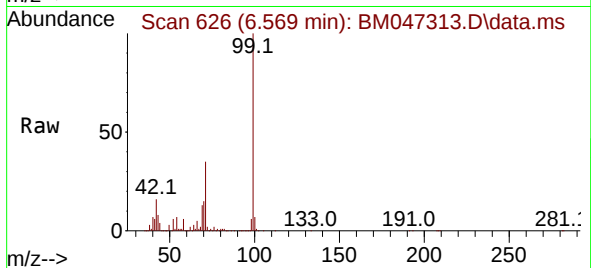

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.104 min Scan# 1227
Delta R.T. -0.030 min
Lab File: BM047313.D
Acq: 22 Aug 2024 12:32

Tgt Ion: 136 Resp: 1111486
Ion Ratio Lower Upper
136 100
137 10.6 8.8 13.2
54 6.9 6.0 9.0
68 5.8 4.8 7.2

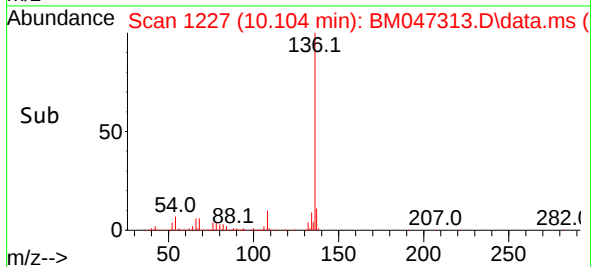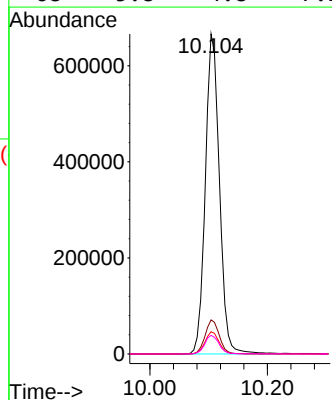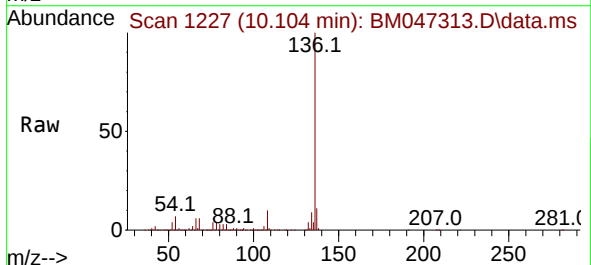



#23

Nitrobenzene-d5

Concen: 75.019 ng

RT: 8.504 min Scan# 91

Delta R.T. -0.018 min

Lab File: BM047313.D

Acq: 22 Aug 2024 12:32

Instrument :





BNA_M

ClientSampleId :

PB162757BL

Tgt Ion: 82 Resp: 1655941

Ion	Ratio	Lower	Upper
82	100		
128	43.4	32.3	48.5
54	43.5	37.4	56.2

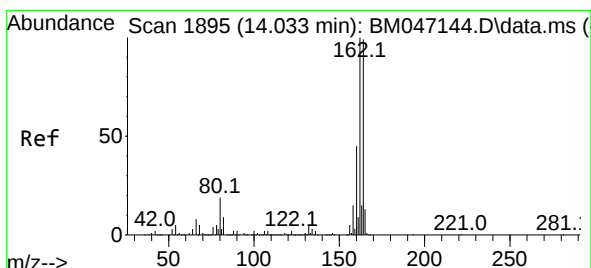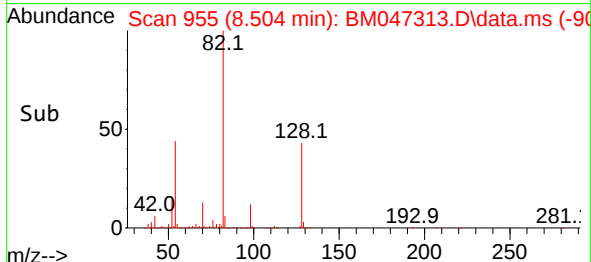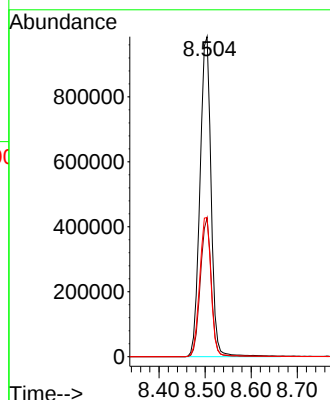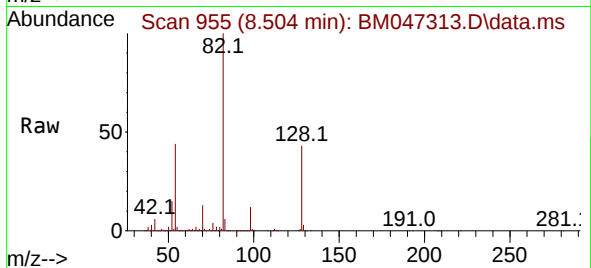

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.010 min Scan# 1891




Delta R.T. -0.024 min

Lab File: BM047313.D

Acq: 22 Aug 2024 12:32

Tgt Ion: 164 Resp: 771992

Ion	Ratio	Lower	Upper
164	100		
162	100.3	80.7	121.1
160	44.8	36.0	54.0

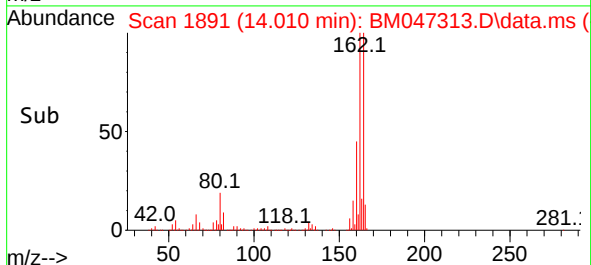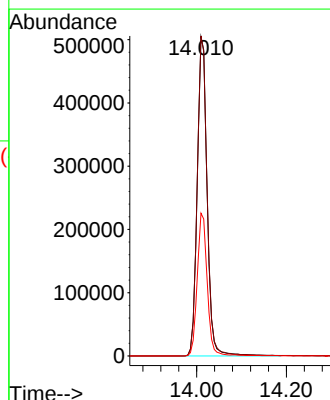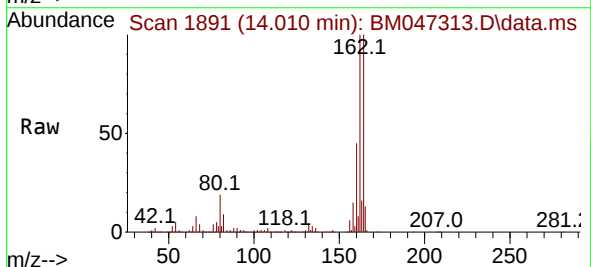







#42
 2,4,6-Tribromophenol
 Concen: 131.253 ng
 RT: 15.527 min Scan# 2151
 Delta R.T. -0.012 min
 Lab File: BM047313.D
 Acq: 22 Aug 2024 12:32

Instrument :
 BNA_M
 ClientSampleId :
 PB162757BL

Tgt Ion:330 Resp: 1174894




Ion	Ratio	Lower	Upper
330	100		
332	95.8	77.4	116.2
141	35.7	31.6	47.4

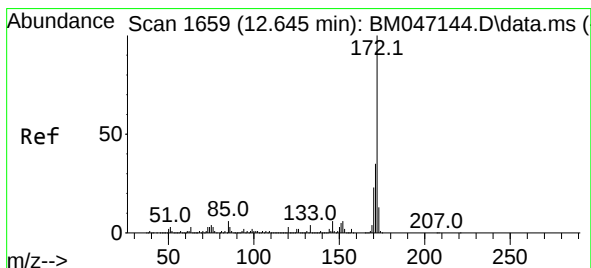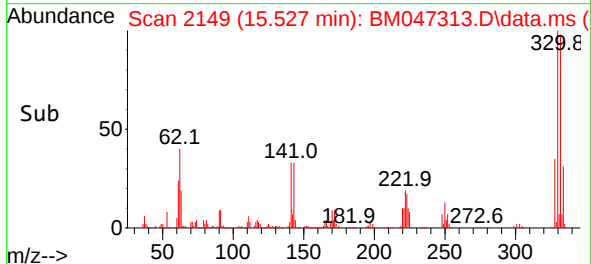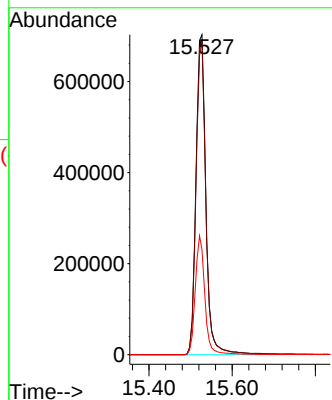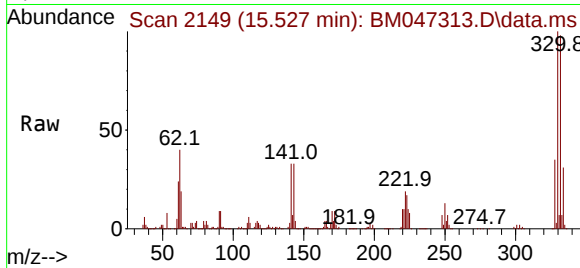


#45
 2-Fluorobiphenyl
 Concen: 79.099 ng
 RT: 12.621 min Scan# 1655
 Delta R.T. -0.024 min
 Lab File: BM047313.D
 Acq: 22 Aug 2024 12:32

Tgt Ion:172 Resp: 3958679

Ion	Ratio	Lower	Upper
172	100		
171	34.9	27.8	41.6
170	23.3	18.7	28.1


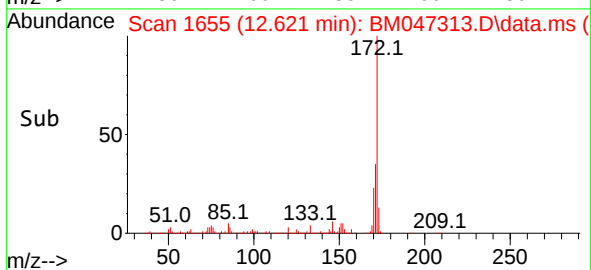
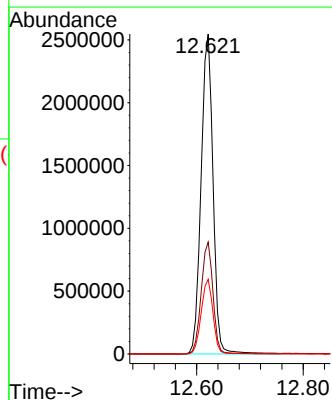
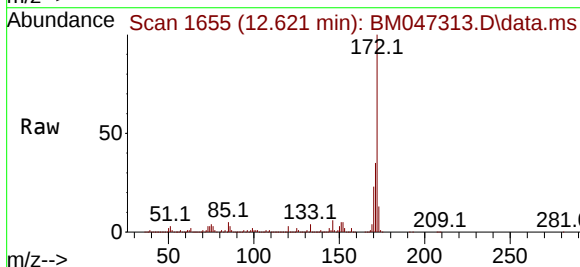


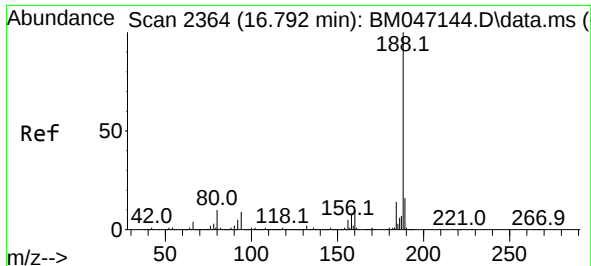

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.774 min Scan# 21
Delta R.T. -0.018 min
Lab File: BM047313.D
Acq: 22 Aug 2024 12:32




Instrument :
BNA_M
ClientSampleId :
PB162757BL


Tgt Ion:188 Resp: 1724658
Ion Ratio Lower Upper
188 100
94 8.4 7.0 10.6
80 9.4 8.0 12.0

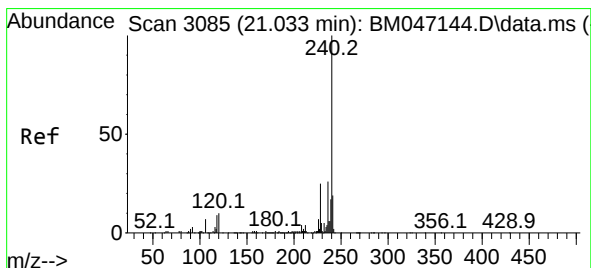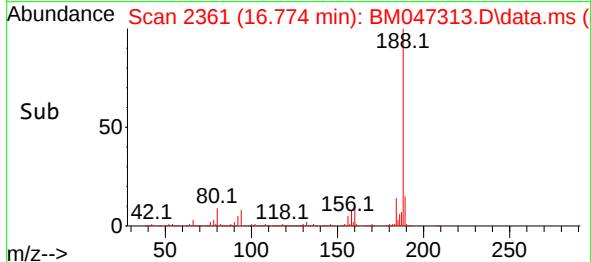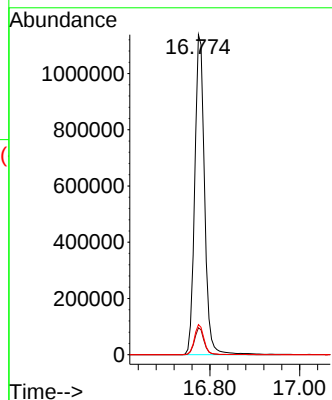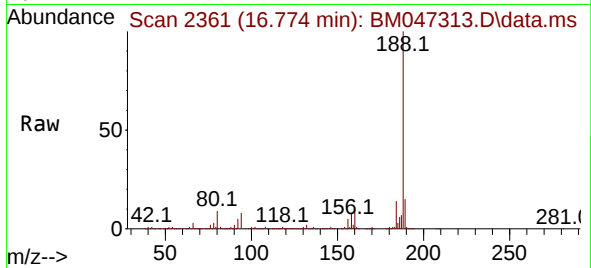

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.015 min Scan# 3082
Delta R.T. -0.018 min
Lab File: BM047313.D
Acq: 22 Aug 2024 12:32

Tgt Ion:240 Resp: 1583438
Ion Ratio Lower Upper
240 100
120 9.9 8.2 12.2
236 25.5 20.6 30.8


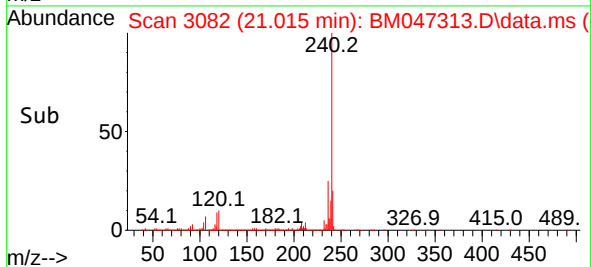
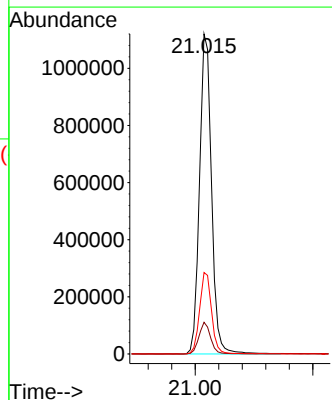
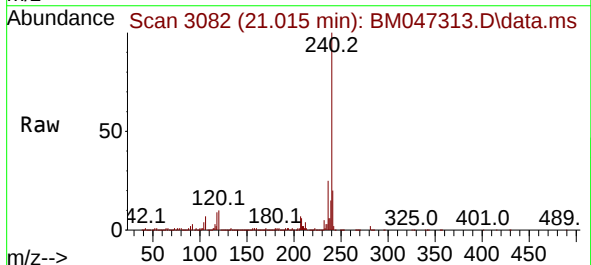


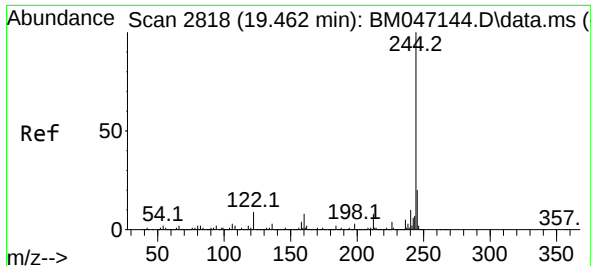

#79
 Terphenyl-d14
 Concen: 96.357 ng
 RT: 19.445 min Scan# 21
 Delta R.T. -0.018 min
 Lab File: BM047313.D
 Acq: 22 Aug 2024 12:32

Instrument :
 BNA_M
 ClientSampleId :
 PB162757BL

Tgt Ion:244 Resp: 7120475
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.4
 122 8.7 7.1 10.7

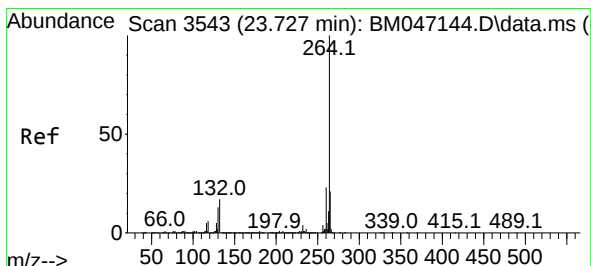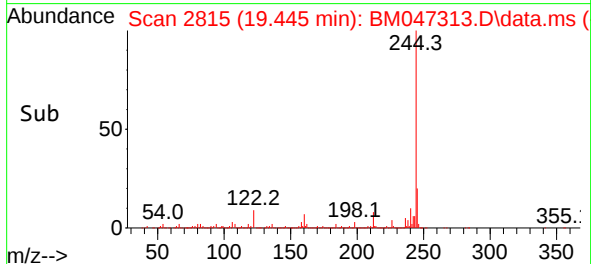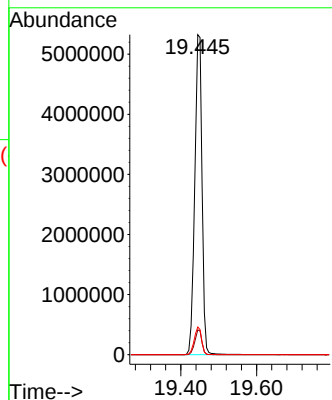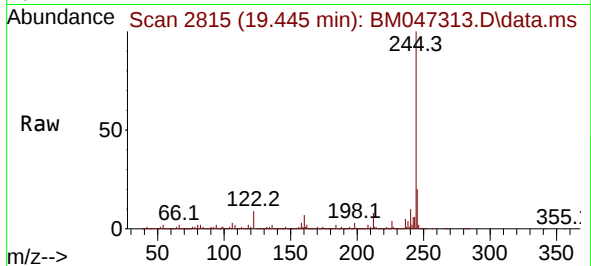

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.709 min Scan# 3540
 Delta R.T. -0.018 min
 Lab File: BM047313.D
 Acq: 22 Aug 2024 12:32

Tgt Ion:264 Resp: 1534865
 Ion Ratio Lower Upper
 264 100
 260 23.0 18.5 27.7
 265 22.0 17.3 25.9

