
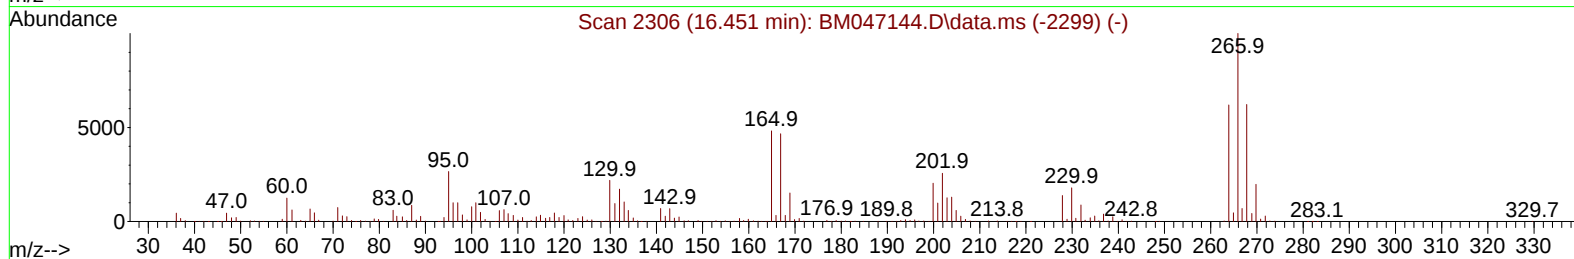
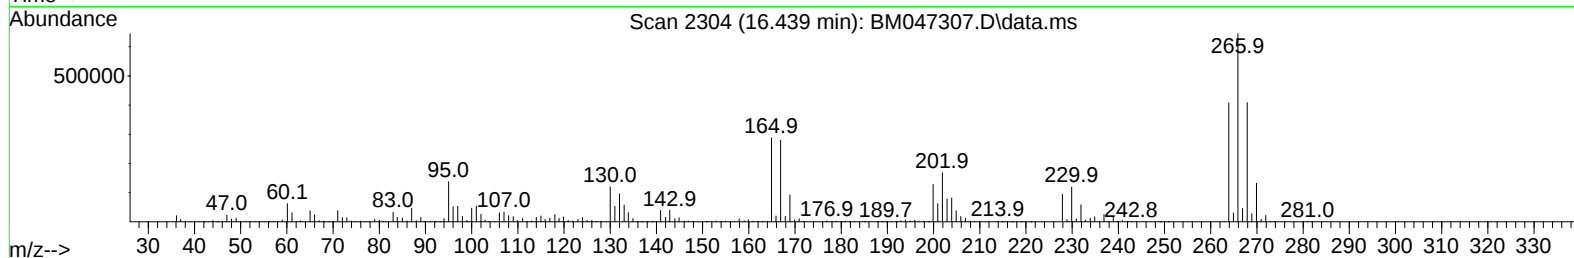


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047307.D
Acq On : 22 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

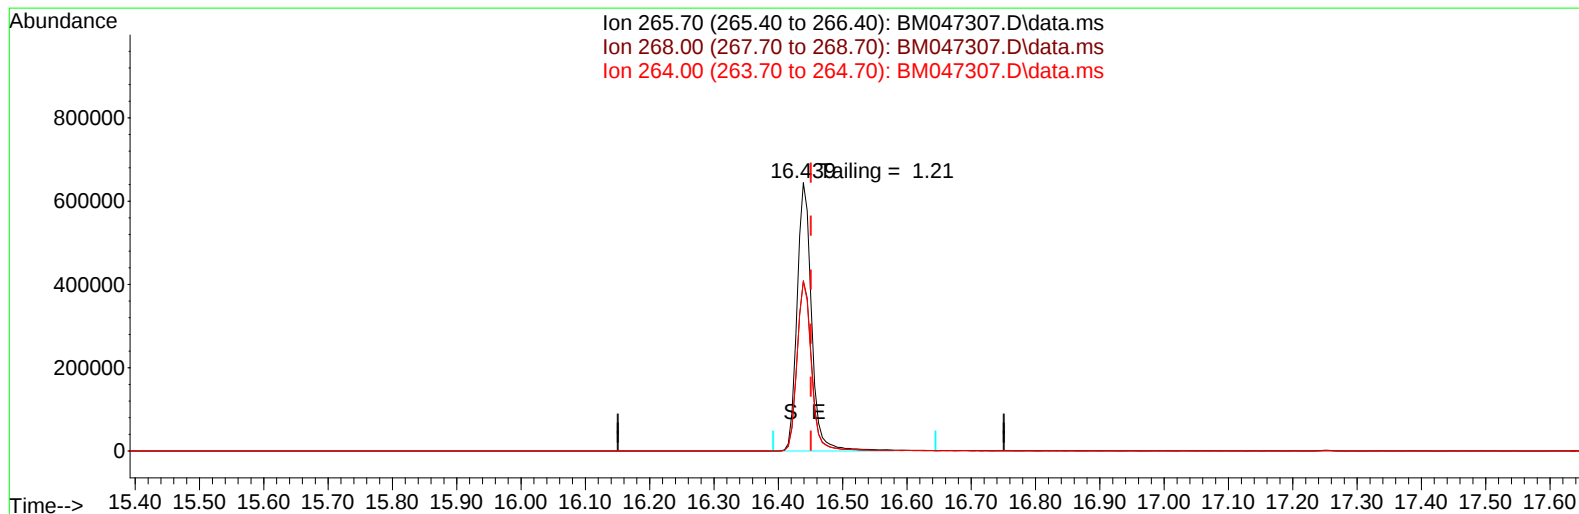

TIC: BM047307.D\data.ms

(70) Pentachlorophenol (C)




16.439min (-0.012) 305697.00 ng

response 1016426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.44
264.00	62.00	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082224\
Data File : BM047307.D
Acq On : 22 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:58:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

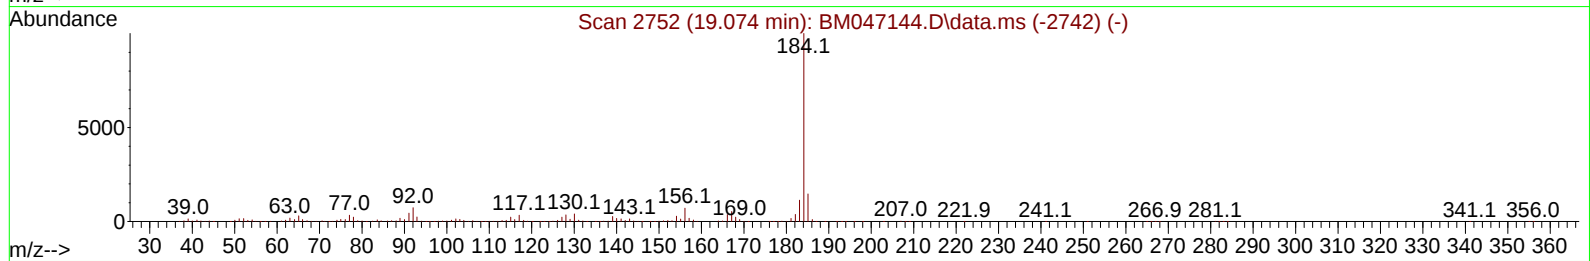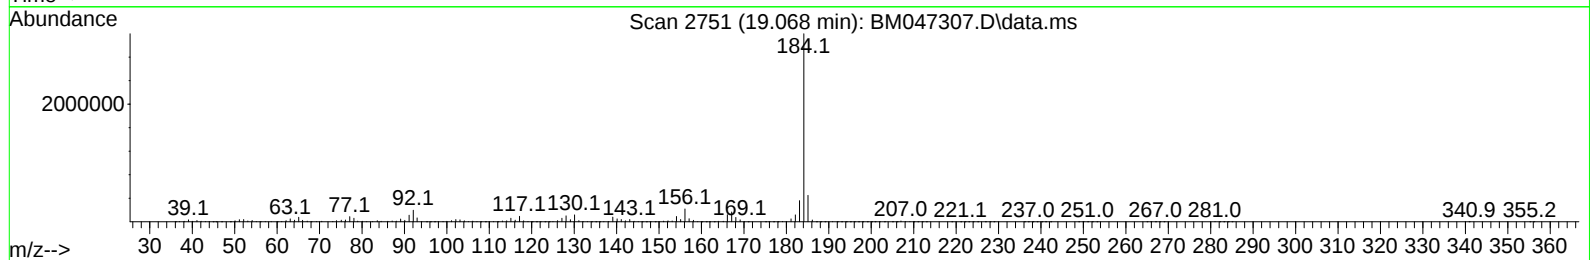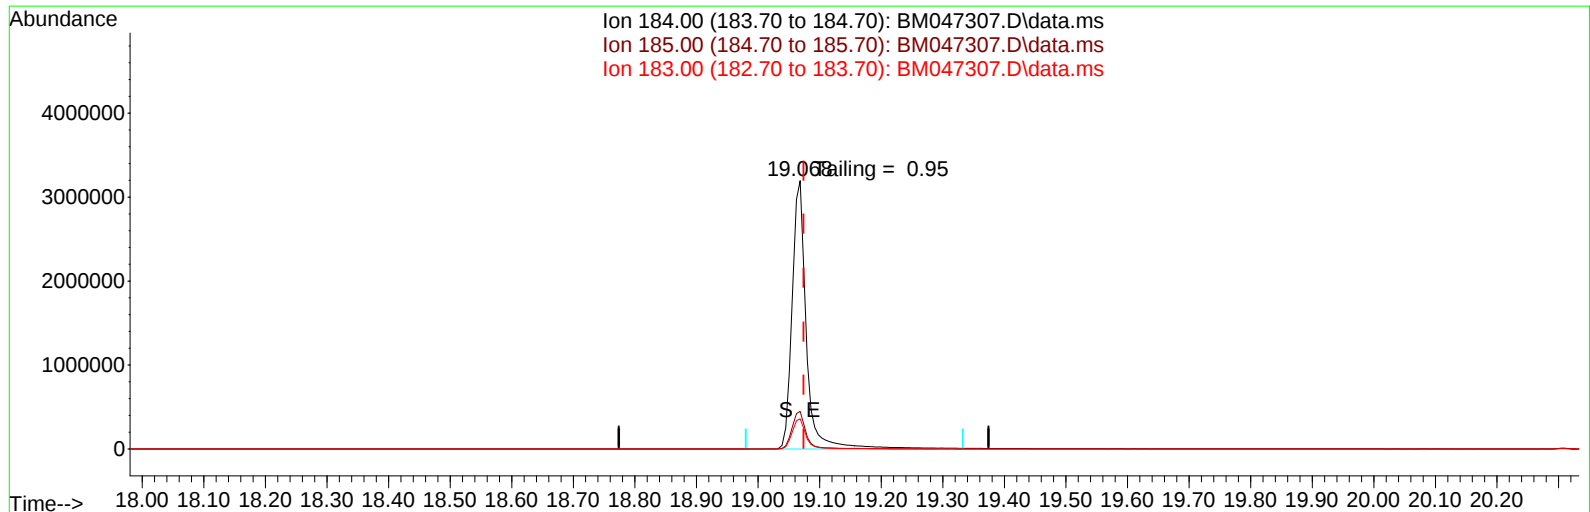

TIC: BM047307.D\data.ms

(77) Benzidine

19.068min (-0.006) 142115.28 ng

response 5191261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.05
183.00	11.30	11.27
0.00	0.00	0.00