
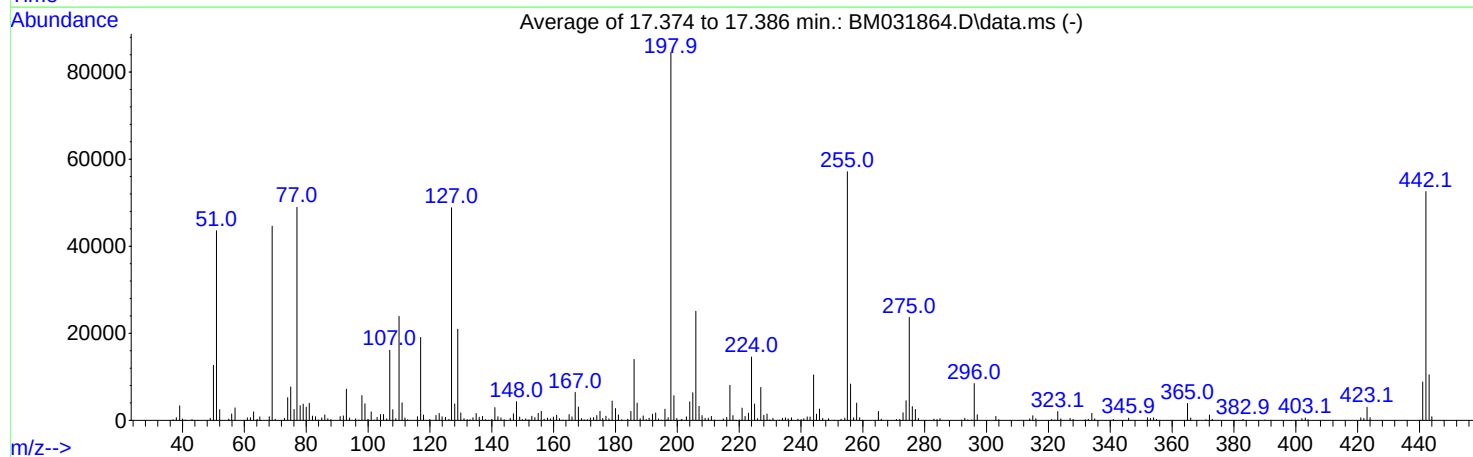


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082321\
 Data File : BM031864.D
 Acq On : 23 Aug 2021 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 16:34:26 2021

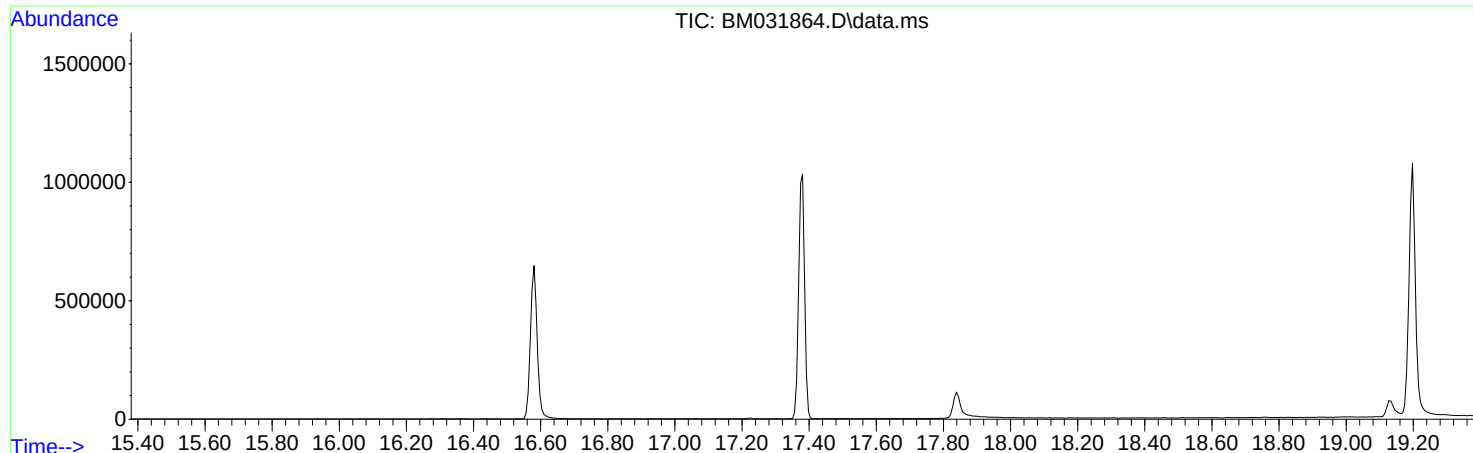




AutoFind: Scans 2429, 2430, 2431; Background Corrected with Scan 2422

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	43568	PASS
68	69	0.00	2	1.9	854	PASS
69	198	0.00	100	52.8	44621	PASS
70	69	0.00	2	0.6	253	PASS
127	198	10	80	57.8	48832	PASS
197	198	0.00	2	0.7	625	PASS
198	198	100	100	100.0	84504	PASS
199	198	5	9	6.7	5668	PASS
275	198	10	60	28.0	23667	PASS
365	198	1	100	4.6	3890	PASS
441	198	0.01	100	10.4	8817	PASS
442	442	50	100	100.0	52549	PASS
443	442	15	24	19.9	10473	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082321\
Data File : BM031864.D
Acq On : 23 Aug 2021 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 23 17:28:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 15:51:36 2021
Response via : Initial Calibration

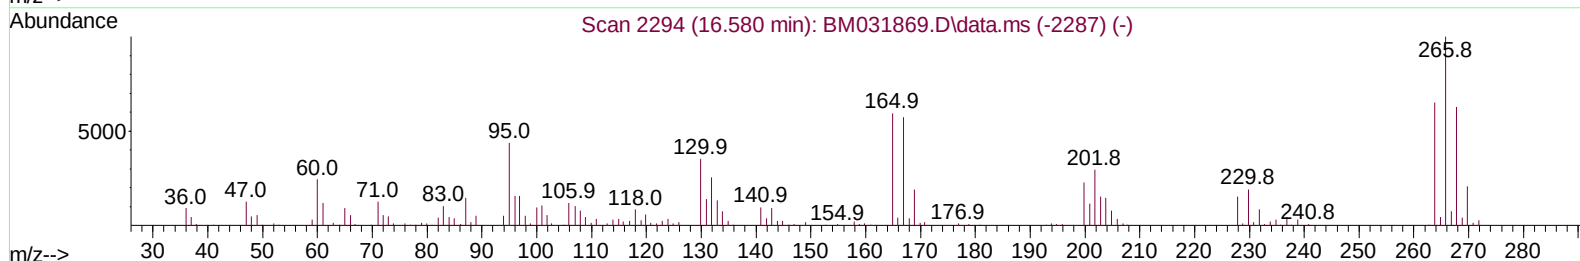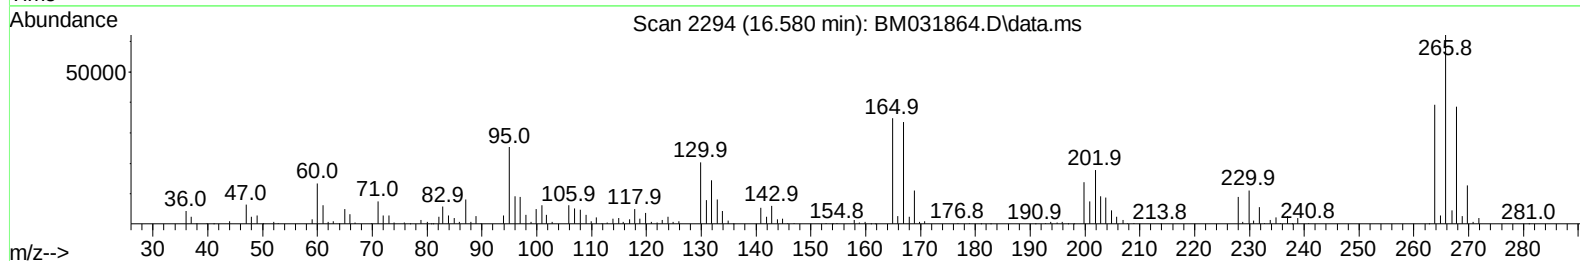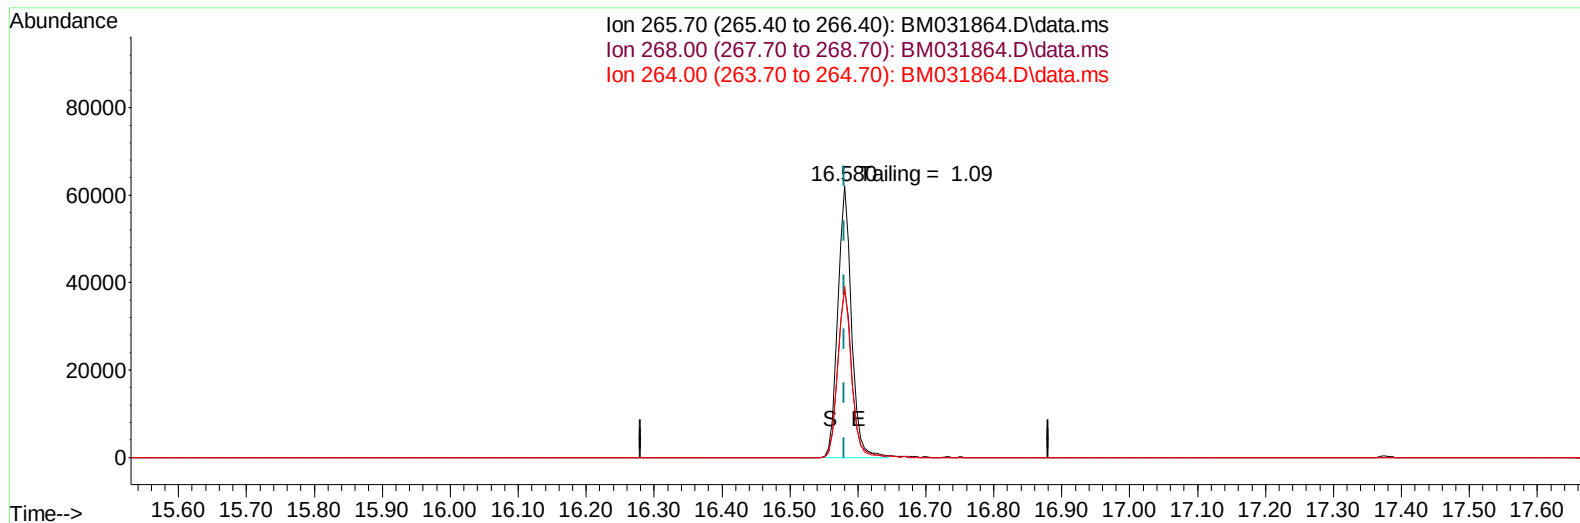

TIC: BM031864.D\data.ms

(70) Pentachlorophenol (C)

16.580min (+ 0.000) 0.00 ng




response 87307

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.12
264.00	65.10	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082321\
Data File : BM031864.D
Acq On : 23 Aug 2021 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 23 17:28:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 15:51:36 2021
Response via : Initial Calibration

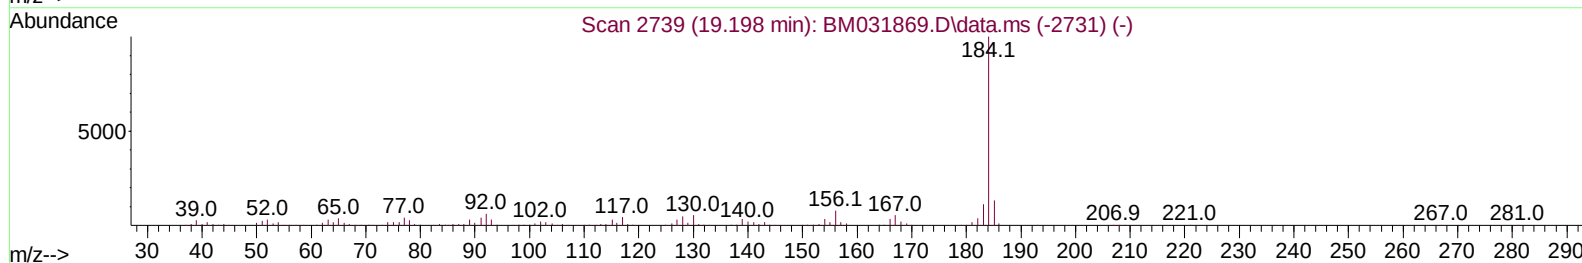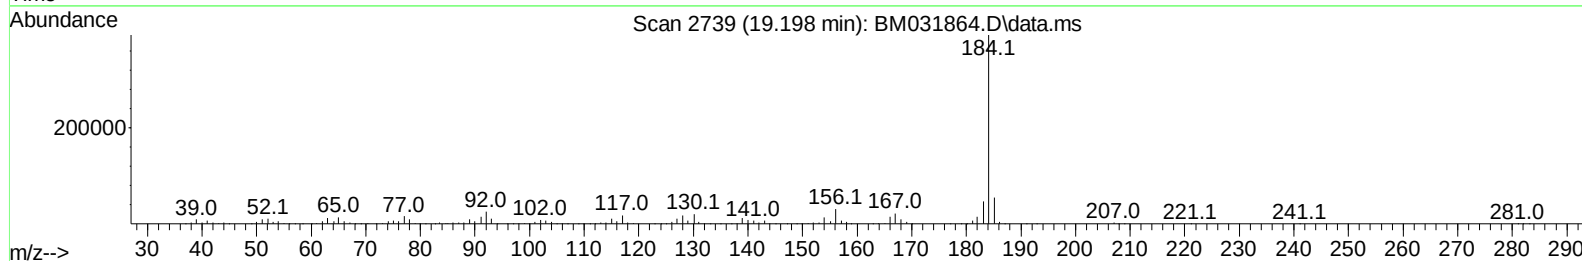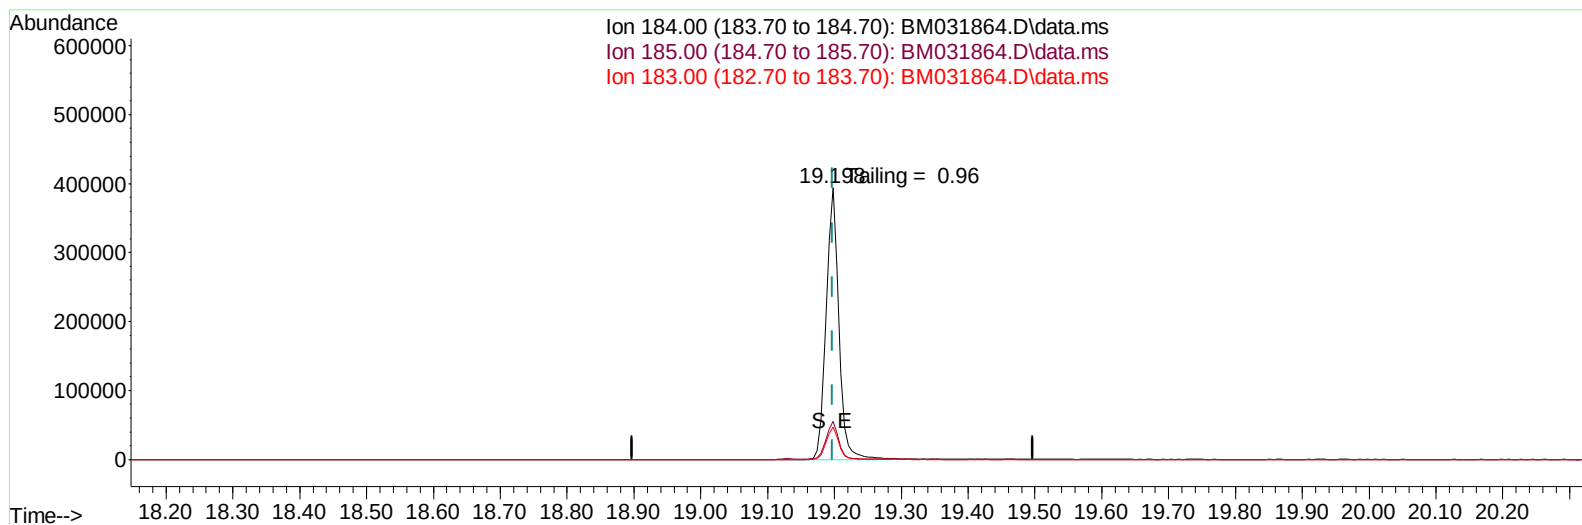

TIC: BM031864.D\data.ms

(77) Benzidine

19.198min (+ 0.000) 0.00 ng

response 518941

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.03
183.00	11.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2021	BNA_M	<u>BM031864.D</u>
Compound Name	Response	Retention Time
DDT	296584	20.42
DDD	2017	19.99
DDE	421	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2438	299022	0.82

Instrument :
BNA_M
ClientSampleId :
DFTPP