

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047327.D
Acq On : 23 Aug 2024 10:48
Operator : RC/JU
Sample : PB162815BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162815BL

Quant Time: Aug 23 11:56:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.351	152	315846	20.000	ng	-0.02
21) Naphthalene-d8	10.104	136	1133981	20.000	ng	-0.03
39) Acenaphthene-d10	14.010	164	773133	20.000	ng	-0.02
64) Phenanthrene-d10	16.774	188	1691306	20.000	ng	-0.02
76) Chrysene-d12	21.015	240	1674916	20.000	ng	-0.02
86) Perylene-d12	23.709	264	1753650	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.010	112	2071201	117.174	ng	-0.01
7) Phenol-d6	6.569	99	2586743	106.204	ng	-0.02
23) Nitrobenzene-d5	8.498	82	1689132	75.004	ng	-0.02
42) 2,4,6-Tribromophenol	15.521	330	1194073	133.199	ng	-0.02
45) 2-Fluorobiphenyl	12.622	172	3985751	79.522	ng	-0.02
79) Terphenyl-d14	19.445	244	7246274	92.704	ng	-0.02


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047327.D
Acq On : 23 Aug 2024 10:48
Operator : RC/JU
Sample : PB162815BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162815BL


Quant Time: Aug 23 11:56:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

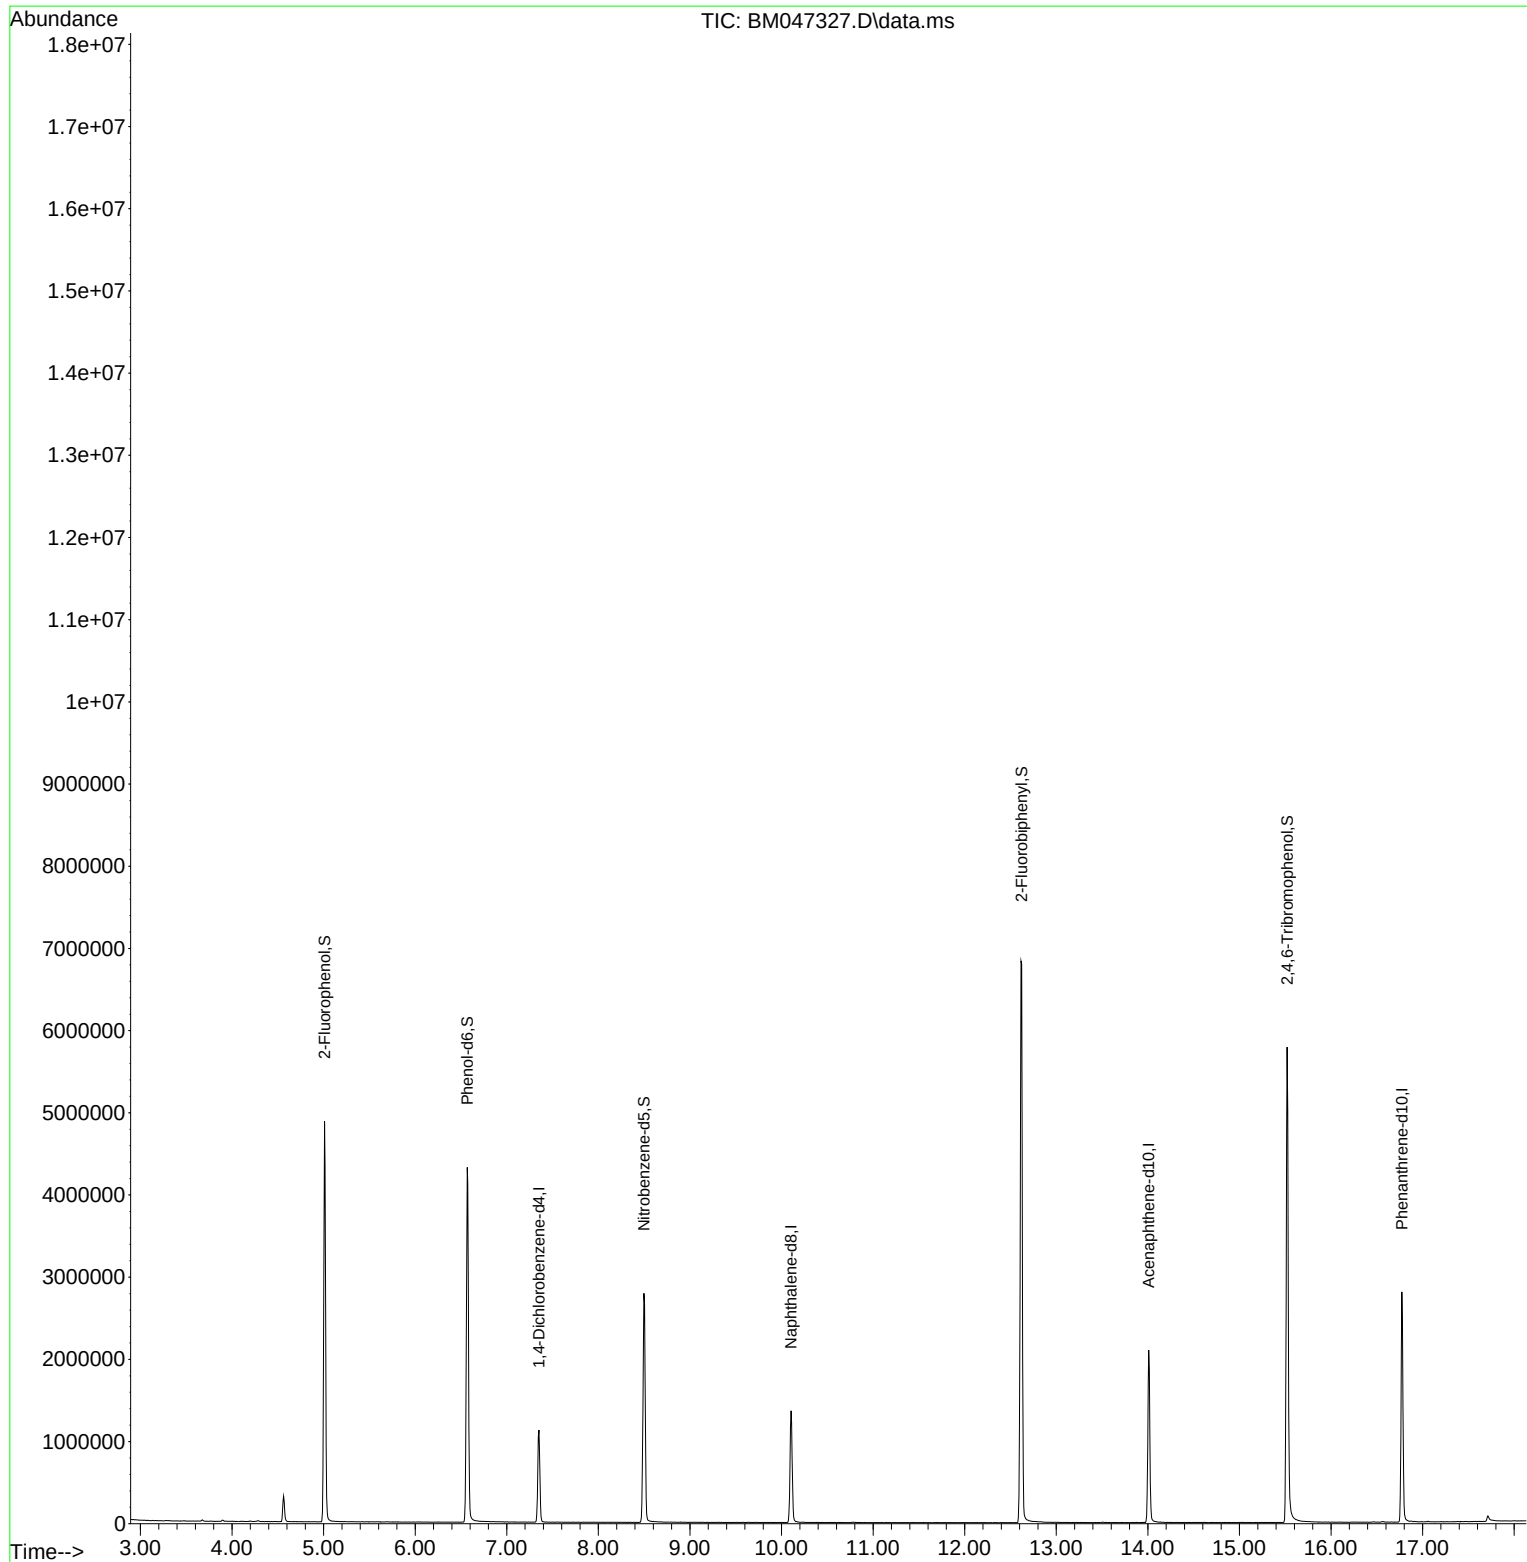


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047327.D
Acq On : 23 Aug 2024 10:48
Operator : RC/JU
Sample : PB162815BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162815BL

Quant Time: Aug 23 11:56:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration




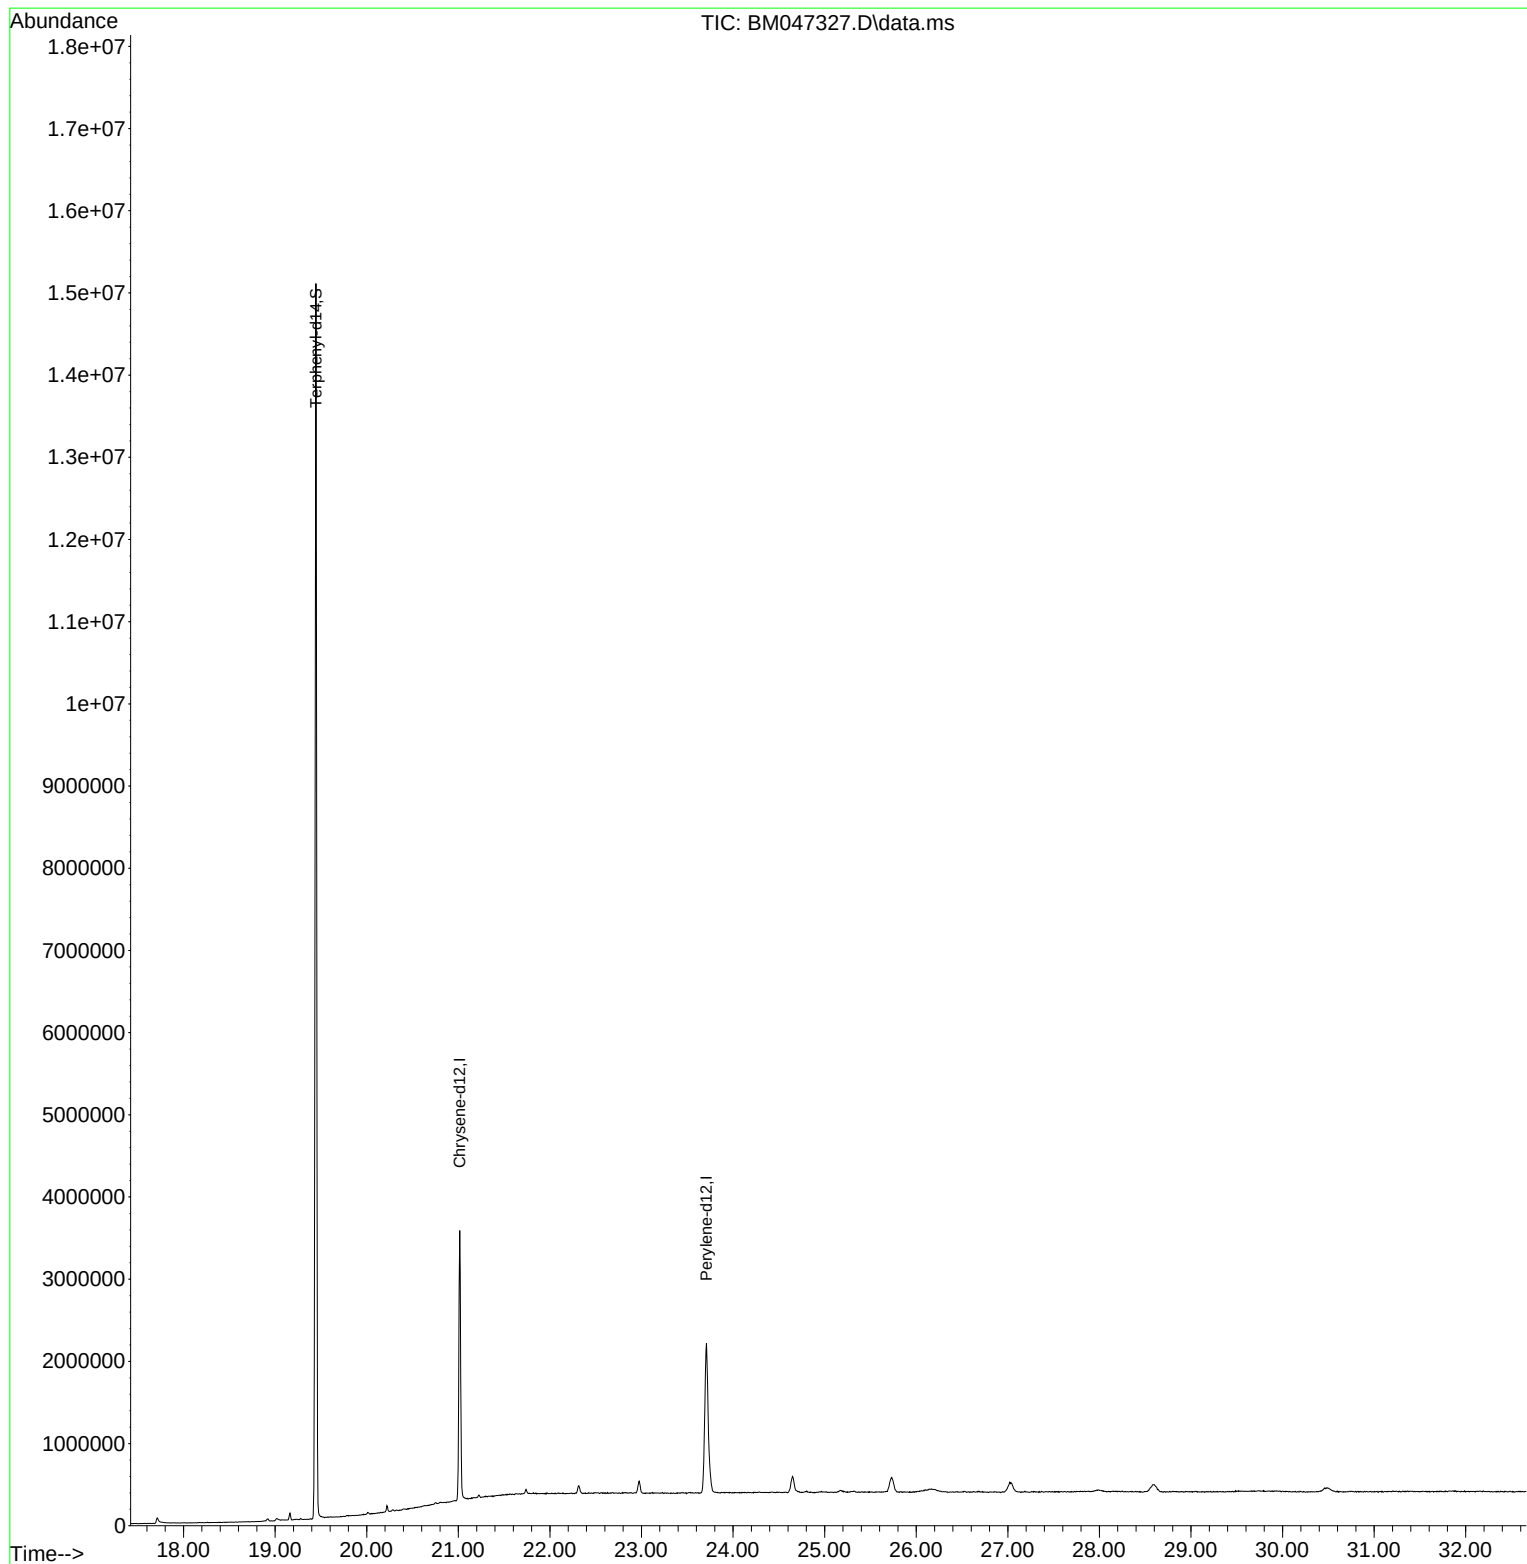


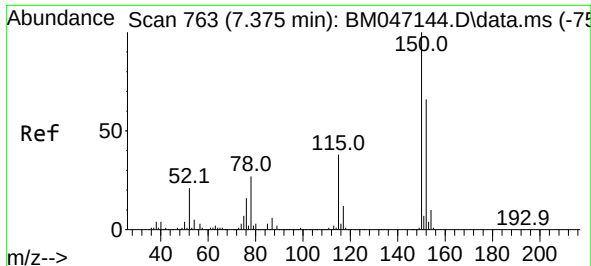

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.351 min Scan# 71
Delta R.T. -0.024 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48




Instrument :
BNA_M
ClientSampleId :
PB162815BL


Tgt Ion:152 Resp: 315846
Ion Ratio Lower Upper
152 100
150 157.0 120.5 180.7
115 54.3 45.5 68.3

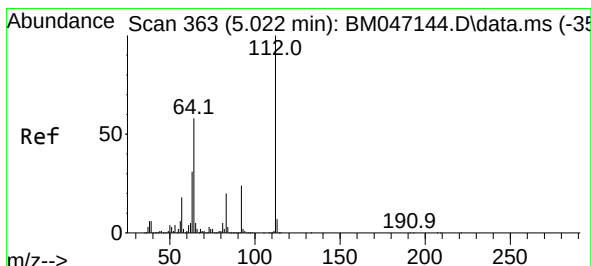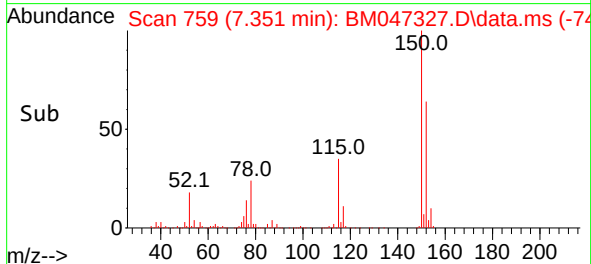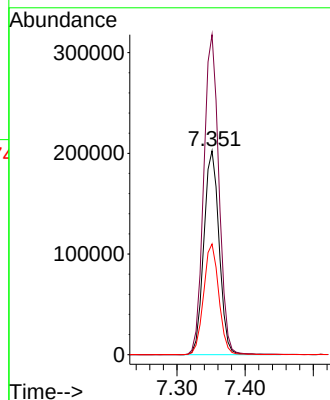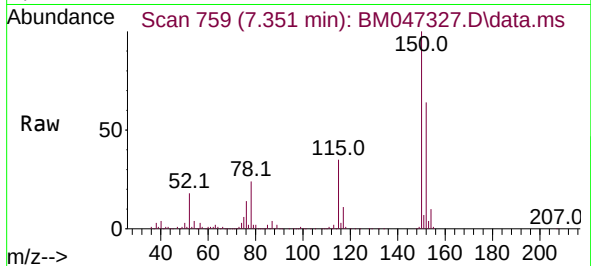

#5
2-Fluorophenol
Concen: 117.174 ng
RT: 5.010 min Scan# 361
Delta R.T. -0.012 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Tgt Ion:112 Resp: 2071201
Ion Ratio Lower Upper
112 100
64 55.5 46.7 70.1
63 29.5 24.8 37.2


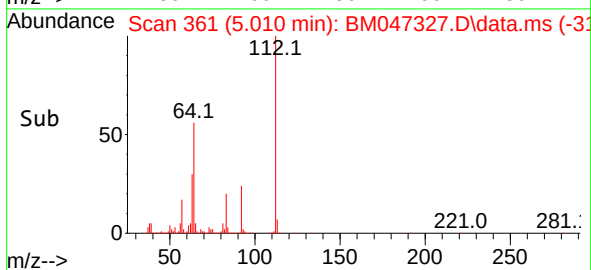
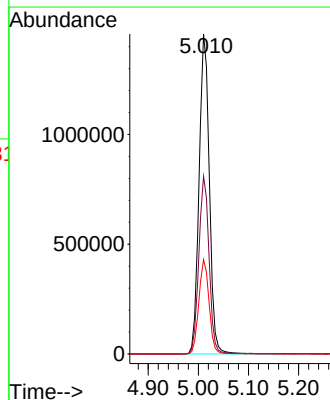
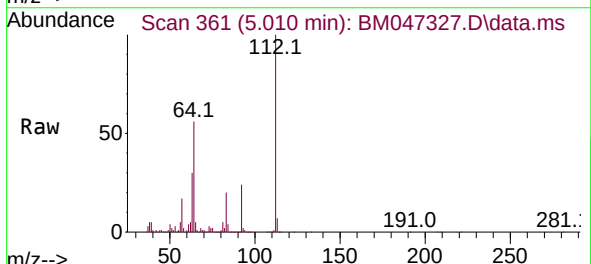


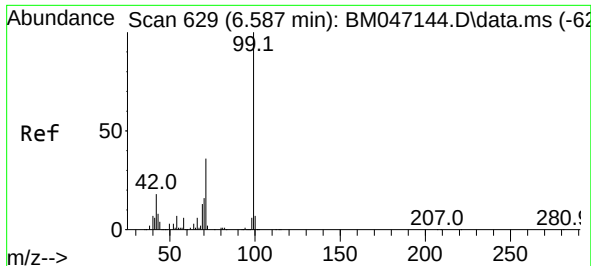

#7
Phenol-d6
Concen: 106.204 ng
RT: 6.569 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48




Instrument :
BNA_M
ClientSampleId :
PB162815BL


Tgt Ion: 99 Resp: 2586743
Ion Ratio Lower Upper
99 100
42 16.3 14.1 21.1
71 35.2 28.5 42.7

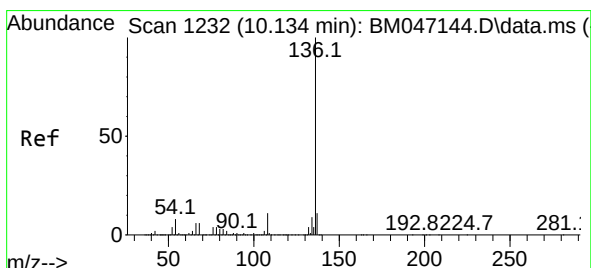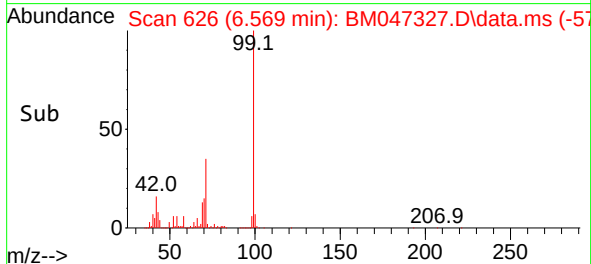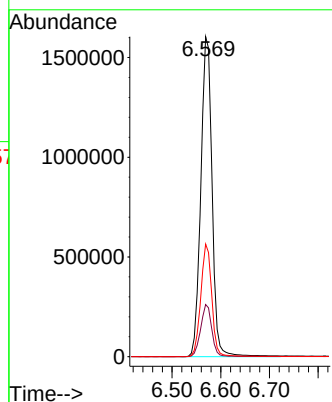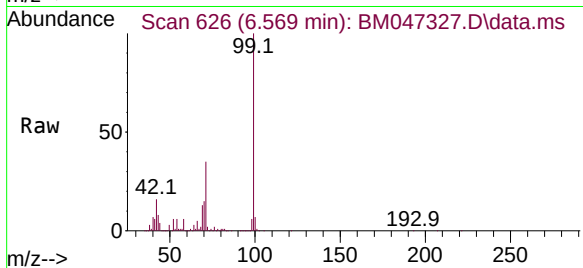

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.104 min Scan# 1227
Delta R.T. -0.030 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Tgt Ion: 136 Resp: 1133981
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 7.0 6.0 9.0
68 5.7 4.8 7.2


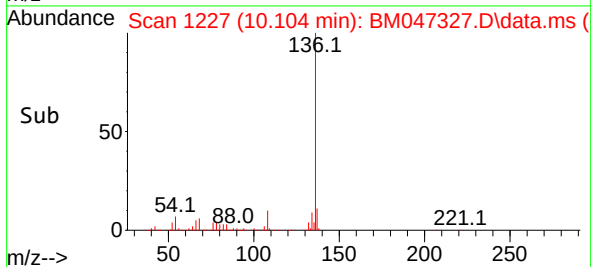
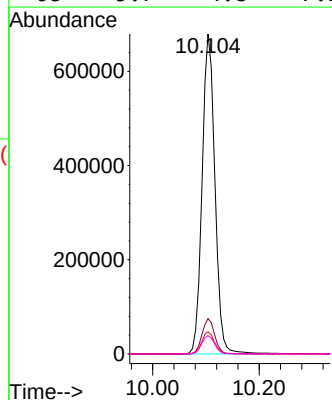
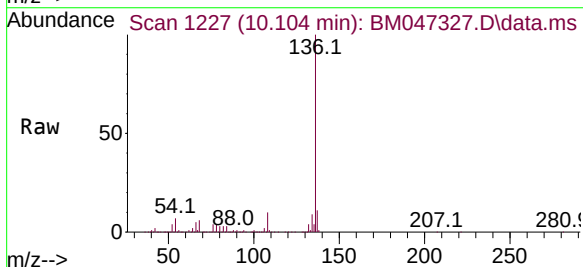


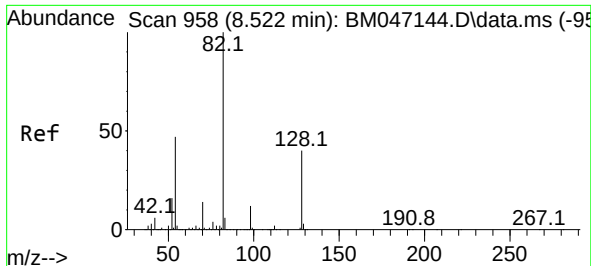

#23
 Nitrobenzene-d5
 Concen: 75.004 ng
 RT: 8.498 min Scan# 91
 Delta R.T. -0.024 min
 Lab File: BM047327.D
 Acq: 23 Aug 2024 10:48




Instrument :
 BNA_M
 ClientSampleId :
 PB162815BL


Tgt Ion: 82 Resp: 1689132
 Ion Ratio Lower Upper
 82 100
 128 42.9 32.3 48.5
 54 45.1 37.4 56.2

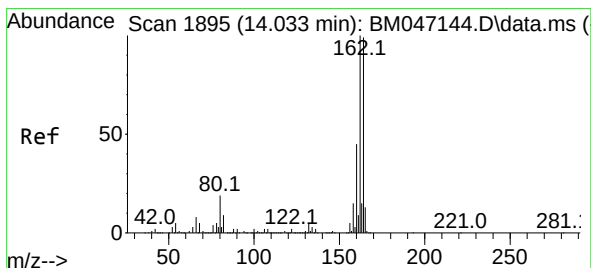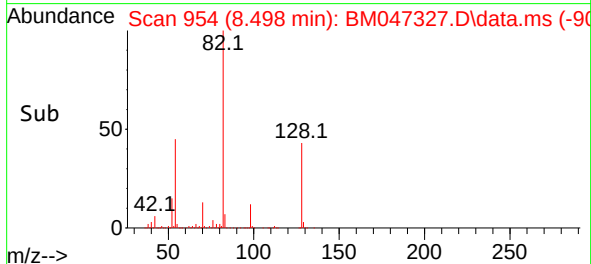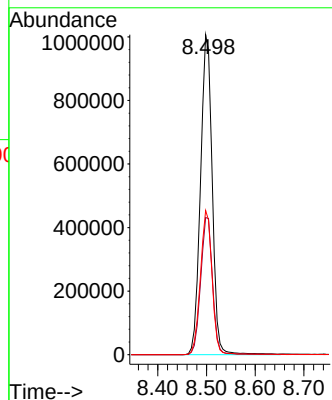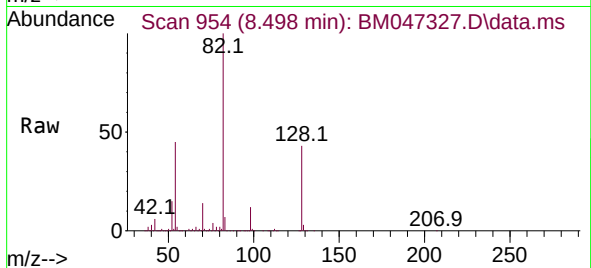

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.010 min Scan# 1891
 Delta R.T. -0.024 min
 Lab File: BM047327.D
 Acq: 23 Aug 2024 10:48

Tgt Ion: 164 Resp: 773133
 Ion Ratio Lower Upper
 164 100
 162 98.3 80.7 121.1
 160 44.0 36.0 54.0


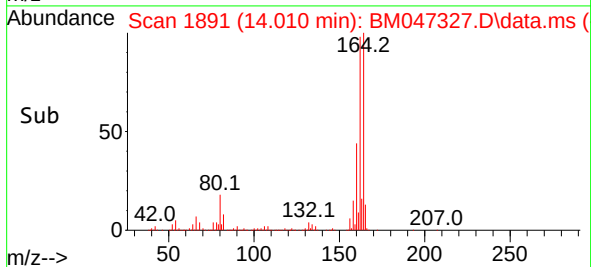
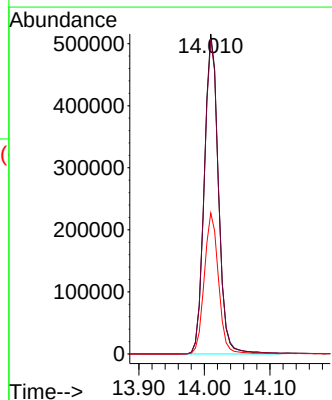
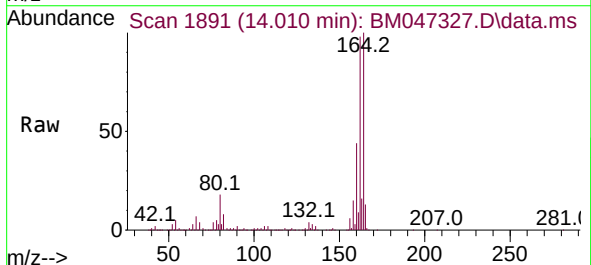


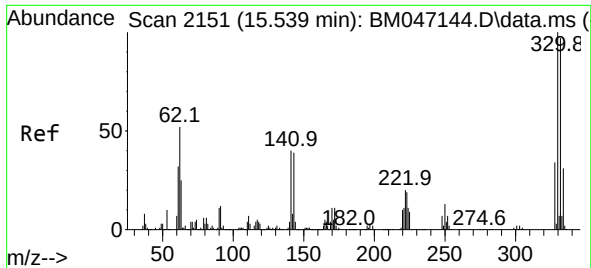

#42
2,4,6-Tribromophenol
Concen: 133.199 ng
RT: 15.521 min Scan# 2151
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48




Instrument :
BNA_M
ClientSampleId :
PB162815BL


Tgt Ion:330 Resp: 1194073
Ion Ratio Lower Upper
330 100
332 96.9 77.4 116.2
141 33.8 31.6 47.4

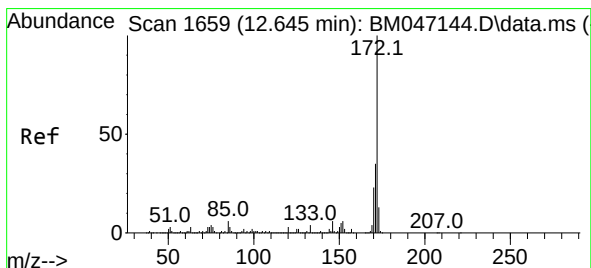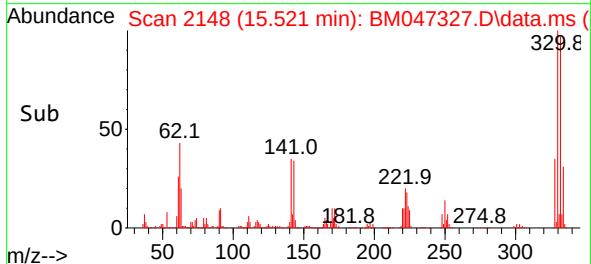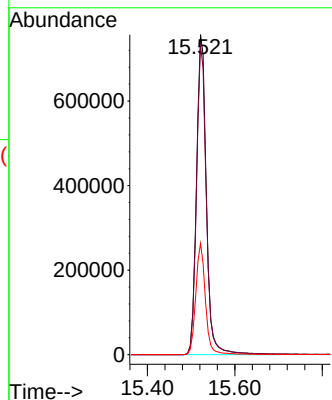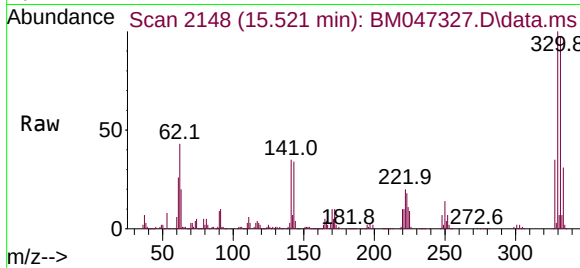

#45
2-Fluorobiphenyl
Concen: 79.522 ng
RT: 12.622 min Scan# 1655
Delta R.T. -0.023 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Tgt Ion:172 Resp: 3985751
Ion Ratio Lower Upper
172 100
171 34.6 27.8 41.6
170 23.3 18.7 28.1


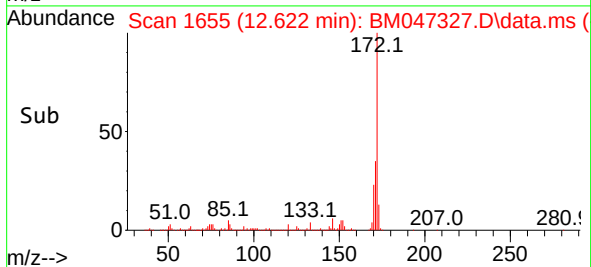
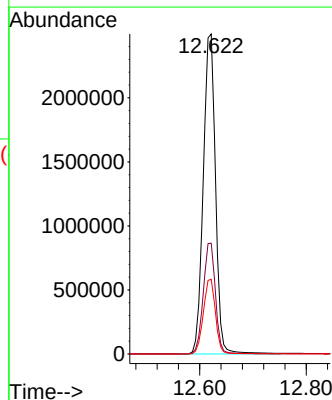
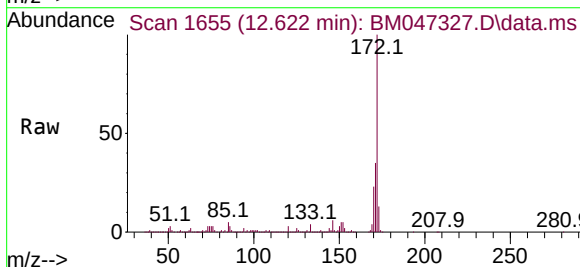


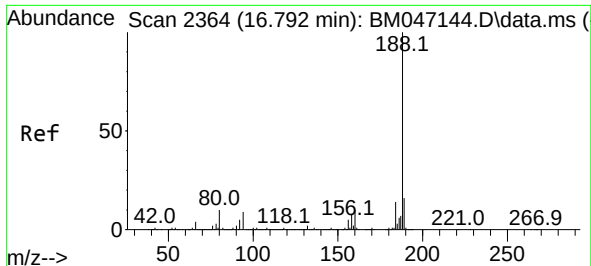

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.774 min Scan# 21
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48




Instrument :
BNA_M
ClientSampleId :
PB162815BL


Tgt Ion:188 Resp: 1691306
Ion Ratio Lower Upper
188 100
94 8.1 7.0 10.6
80 9.2 8.0 12.0

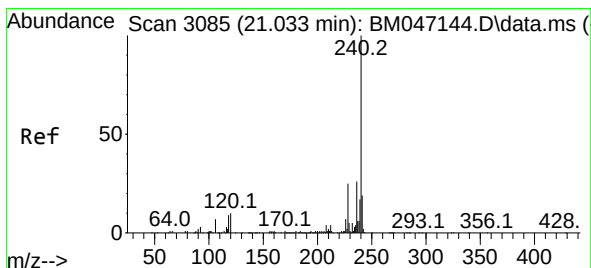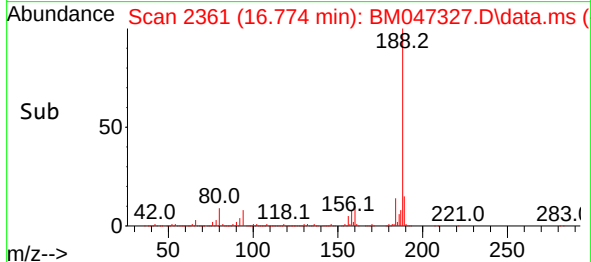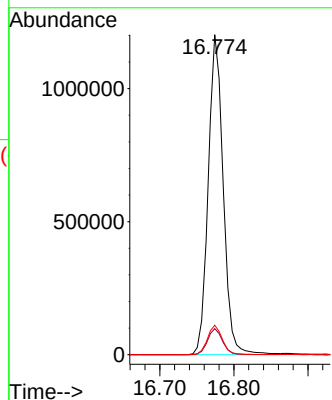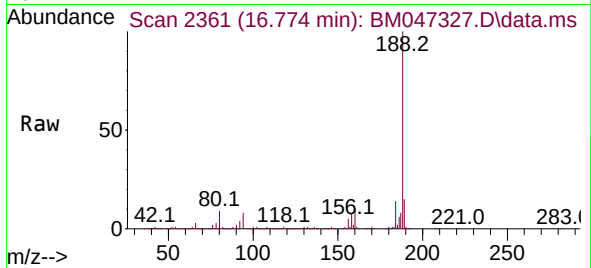

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.015 min Scan# 3082
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Tgt Ion:240 Resp: 1674916
Ion Ratio Lower Upper
240 100
120 9.4 8.2 12.2
236 25.5 20.6 30.8


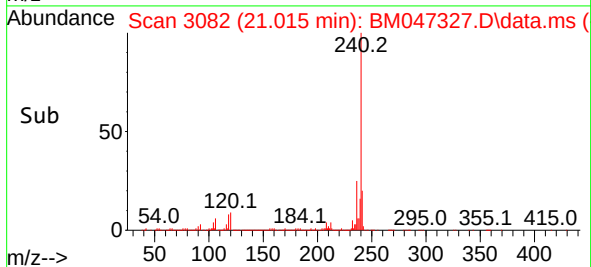
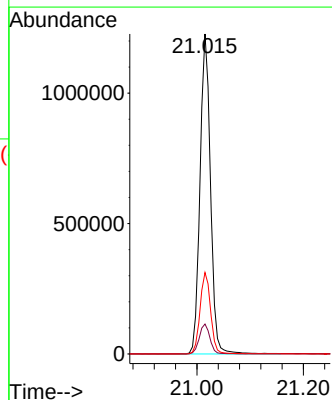
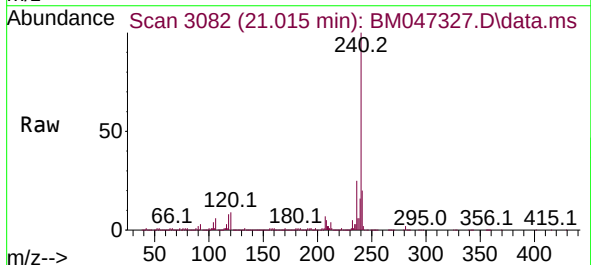


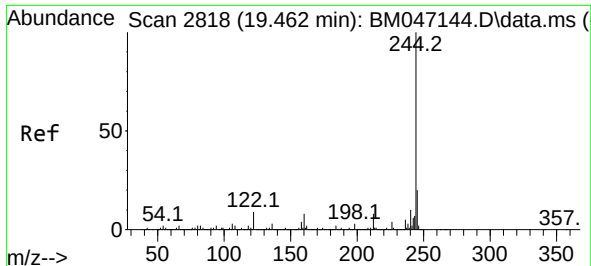

#79
Terphenyl-d14
Concen: 92.704 ng
RT: 19.445 min Scan# 21
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Instrument :
BNA_M
ClientSampleId :
PB162815BL

Tgt Ion:244 Resp: 7246274
Ion Ratio Lower Upper
244 100
212 7.6 6.2 9.4
122 8.2 7.1 10.7

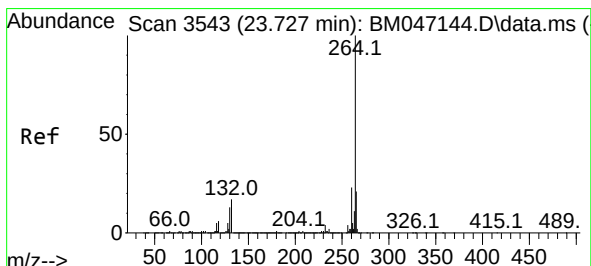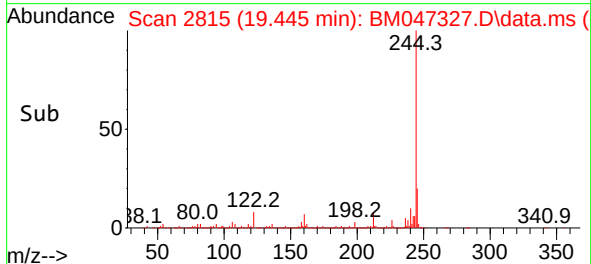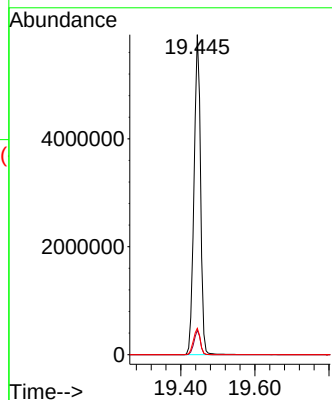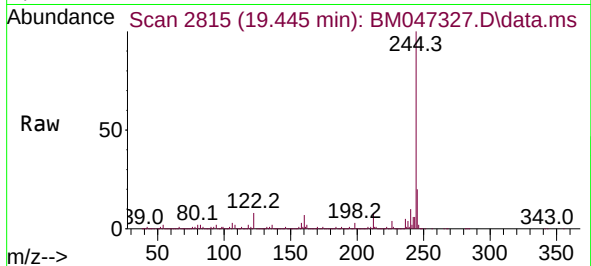

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.709 min Scan# 3540
Delta R.T. -0.018 min
Lab File: BM047327.D
Acq: 23 Aug 2024 10:48

Tgt Ion:264 Resp: 1753650
Ion Ratio Lower Upper
264 100
260 23.2 18.5 27.7
265 21.3 17.3 25.9

