

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
 Data File : BM047332.D
 Acq On : 23 Aug 2024 14:09
 Operator : RC/JU
 Sample : P3518-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-09-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	60	63	78	rBV	379214	505862	6.21%	0.673%
2	4.563	279	285	297	rVB	240094	340154	4.18%	0.453%
3	5.010	355	361	379	rBV	3522902	5038857	61.88%	6.706%
4	6.434	597	603	613	rBV3	30679	97254	1.19%	0.129%
5	6.569	619	626	642	rBV	3305719	5239597	64.35%	6.973%
6	6.981	691	696	711	rBV	143582	255112	3.13%	0.340%
7	7.351	751	759	768	rBV	1115180	1716250	21.08%	2.284%
8	8.498	946	954	968	rBV	2174651	3525488	43.29%	4.692%
9	9.081	1047	1053	1061	rBV2	73072	127658	1.57%	0.170%
10	10.104	1217	1227	1241	rBV	1373548	2304175	28.30%	3.066%
11	10.869	1350	1357	1371	rBV	201401	432749	5.31%	0.576%
12	12.616	1646	1654	1671	rBV	4469411	6783184	83.30%	9.027%
13	14.010	1883	1891	1899	rBV	2086812	3072687	37.73%	4.089%
14	14.251	1925	1932	1933	rBV	2995791	3999207	49.11%	5.322%
15	14.269	1933	1935	1952	rVB	4025160	5044086	61.94%	6.713%
16	15.521	2141	2148	2159	rBV	4296393	6427399	78.93%	8.554%
17	16.015	2226	2232	2238	rVB	60373	99108	1.22%	0.132%
18	16.774	2356	2361	2366	rVV	2646580	3645635	44.77%	4.852%
19	16.815	2366	2368	2372	rVB	171801	202717	2.49%	0.270%
20	16.910	2379	2384	2392	rVB2	80893	136312	1.67%	0.181%
21	17.486	2478	2482	2488	rVB	74139	103579	1.27%	0.138%
22	17.551	2489	2493	2496	rBV	78844	100590	1.24%	0.134%
23	17.715	2515	2521	2538	rBV	2436353	3574874	43.90%	4.757%
24	17.980	2562	2566	2573	rBV5	56423	129820	1.59%	0.173%
25	18.586	2665	2669	2674	rBV3	95611	164074	2.01%	0.218%
26	18.674	2680	2684	2688	rVB	207789	261208	3.21%	0.348%
27	18.851	2710	2714	2718	rBV	505139	740288	9.09%	0.985%
28	18.892	2718	2721	2729	rVB2	157971	320267	3.93%	0.426%
29	19.015	2737	2742	2755	rBV	1116562	1707653	20.97%	2.273%
30	19.221	2769	2777	2783	rBV	409205	672945	8.26%	0.896%
31	19.445	2809	2815	2819	rBV	6481415	8142958	100.00%	10.837%
32	19.480	2819	2821	2828	rVB3	138995	170273	2.09%	0.227%
33	19.756	2865	2868	2876	rVB2	184014	309344	3.80%	0.412%
34	20.109	2923	2928	2933	rVB	402592	479970	5.89%	0.639%
35	20.750	3033	3037	3048	rVB2	775277	1156471	14.20%	1.539%
36	21.015	3075	3082	3087	rBV2	2597868	4208126	51.68%	5.600%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047332.D
Acq On : 23 Aug 2024 14:09
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-09-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.974	3410	3415	3422	rVB	408723	708963	8.71%	0.943%
38	23.709	3533	3540	3555	rVB	1342368	3197120	39.26%	4.255%




Sum of corrected areas: 75142014

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047332.D
Acq On : 23 Aug 2024 14:09
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

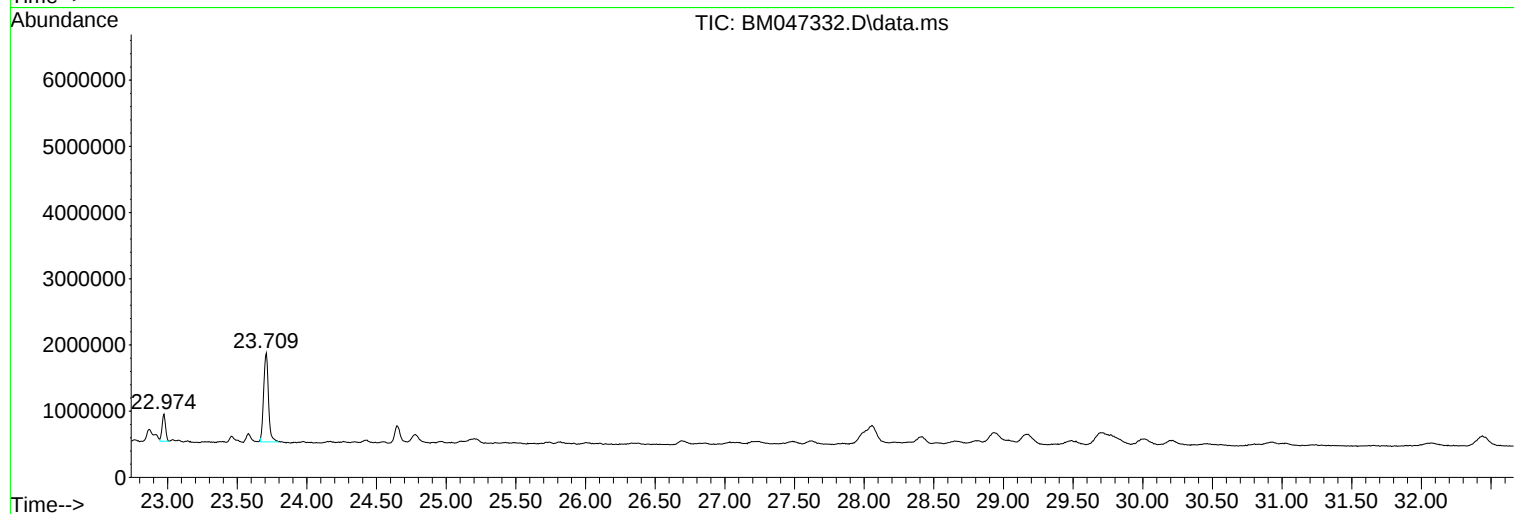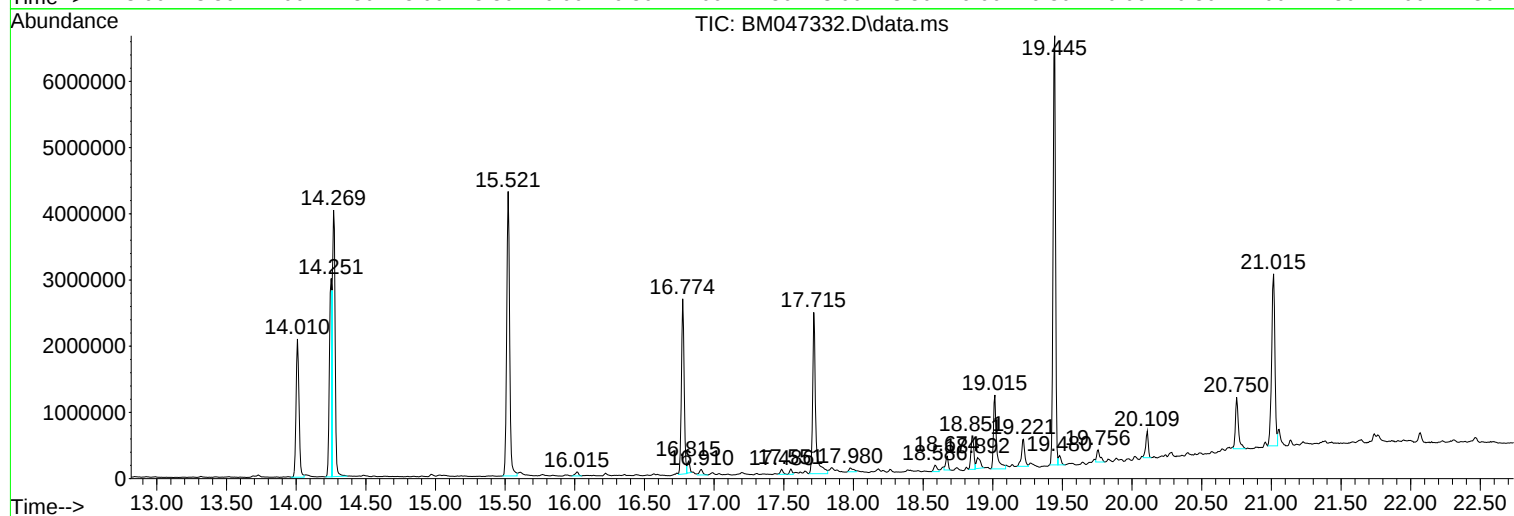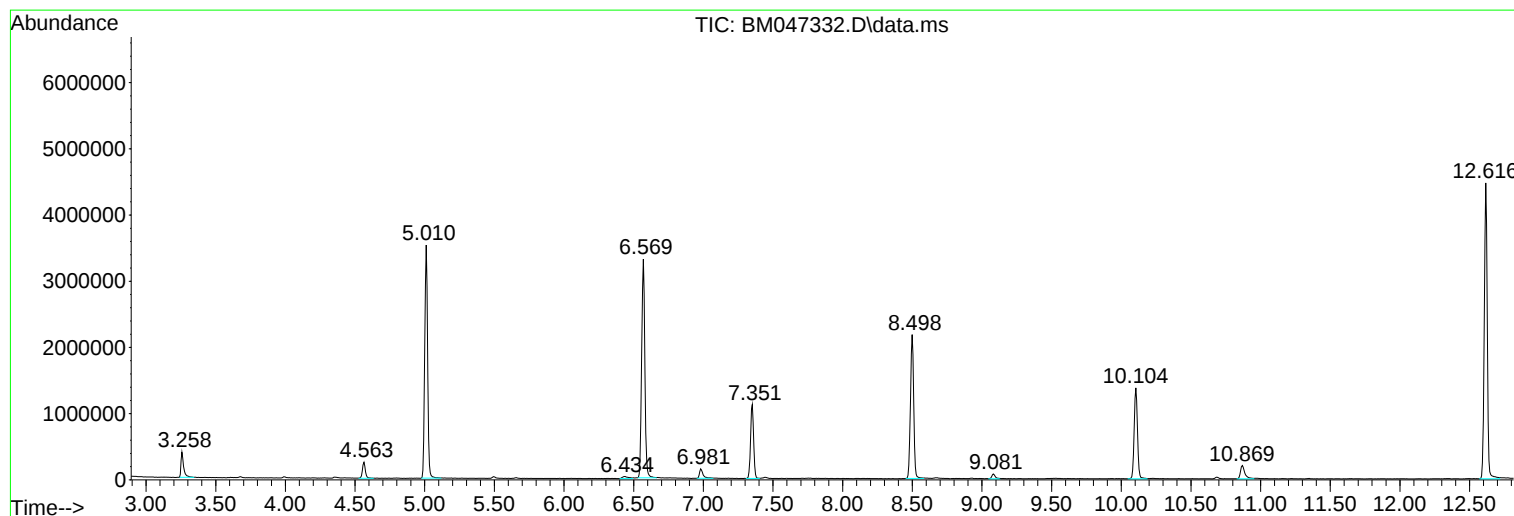

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047332.D
Acq On : 23 Aug 2024 14:09
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047332.D
Acq On : 23 Aug 2024 14:09
Operator : RC/JU
Sample : P3518-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-09-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------