


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047325.D
Acq On : 23 Aug 2024 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

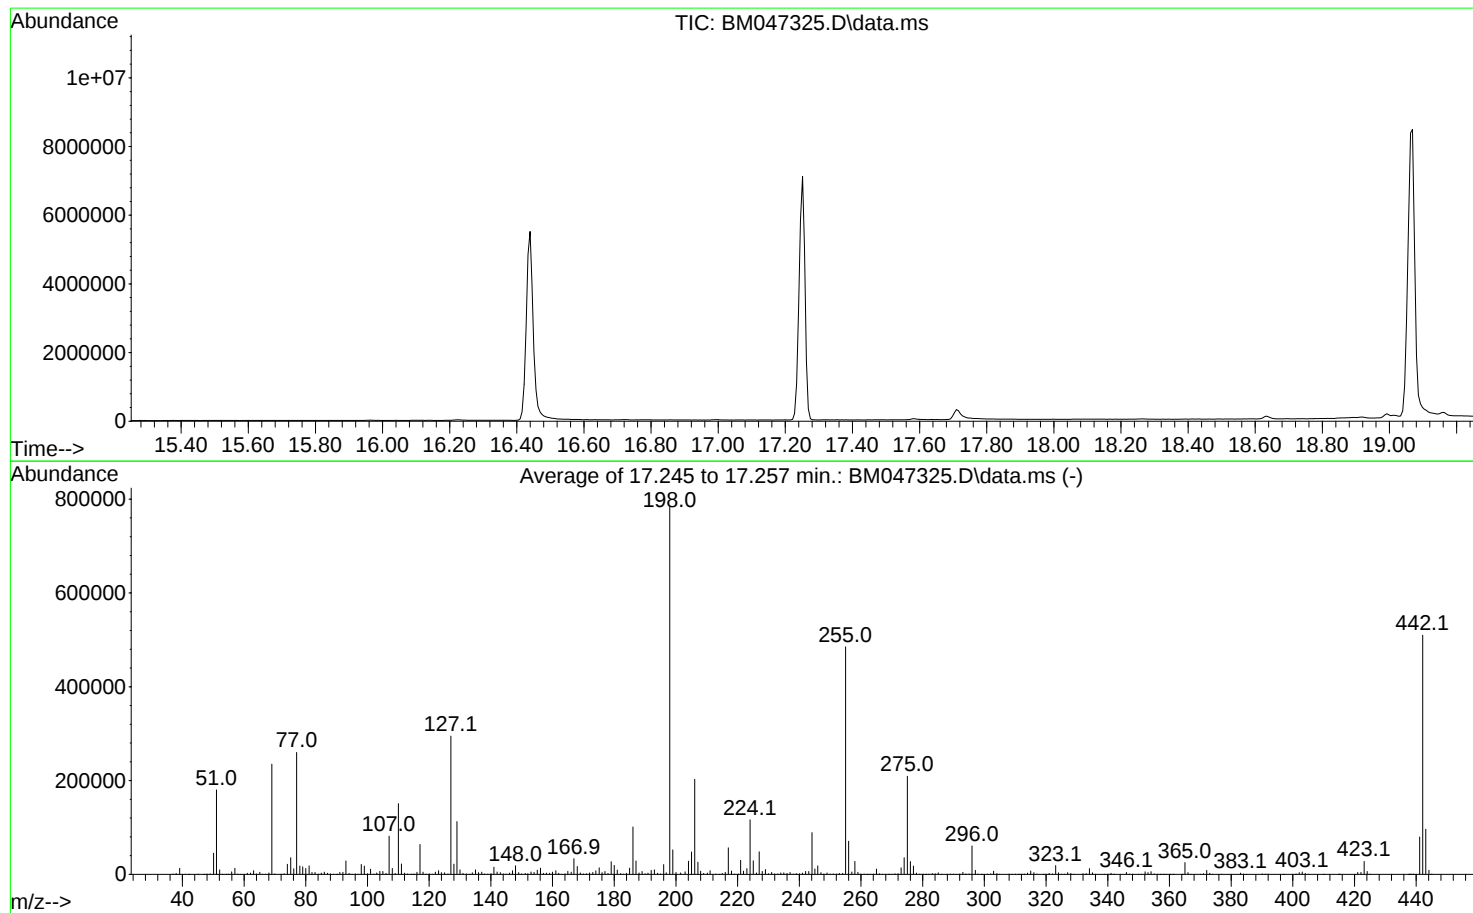

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	180298	PASS
68	69	0.00	2	1.3	3011	PASS
69	198	0.00	100	30.0	234922	PASS
70	69	0.00	2	0.4	874	PASS
127	198	10	80	37.6	294763	PASS
197	198	0.00	2	0.4	3299	PASS
198	198	100	100	100.0	784341	PASS
199	198	5	9	6.6	52149	PASS
275	198	10	60	26.7	209237	PASS
365	198	1	100	3.2	25216	PASS
441	198	0.01	100	10.2	79765	PASS
442	442	50	100	100.0	510016	PASS
443	442	15	24	18.9	96283	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/23/2024	BNA_M	<u>BM047325.D</u>
Compound Name	Response	Retention Time
DDT	2867754	20.31
DDD	62633	19.863
DDE	2819	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65452	2933206	2.23

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
Data File : BM047325.D
Acq On : 23 Aug 2024 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:16:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

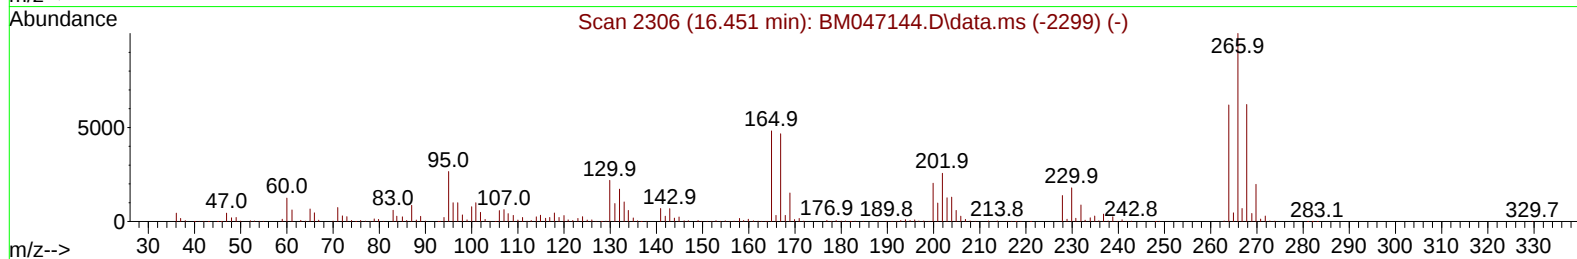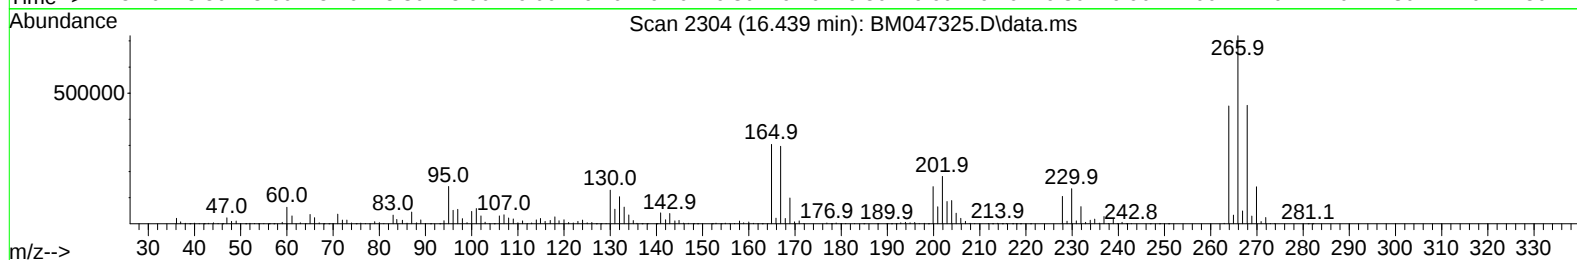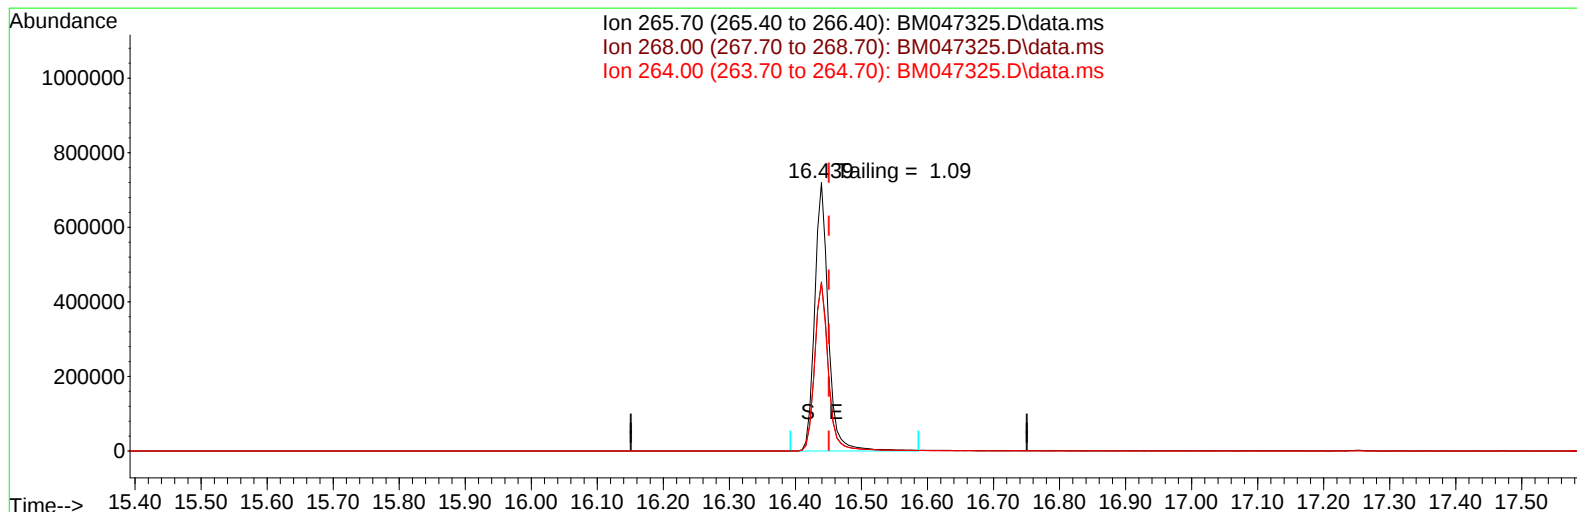

TIC: BM047325.D\data.ms

(70) Pentachlorophenol (C)

16.439min (-0.012) 0.00 ng




response 1030146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.03
264.00	62.00	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082324\
 Data File : BM047325.D
 Acq On : 23 Aug 2024 09:29
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 23 11:16:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 11 23:47:58 2024
 Response via : Initial Calibration

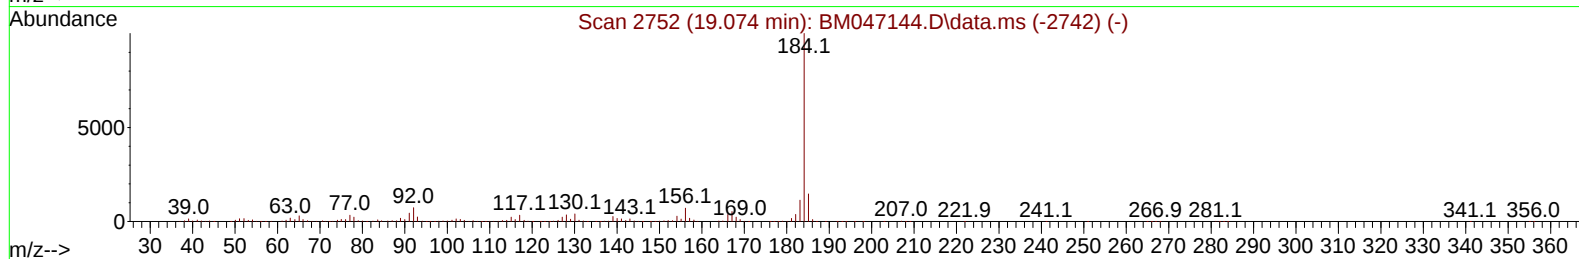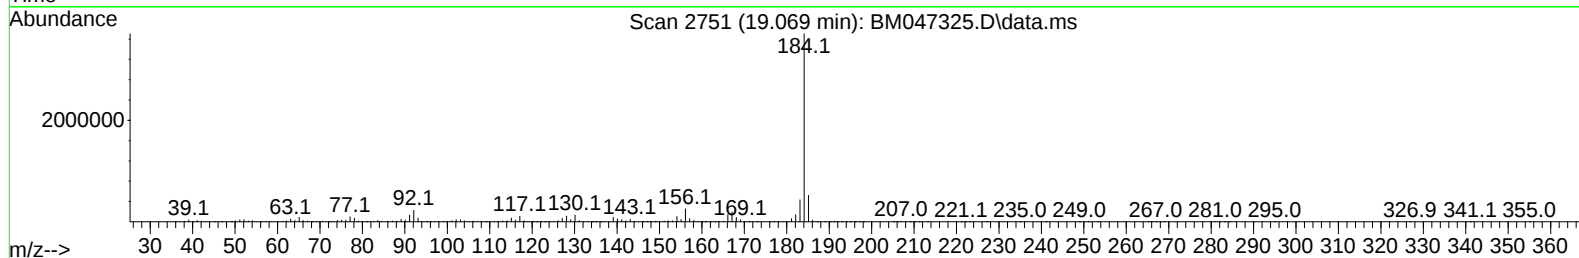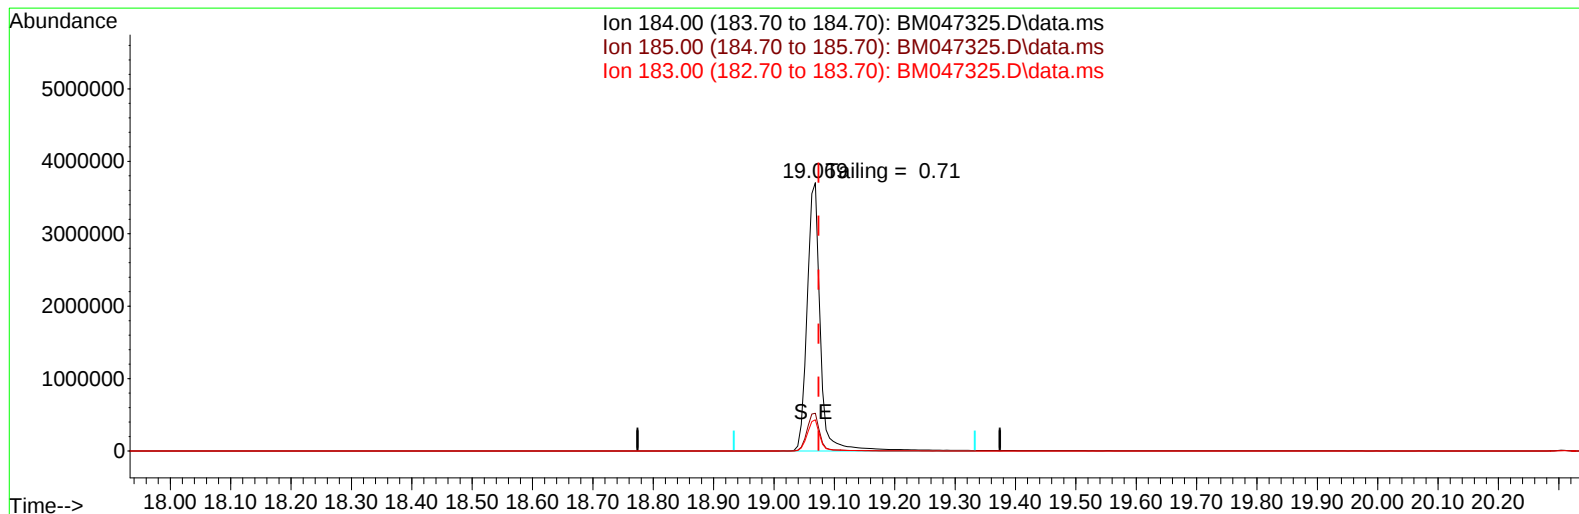

TIC: BM047325.D\data.ms

(77) Benzidine

19.069min (-0.006) 676188.76 ng

response 5676224

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.07
183.00	11.30	11.63
0.00	0.00	0.00