

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082418\
 Data File : BM016589.D
 Acq On : 24 Aug 2018 15:39
 Operator : SJ/JU
 Sample : J4556-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 20180517-FIELD-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.552	380	385	400	rBV	534663	1011273	4.27%	1.542%
2	7.187	658	663	681	rBV	301970	597764	2.53%	0.911%
3	7.534	716	722	737	rBV	1858705	3094855	13.08%	4.718%
4	8.010	797	803	816	rBV	436048	808061	3.41%	1.232%
5	8.322	849	856	876	rBV	2143111	3539280	14.95%	5.395%
6	9.193	998	1004	1025	rBV	1357029	2393033	10.11%	3.648%
7	10.816	1272	1280	1291	rBV	497868	938916	3.97%	1.431%
8	13.263	1690	1696	1709	rBV	6229172	8570646	36.21%	13.066%
9	14.645	1924	1931	1947	rBV2	1346169	2109281	8.91%	3.216%
10	16.145	2179	2186	2205	rBV	7552689	10247464	43.29%	15.622%
11	17.392	2392	2398	2410	rBV	1445344	2163956	9.14%	3.299%
12	19.980	2832	2838	2847	rBV	21077977	23668984	100.00%	36.082%
13	21.533	3098	3102	3110	rBV	2374265	3079998	13.01%	4.695%
14	23.815	3484	3490	3499	rBV	1610083	3373699	14.25%	5.143%


Sum of corrected areas: 65597210

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082418\
Data File : BM016589.D
Acq On : 24 Aug 2018 15:39
Operator : SJ/JU
Sample : J4556-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20180517-FIELD-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

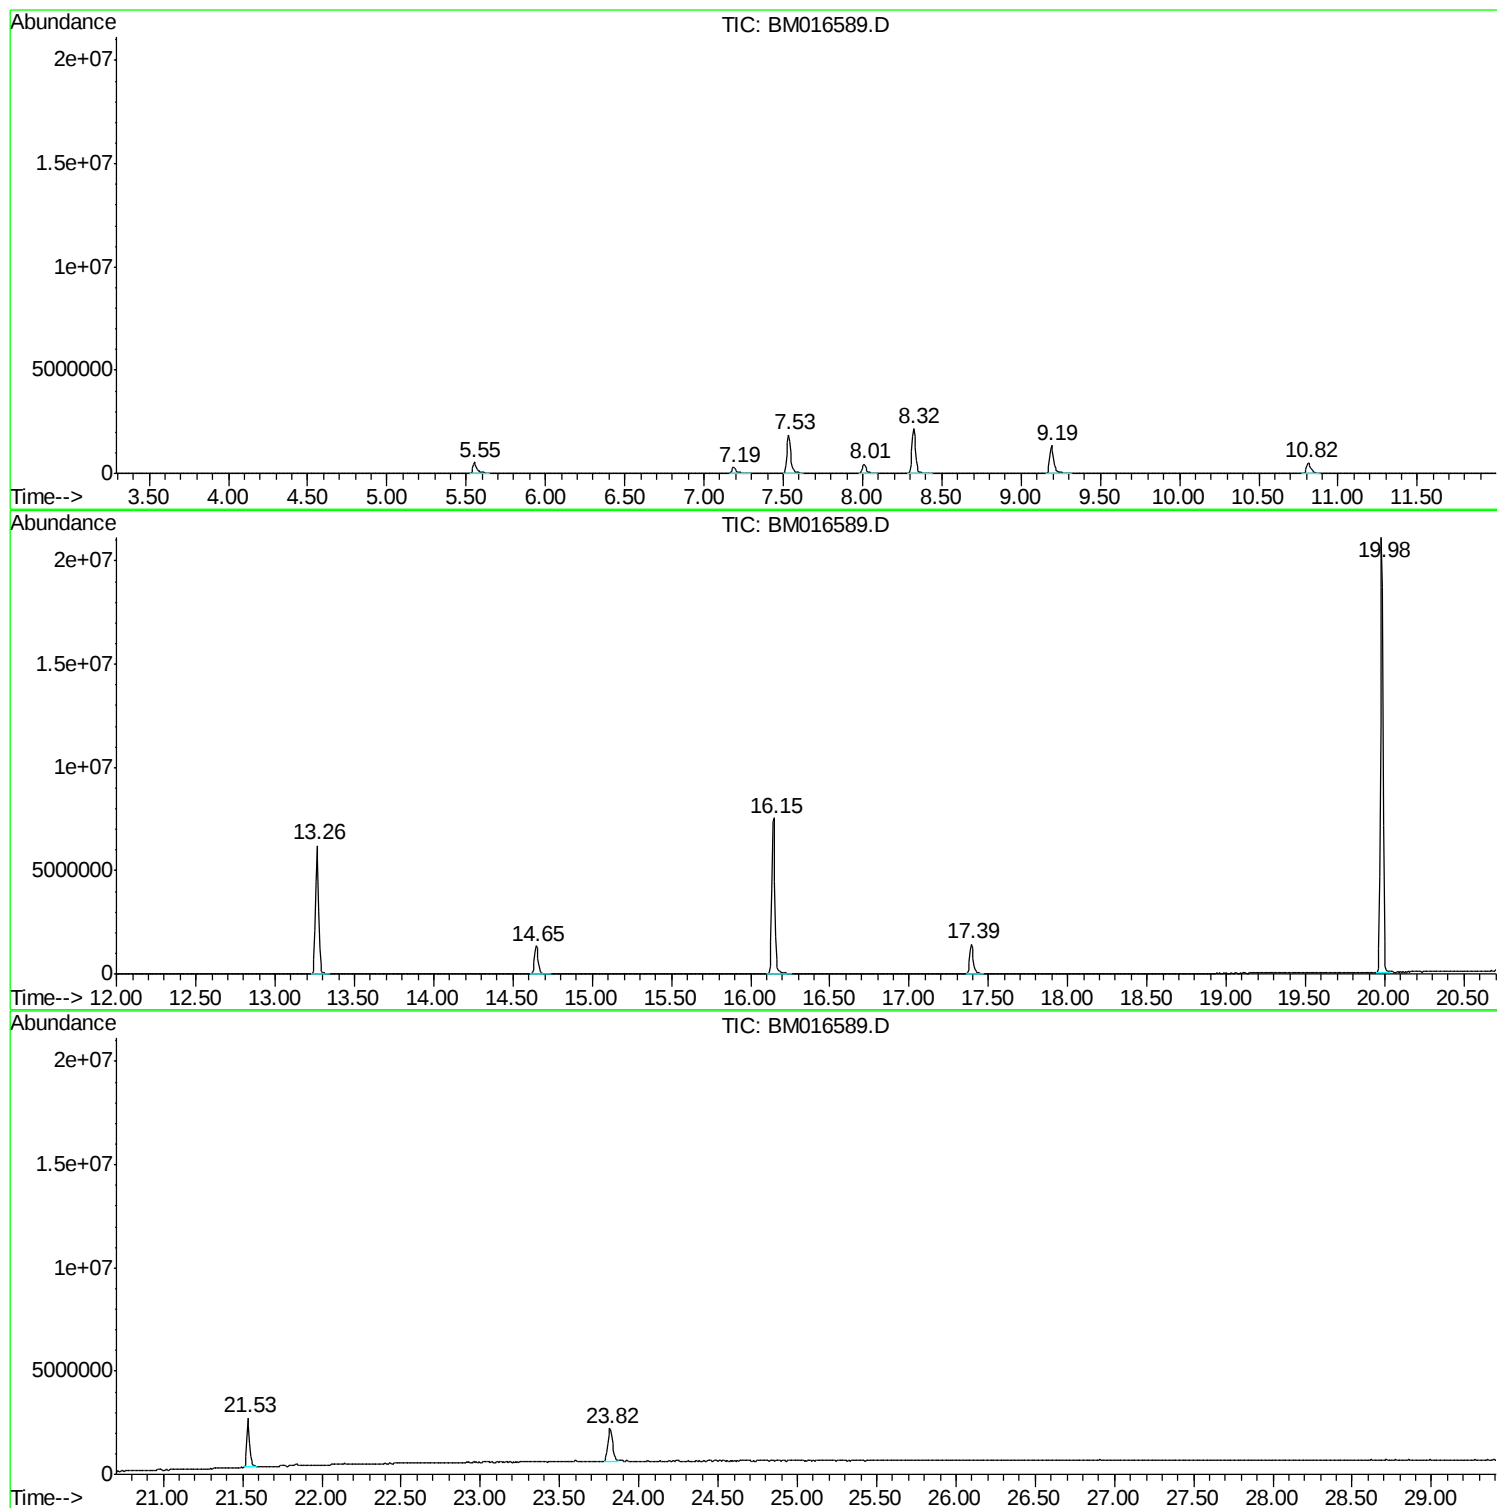

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082418\
Data File : BM016589.D
Acq On : 24 Aug 2018 15:39
Operator : SJ/JU
Sample : J4556-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20180517-FIELD-BLANK










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	76.60 ng	3094860	1,4-Dichlorobenzene-d4	8.01

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
3			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10
4			3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10
5			(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10

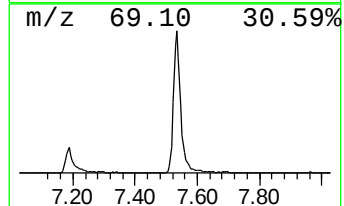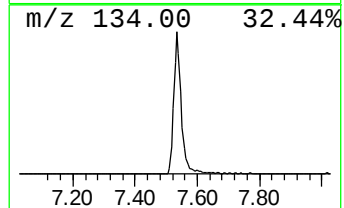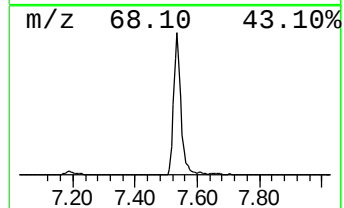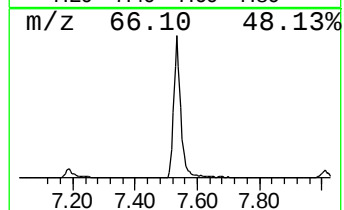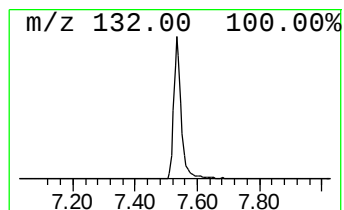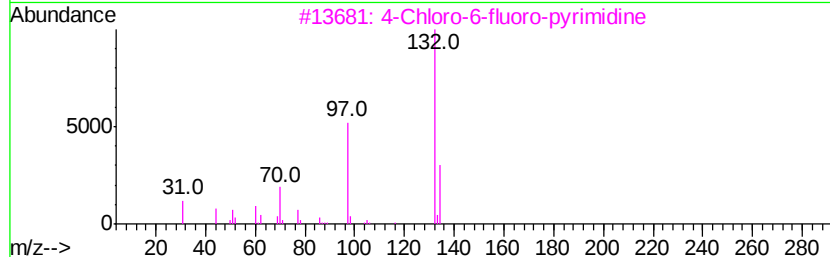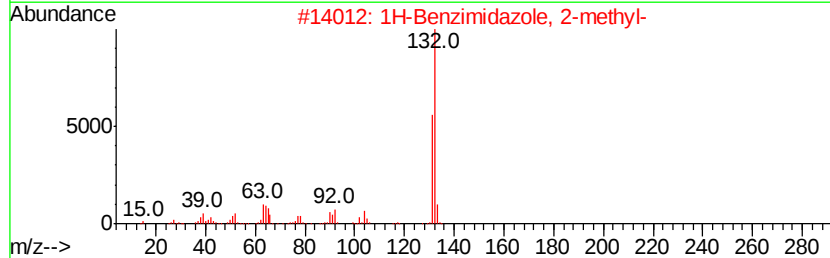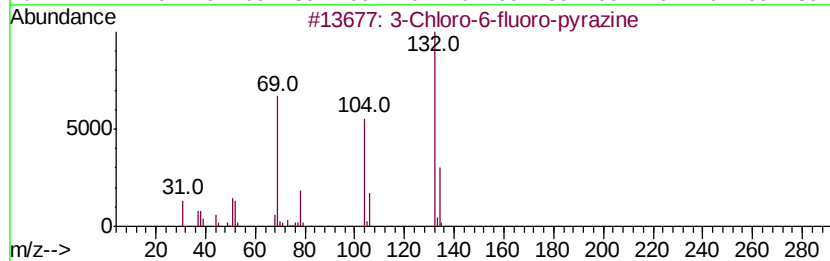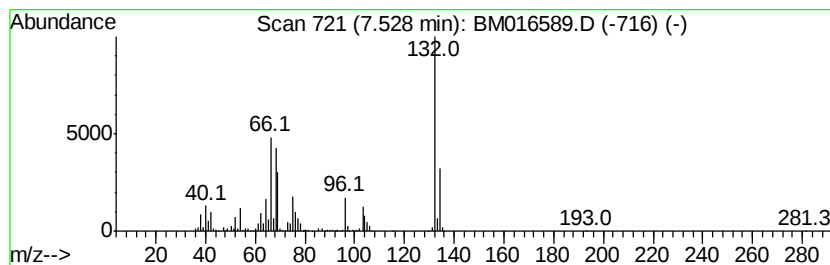

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082418\
Data File : BM016589.D
Acq On : 24 Aug 2018 15:39
Operator : SJ/JU
Sample : J4556-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20180517-FIELD-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.53	7.53	76.6	ng	3094860	1	8.01	808061	20.0