

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082418\
 Data File : BM016592.D
 Acq On : 24 Aug 2018 17:27
 Operator : SJ/JU
 Sample : PB112017BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112017BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.546	379	384	397	rBV	1894880	2956451	18.90%	5.176%
2	7.181	656	662	684	rBV	1866140	3046755	19.47%	5.334%
3	7.534	716	722	741	rBV	2327760	3739205	23.90%	6.547%
4	8.004	796	802	814	rBV	506764	950376	6.07%	1.664%
5	8.322	849	856	870	rBV	2017210	3286587	21.01%	5.754%
6	9.192	998	1004	1018	rBV	1123854	1951722	12.47%	3.417%
7	10.816	1273	1280	1291	rBV	554641	1058958	6.77%	1.854%
8	13.263	1690	1696	1712	rBV	5085998	6982279	44.62%	12.225%
9	14.645	1923	1931	1947	rBV2	1006600	1595865	10.20%	2.794%
10	16.139	2179	2185	2205	rBV	5106773	7162013	45.77%	12.539%
11	17.392	2392	2398	2408	rBV	1631603	2362717	15.10%	4.137%
12	19.980	2832	2838	2848	rBV	14225154	15646588	100.00%	27.394%
13	21.533	3097	3102	3111	rBV	2342427	3134078	20.03%	5.487%
14	23.815	3484	3490	3500	rBV	1629811	3242412	20.72%	5.677%


Sum of corrected areas: 57116006

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082418\
Data File : BM016592.D
Acq On : 24 Aug 2018 17:27
Operator : SJ/JU
Sample : PB112017BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112017BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

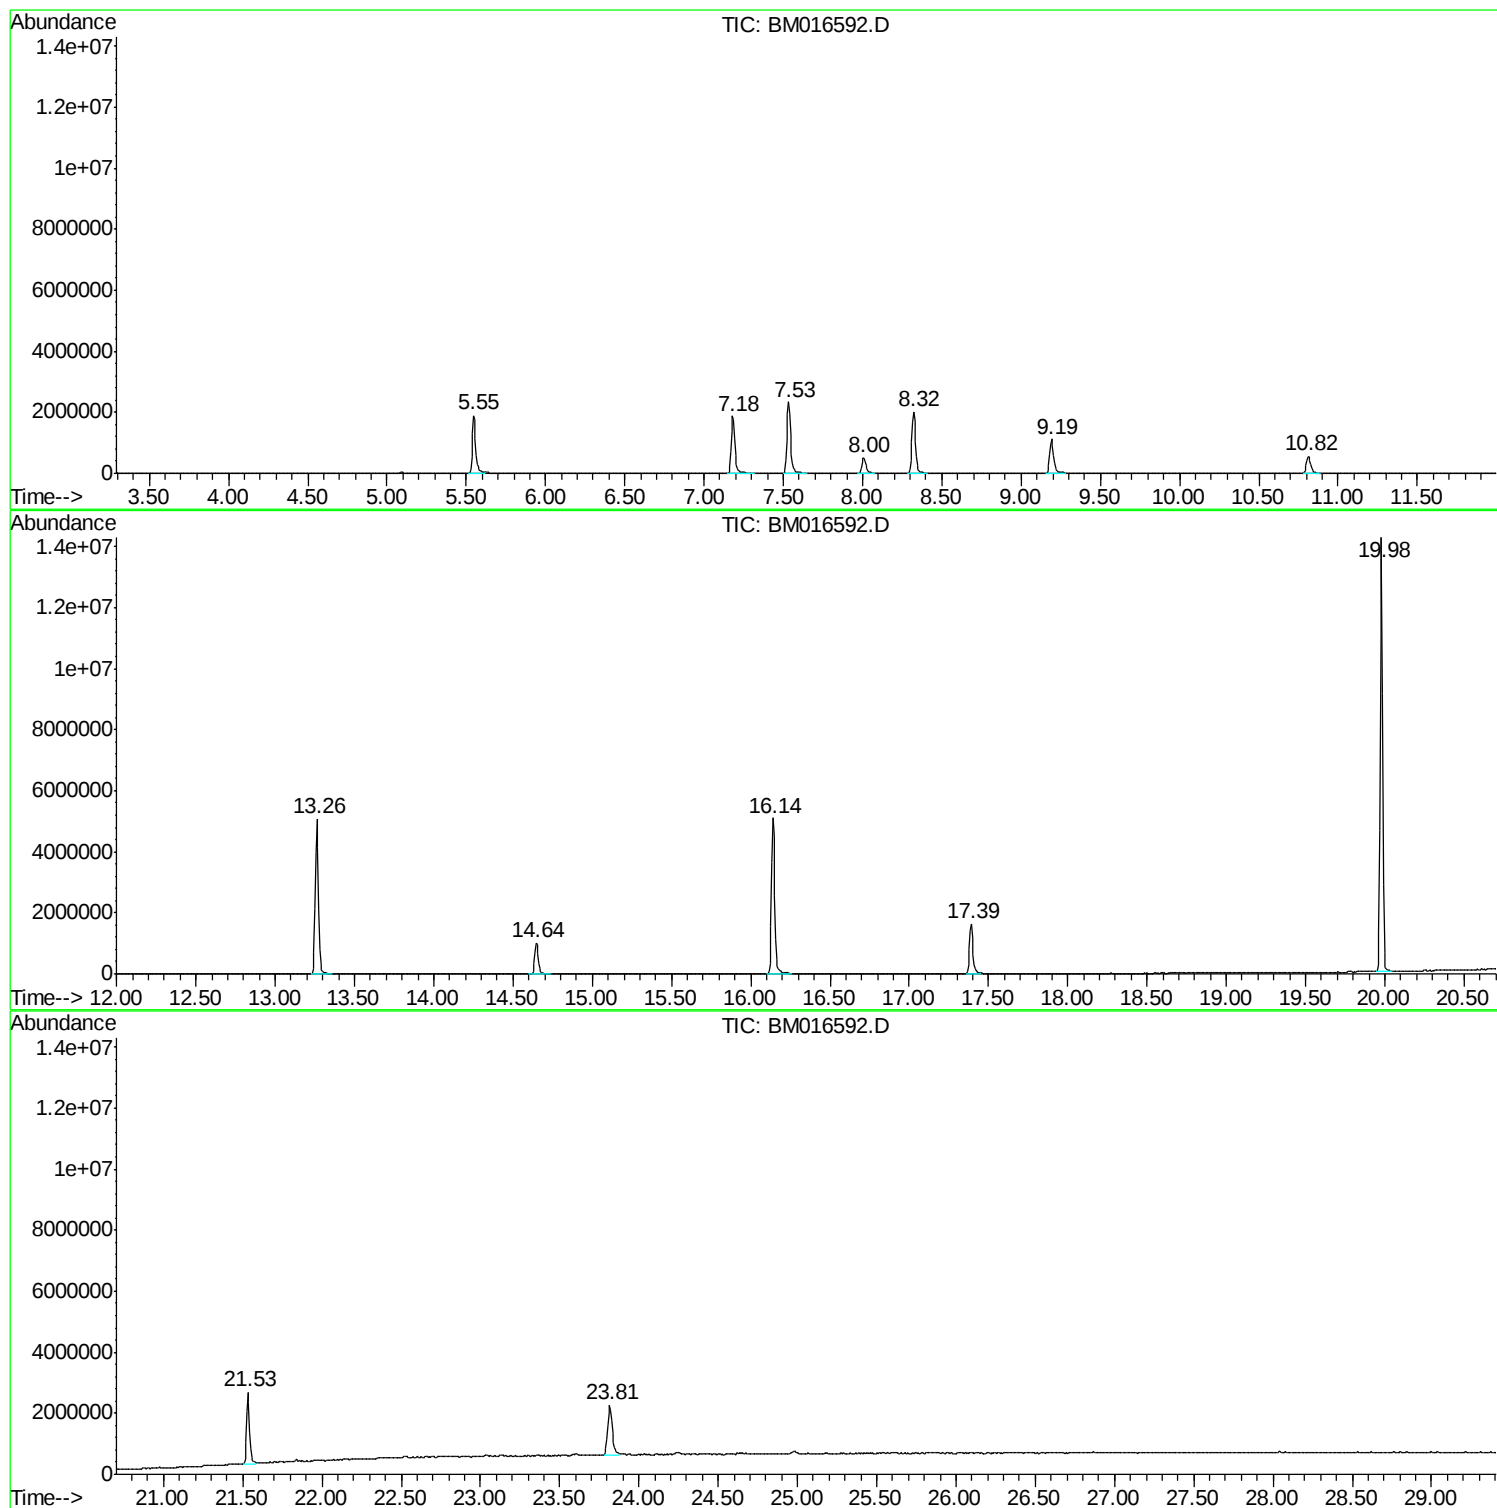

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082418\
Data_File : BM016592.D
Acq_On : 24 Aug 2018 17:277
Operator : SJ/JUU
Sample : PB112017BLL
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
PB112017BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
