


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082418\
 Data File : BM016578.D
 Acq On : 24 Aug 2018 08:27
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 24 10:59:20 2018

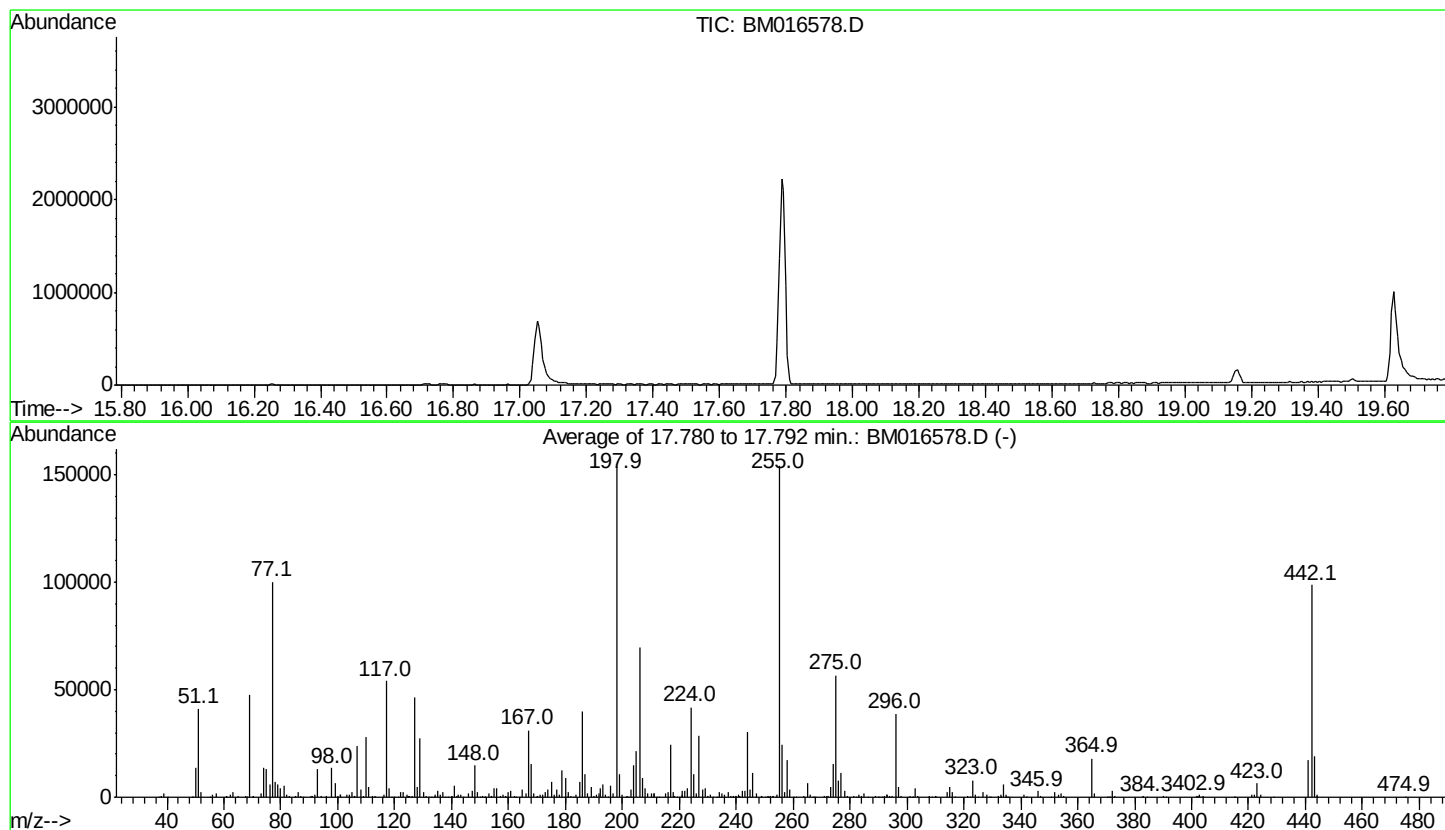

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	41109	PASS
68	69	0.00	2	1.5	706	PASS
69	198	0.00	100	31.1	47872	PASS
70	69	0.00	2	0.9	430	PASS
127	198	10	80	30.2	46480	PASS
197	198	0.00	2	1.0	1607	PASS
198	198	100	100	100.0	153936	PASS
199	198	5	9	7.1	10909	PASS
275	198	10	60	37.0	56893	PASS
365	198	1	100	11.7	18033	PASS
441	198	0.01	100	11.2	17192	PASS
442	198	50	100	64.2	98760	PASS
443	442	15	24	19.4	19182	PASS