

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
 Data File : BM031877.D
 Acq On : 24 Aug 2021 09:08
 Operator : CG/JU
 Sample : PB138103BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138103BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.728	276	279	297	rVB2	42639	95672	3.52%	0.773%
2	5.163	347	353	366	rVB	1084388	1537662	56.63%	12.430%
3	6.728	611	619	636	rBV	981793	1510415	55.62%	12.209%
4	7.522	748	754	763	rVB	154469	238865	8.80%	1.931%
5	8.681	943	951	967	rBV	560929	928600	34.20%	7.506%
6	10.281	1217	1223	1236	rBV	182850	318178	11.72%	2.572%
7	12.775	1640	1647	1661	rBV	1362944	1914244	70.50%	15.474%
8	14.163	1877	1883	1892	rBV	270709	394147	14.52%	3.186%
9	15.668	2132	2139	2154	rBV	1046252	1490426	54.89%	12.048%
10	16.921	2346	2352	2362	rBV	315534	447680	16.49%	3.619%
11	19.568	2796	2802	2807	rBV	2390296	2715376	100.00%	21.950%
12	21.121	3061	3066	3074	rBV	323232	408122	15.03%	3.299%
13	23.262	3425	3430	3440	rVB	194137	371570	13.68%	3.004%




Sum of corrected areas: 12370957

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
Data File : BM031877.D
Acq On : 24 Aug 2021 09:08
Operator : CG/JU
Sample : PB138103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138103BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

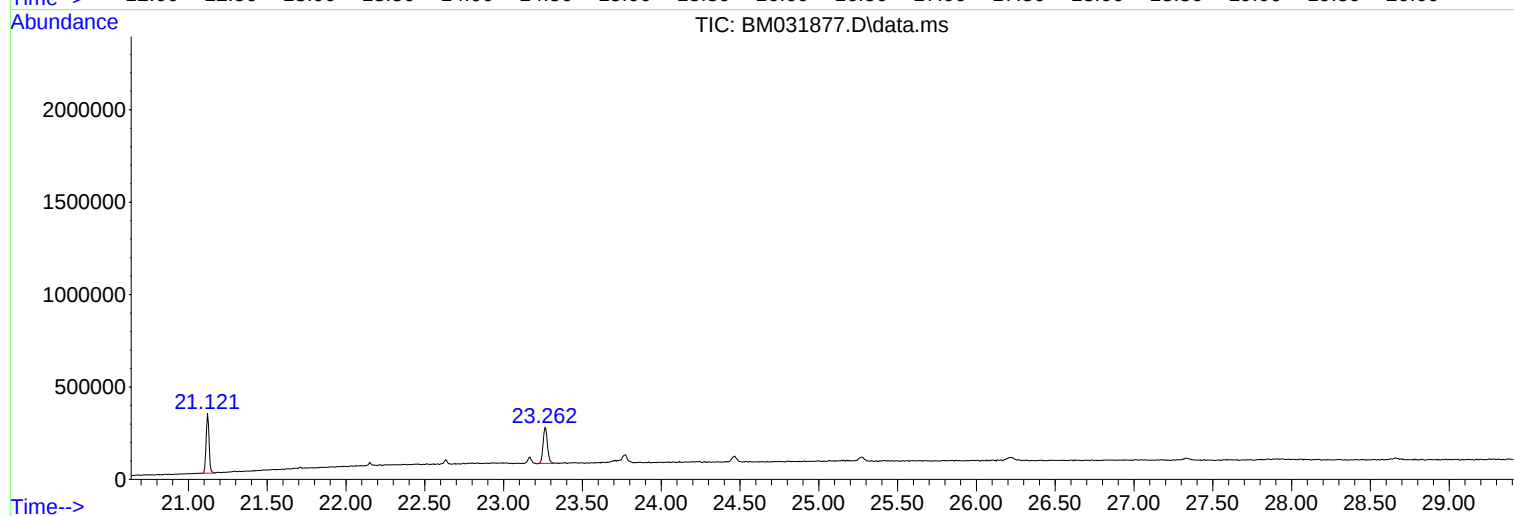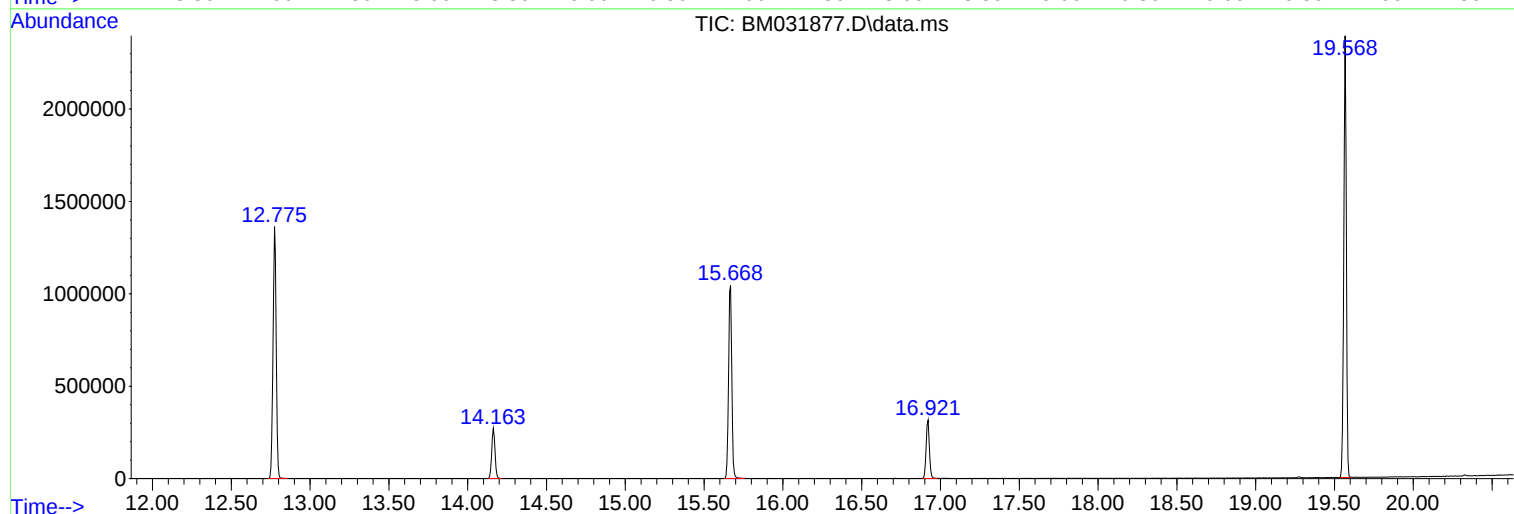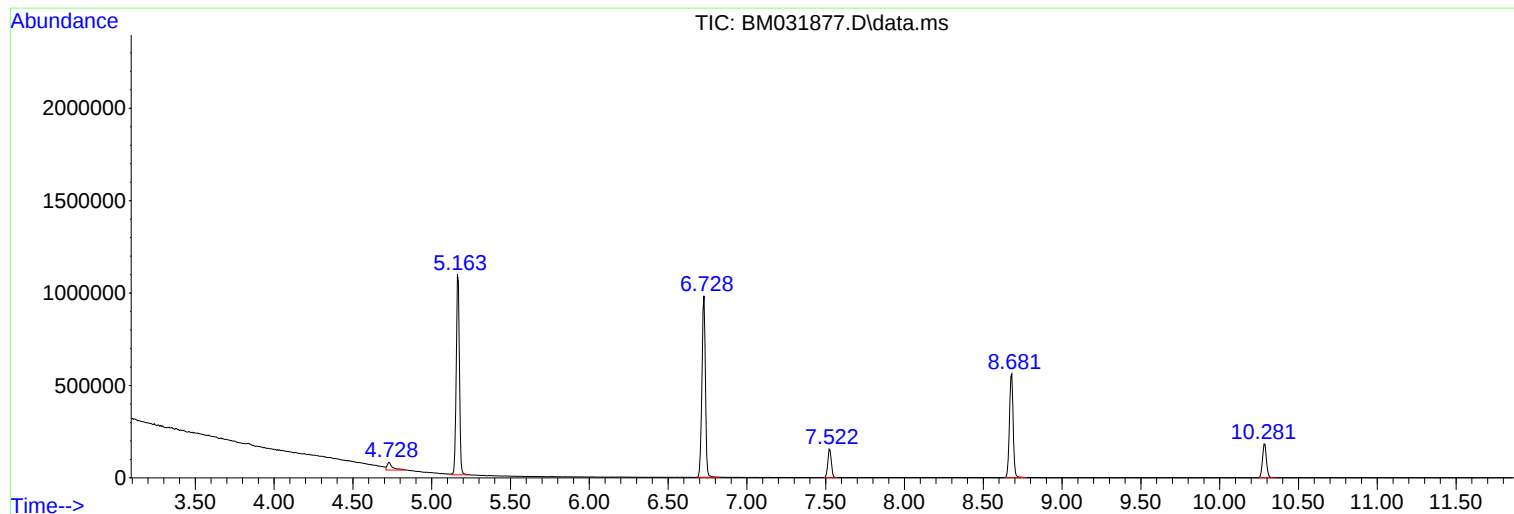

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
Data File : BM031877.D
Acq On : 24 Aug 2021 09:08
Operator : CG/JU
Sample : PB138103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138103BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.728	8.01 ng	95672	1,4-Dichlorobenzene-d4	7.522

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72	
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39	
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36	
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25	
5	1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	17	

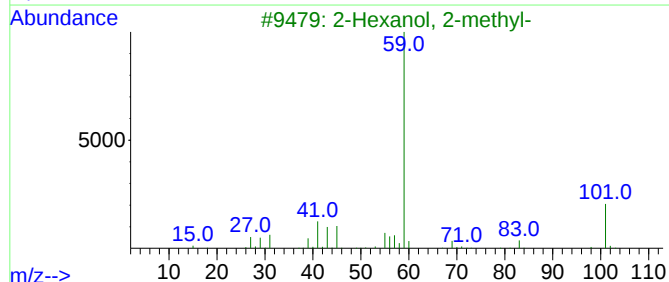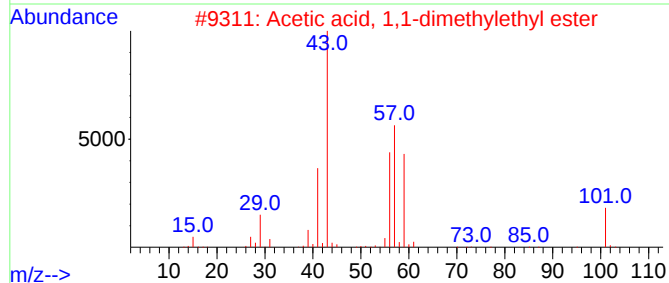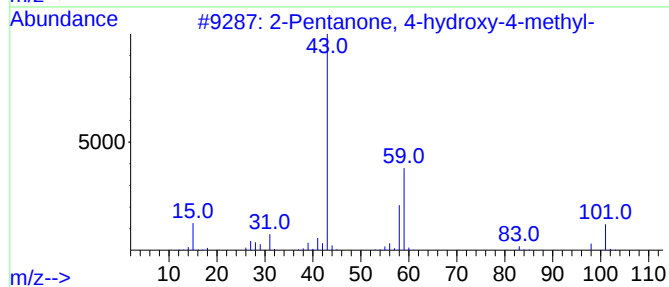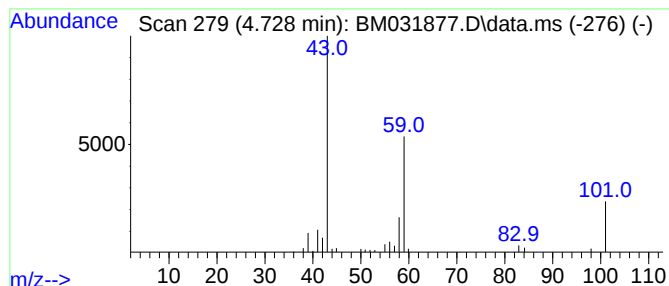

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
Data File : BM031877.D
Acq On : 24 Aug 2021 09:08
Operator : CG/JU
Sample : PB138103BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138103BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.728	8.0	ng	95672	1	7.522	238865	20.0