


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
 Data File : BM031875.D
 Acq On : 24 Aug 2021 06:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 16:34:26 2021

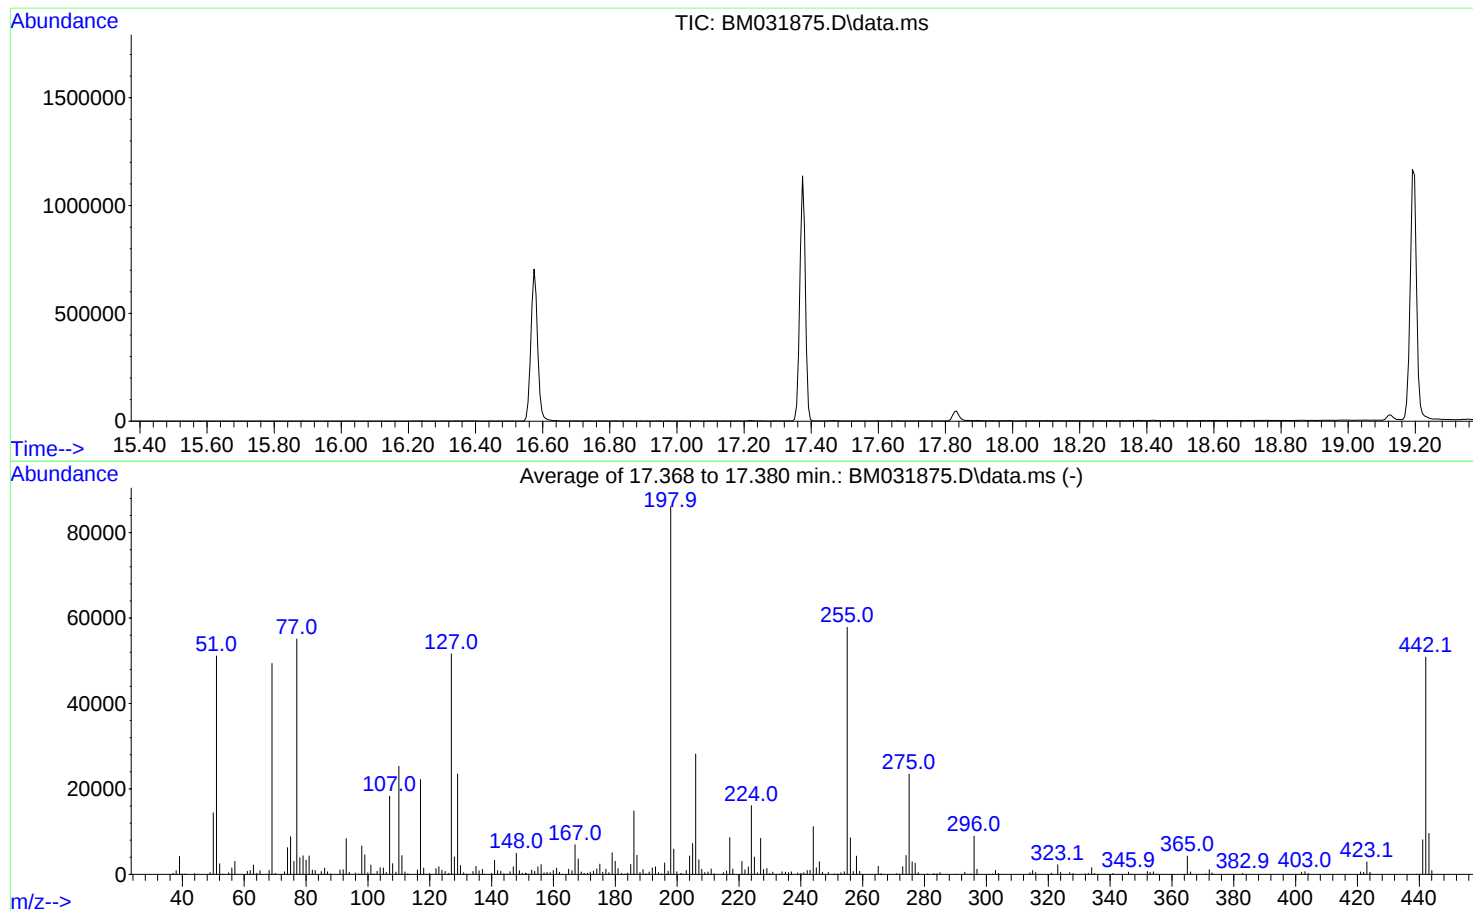




AutoFind: Scans 2428, 2429, 2430; Background Corrected with Scan 2422

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.4	51115	PASS
68	69	0.00	2	1.8	909	PASS
69	198	0.00	100	57.3	49363	PASS
70	69	0.00	2	0.5	260	PASS
127	198	10	80	60.0	51629	PASS
197	198	0.00	2	0.9	754	PASS
198	198	100	100	100.0	86117	PASS
199	198	5	9	6.9	5921	PASS
275	198	10	60	27.2	23448	PASS
365	198	1	100	5.0	4266	PASS
441	198	0.01	100	9.4	8084	PASS
442	442	50	100	100.0	50856	PASS
443	442	15	24	18.9	9592	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
Data File : BM031875.D
Acq On : 24 Aug 2021 06:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 24 13:55:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 15:51:36 2021
Response via : Initial Calibration

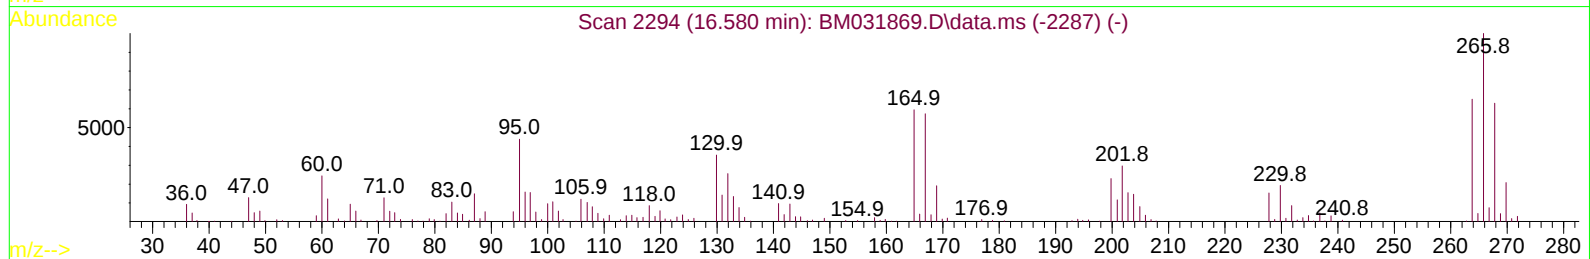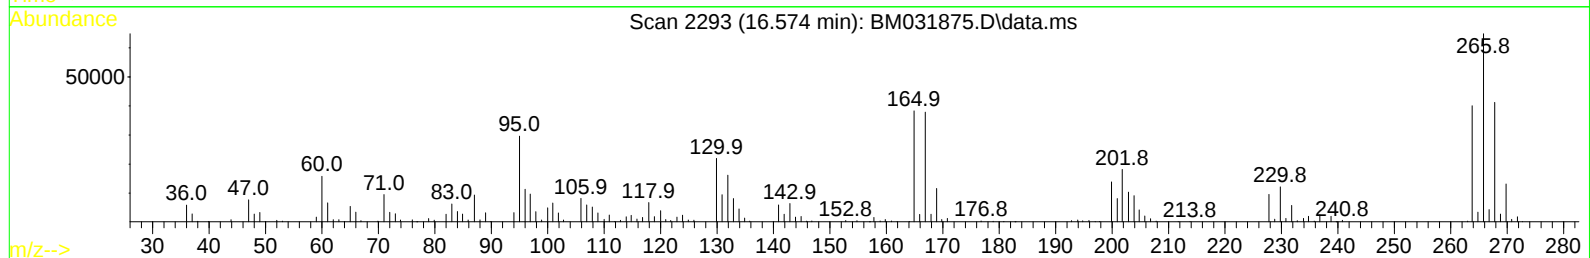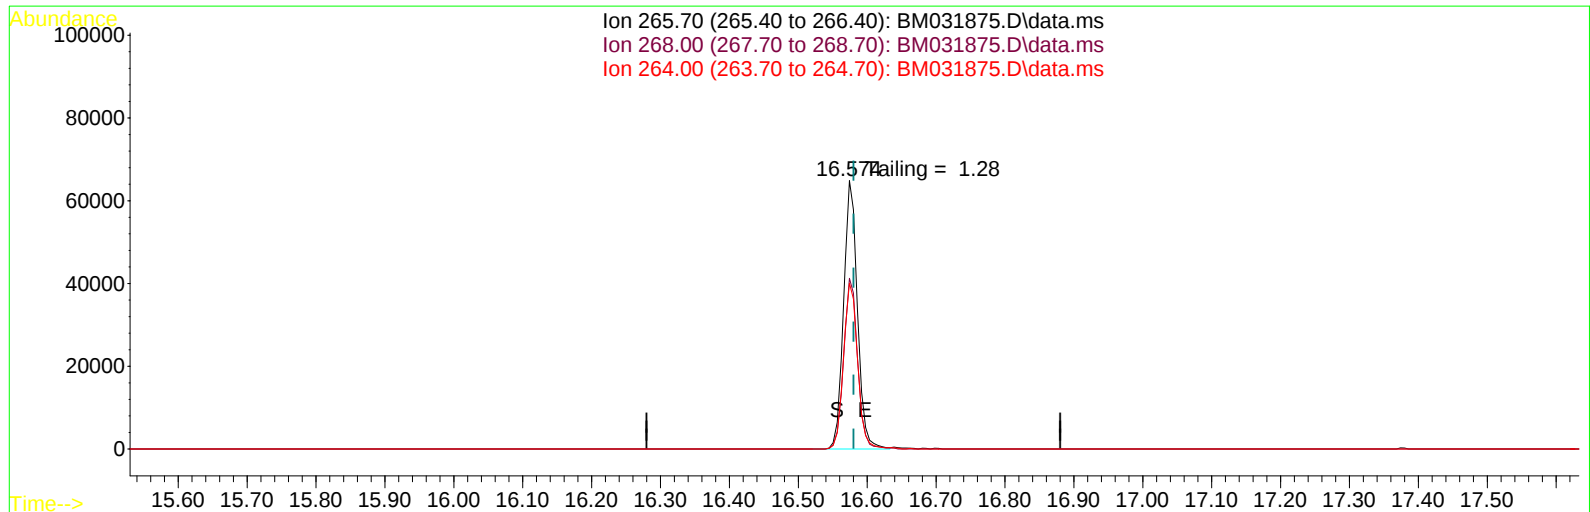

TIC: BM031875.D\data.ms

(70) Pentachlorophenol (C)

16.574min (-0.006) 0.00 ng




response 90692

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.60
264.00	65.10	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082421\
Data File : BM031875.D
Acq On : 24 Aug 2021 06:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 24 13:55:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 15:51:36 2021
Response via : Initial Calibration

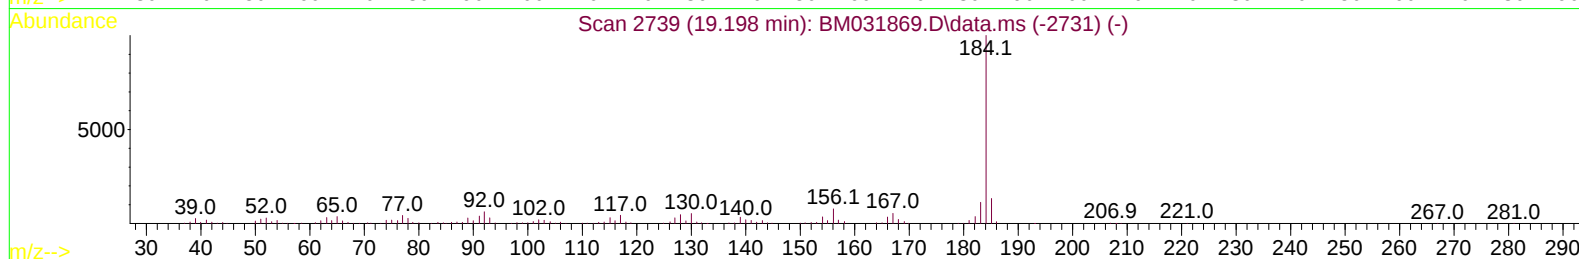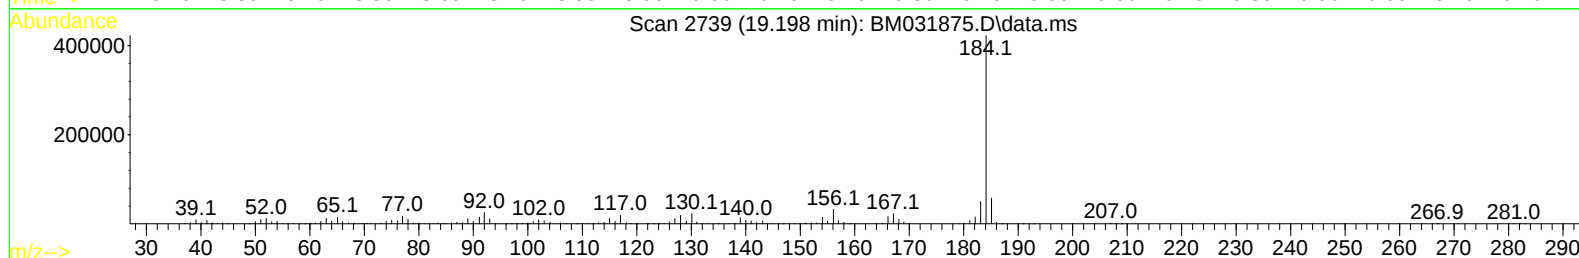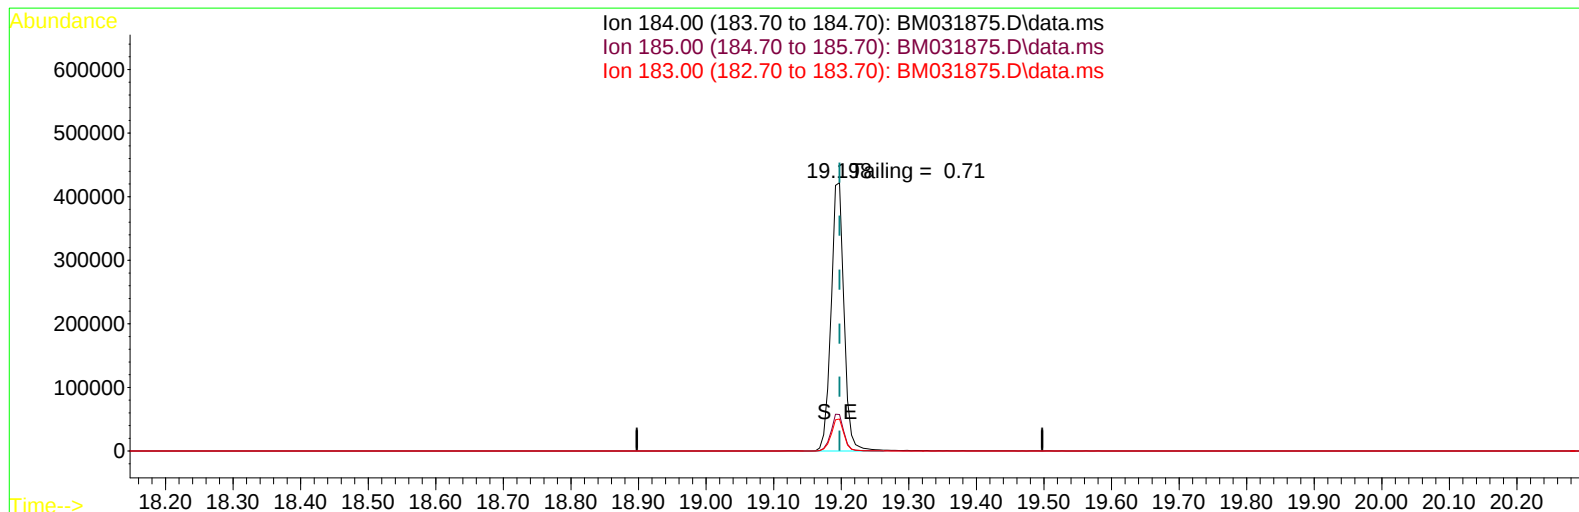

TIC: BM031875.D\data.ms

(77) Benzidine

19.198min (-0.000) 80842.86 ng

response 564371

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.63
183.00	11.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2021	BNA_M	<u>BM031875.D</u>
Compound Name	Response	Retention Time
DDT	313707	20.42
DDD	2266	19.98
DDE	380	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2646	316353	0.84

Instrument :
BNA_M
ClientSampleId :
DFTPP