
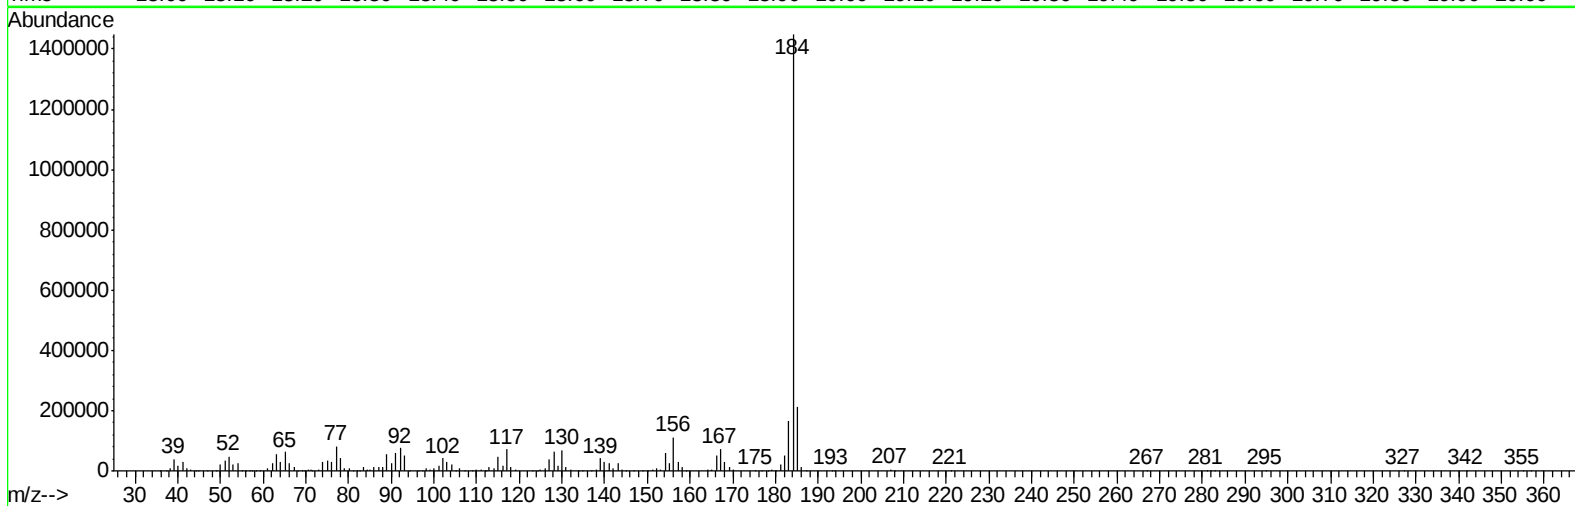


Data Path : Z:\HPCHEM1\BNA M\DATA\BM082517\
Data File : BM011345.D
Acq On : 25 Aug 2017 15:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 01:16:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

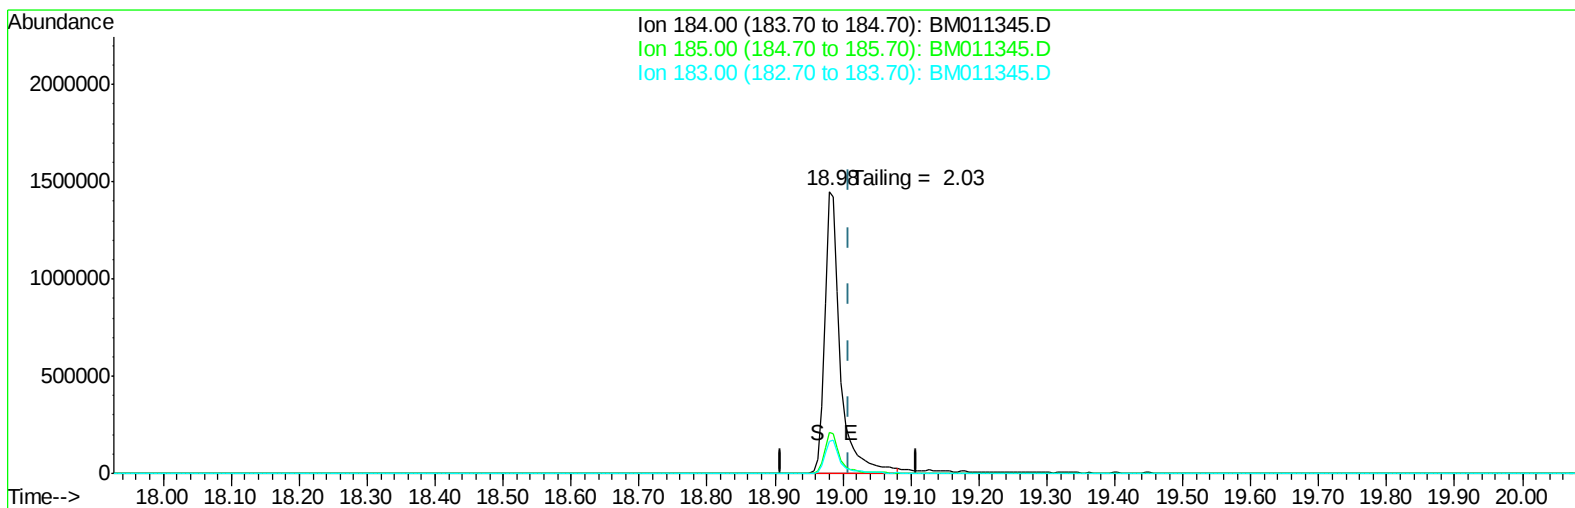

TIC: BM011345.D

(76) Benzidine



18.980min (-0.029) 5596.15ng

response 2339340

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.76
183.00	11.10	11.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM082517\
Data File : BM011345.D
Acq On : 25 Aug 2017 15:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 01:16:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

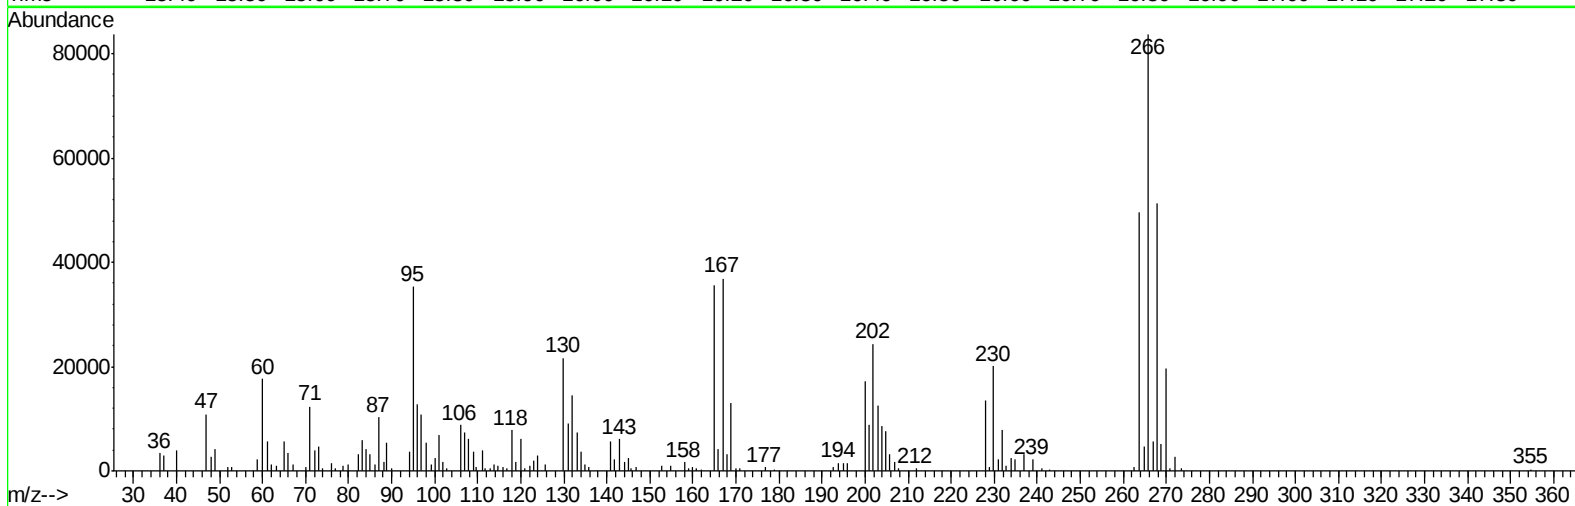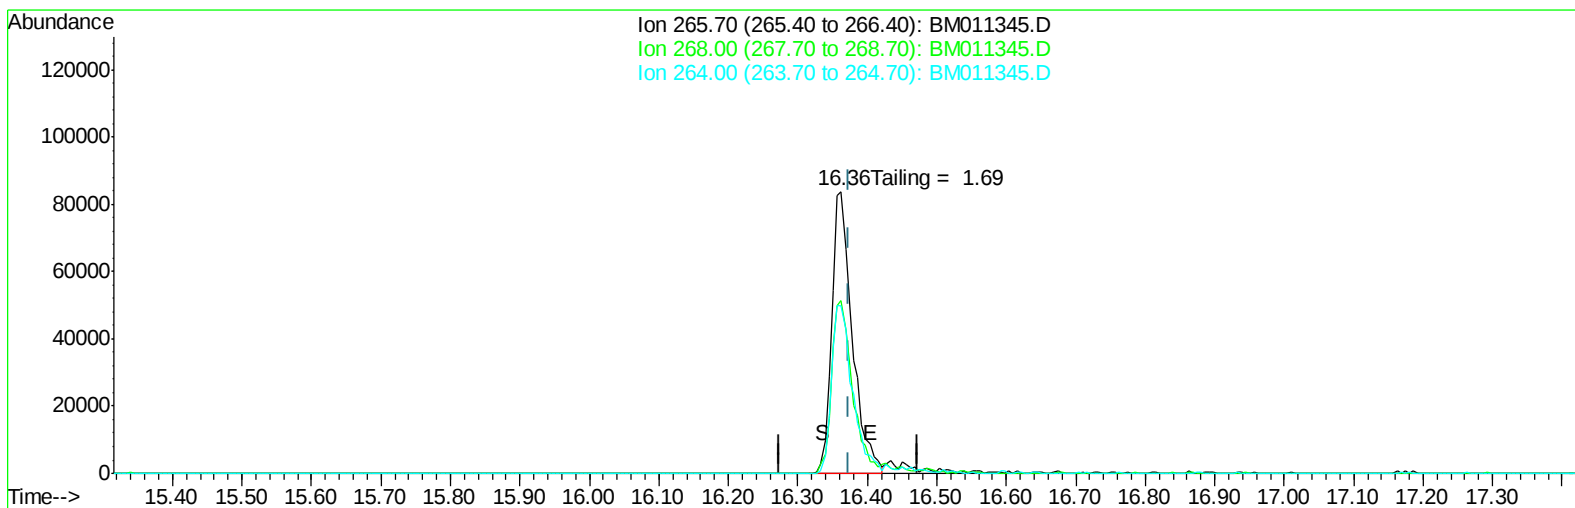

TIC: BM011345.D

(69) Pentachlorophenol (C)

16.363min (-0.012) 1440.33ng

response 171198

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.36
264.00	61.20	59.38
0.00	0.00	0.00