


Data Path : Z:\HPCHEM1\BNA M\Data\BM082517\
 Data File : BM011345.D
 Acq On : 25 Aug 2017 15:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

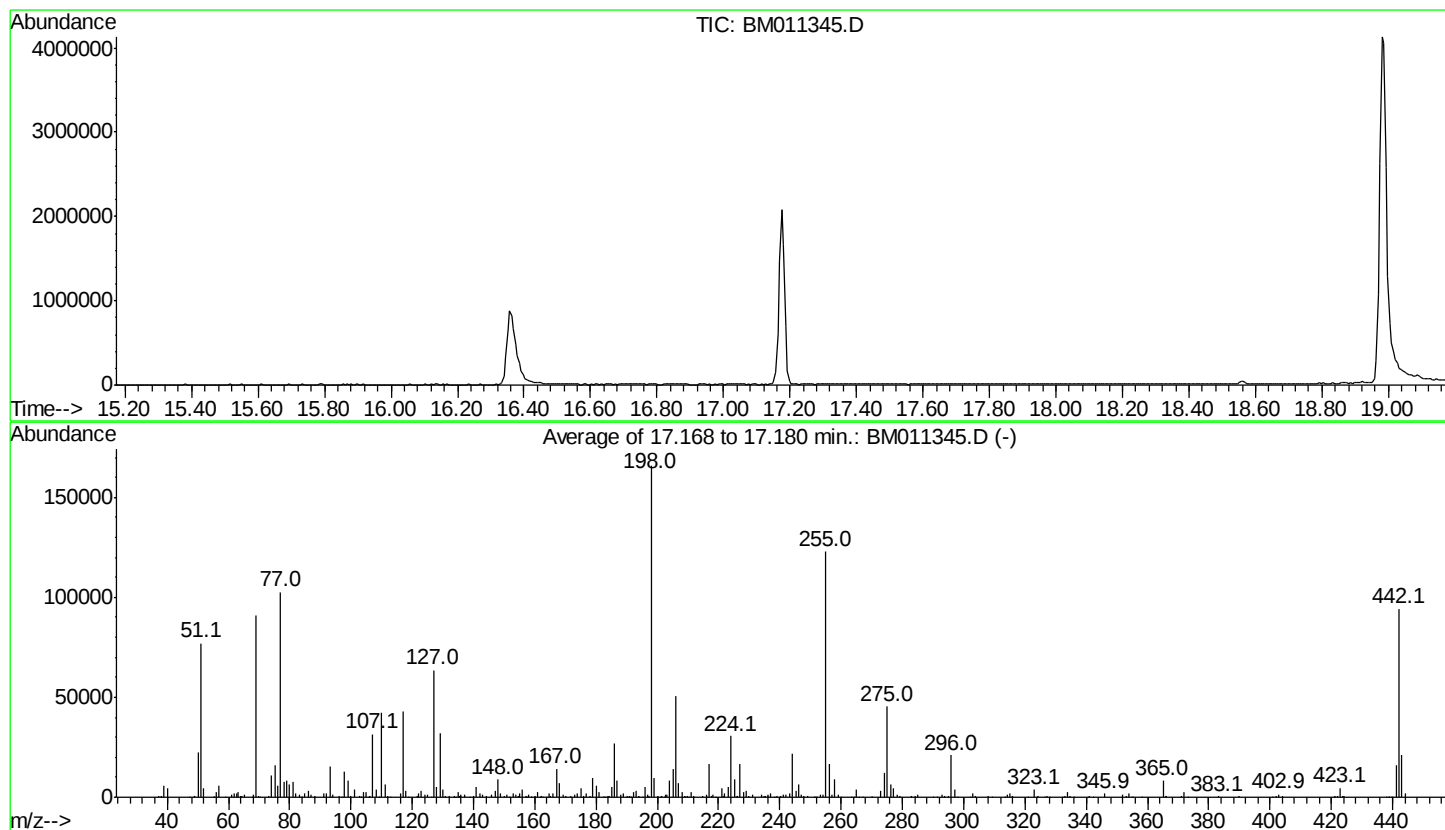

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	76880	PASS
68	69	0.00	2	1.4	1251	PASS
69	198	0.00	100	54.8	90914	PASS
70	69	0.00	2	0.8	720	PASS
127	198	10	80	38.3	63448	PASS
197	198	0.00	2	0.9	1552	PASS
198	198	100	100	100.0	165866	PASS
199	198	5	9	6.0	9923	PASS
275	198	10	60	27.3	45288	PASS
365	198	1	100	4.9	8176	PASS
441	443	0.01	100	77.1	16096	PASS
442	198	50	100	56.8	94288	PASS
443	442	15	24	22.1	20880	PASS