

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
 Data File : BM027235.D
 Acq On : 26 Aug 2020 05:13
 Operator : JU/CG
 Sample : L3613-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBFQ6

Quant Time: Aug 26 06:07:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 26 01:51:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	169503	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	684944	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	483937	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	1080015	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	1115523	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	937341	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	18258	6.10	ng/uL	0.00
5) Phenol-d5	6.78	99	392736	28.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	265823	29.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	311883	29.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	326061	29.55	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	154474	28.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	180219	28.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	357225	27.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	404196	29.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	1122315	29.23	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	1330400	29.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.44	143	153414	23.69	ng/ul	-0.01
58) Fluorene-d10	15.23	176	971742	29.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	151806	21.55	ng/ul	0.00
71) Anthracene-d10	17.08	188	1466470	28.61	ng/ul	0.00
79) Pyrene-d10	19.38	212	1710609	26.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	1556021	29.78	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	454237	11.398	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
Data File : BM027235.D
Acq On : 26 Aug 2020 05:13
Operator : JU/CG
Sample : L3613-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBFQ6

Quant Time: Aug 26 06:07:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 26 01:51:51 2020
Response via : Initial Calibration

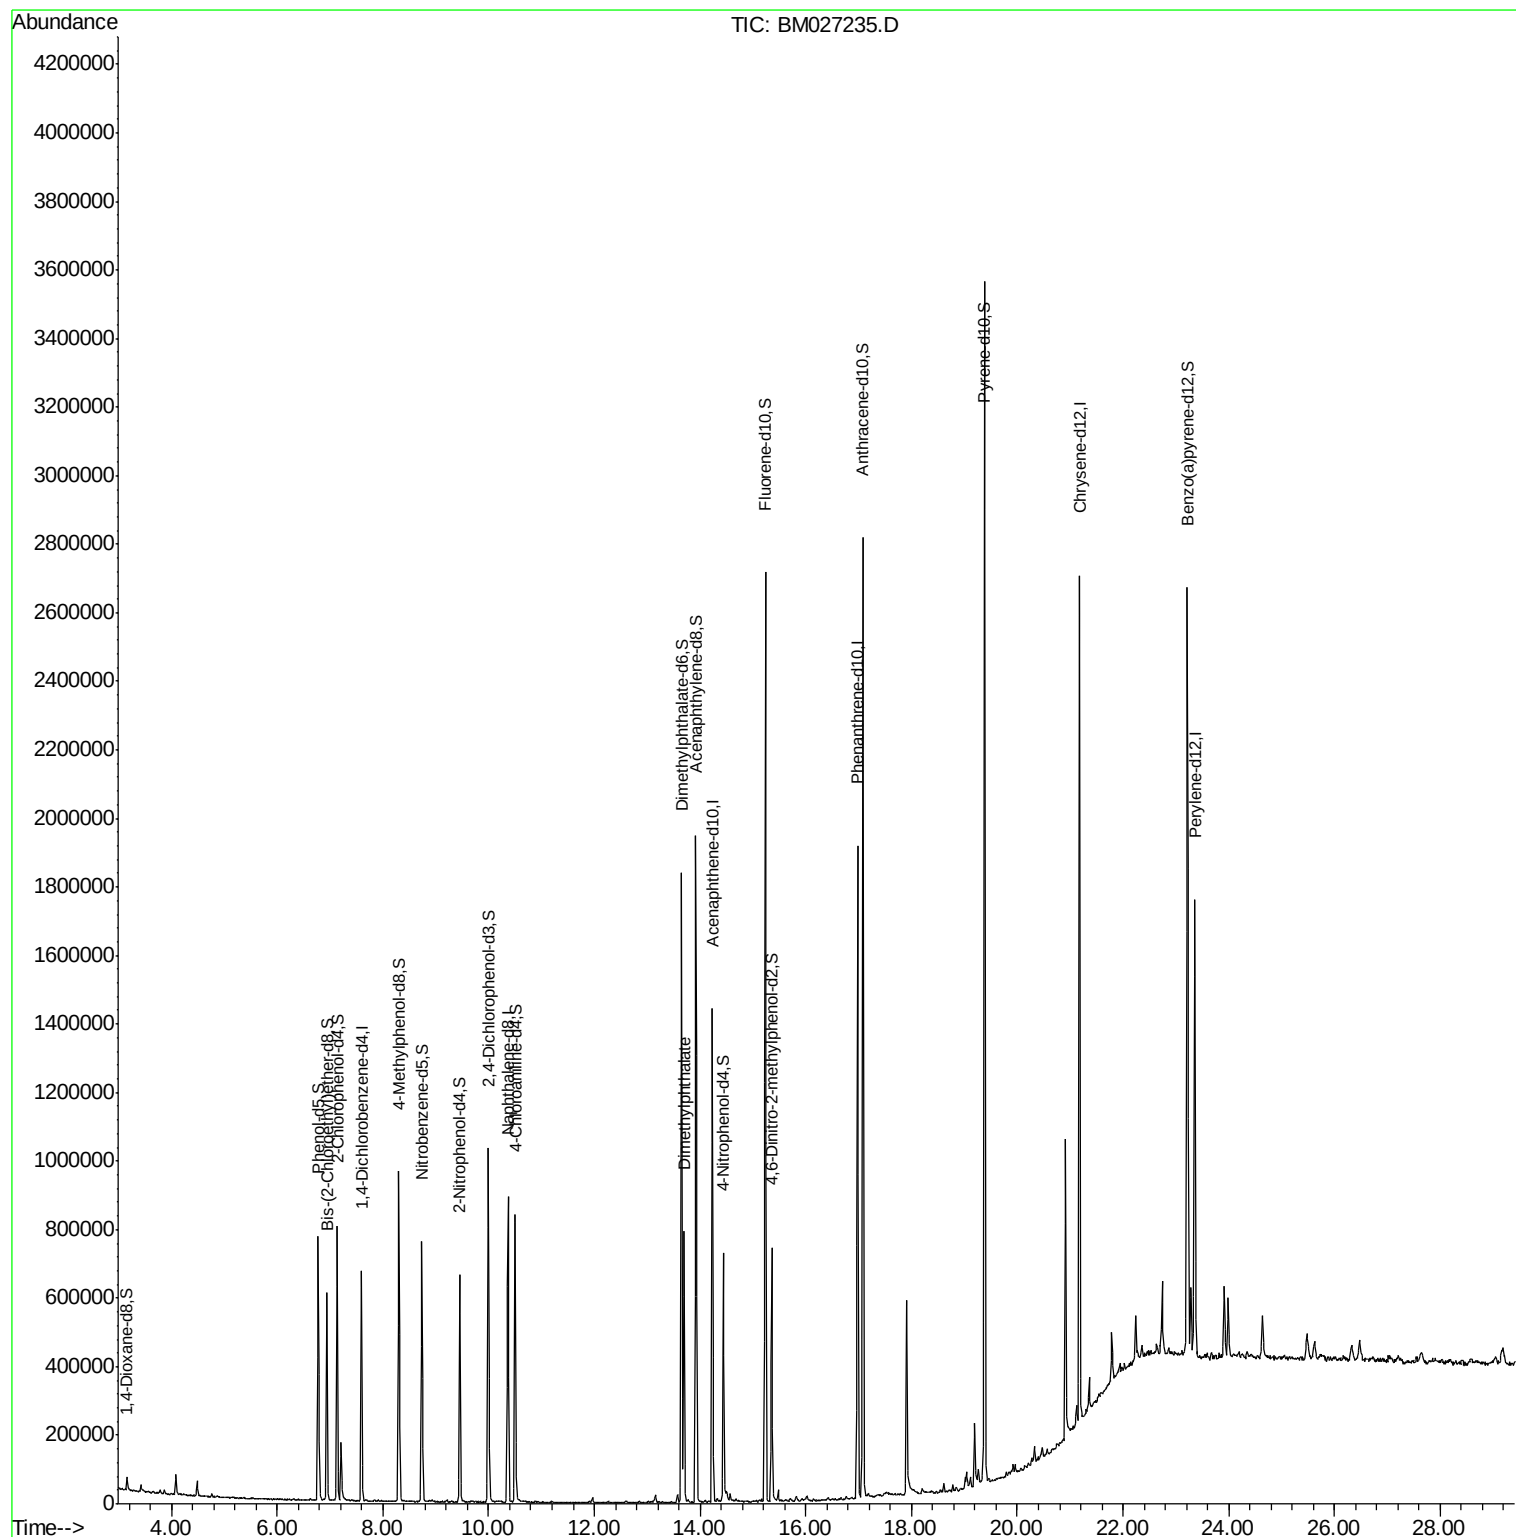

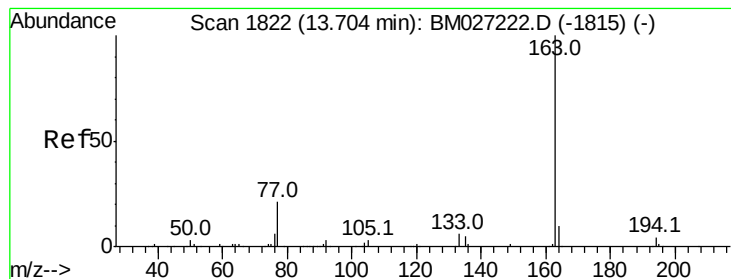

#45

Dimethylphthalate

Concen: 11.398 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM027235.D

Acq: 26 Aug 2020 05:13

Instrument :

BNA_M

ClientSampleId :

DBFQ6


Tot Ion:163 Resp: 454237

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.4 8.2 12.2

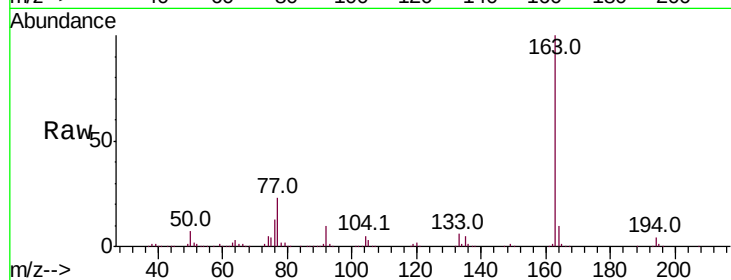

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

