

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
 Data File : BM027238.D
 Acq On : 26 Aug 2020 07:37
 Operator : JU/CG
 Sample : PB131069BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK69

Quant Time: Aug 26 08:26:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 26 08:25:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	191791	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	798051	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	573671	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	1317296	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	1395102	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	1162453	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	24863	7.34	ng/uL	0.00
5) Phenol-d5	6.78	99	469907	30.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	318387	31.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	372389	31.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	382471	30.63	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	188710	29.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	222706	30.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	418851	27.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	525872	32.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	1455310	31.98	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	1680375	31.22	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	224349	29.22	ng/ul	0.00
58) Fluorene-d10	15.23	176	1203532	30.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	219420	25.53	ng/ul	0.00
71) Anthracene-d10	17.08	188	1982486	31.71	ng/ul	0.00
79) Pyrene-d10	19.38	212	2281727	28.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	2069510	31.93	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.30	70	13424	1.115	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
Data File : BM027238.D
Acq On : 26 Aug 2020 07:37
Operator : JU/CG
Sample : PB131069BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK69

Quant Time: Aug 26 08:26:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 26 08:25:09 2020
Response via : Initial Calibration

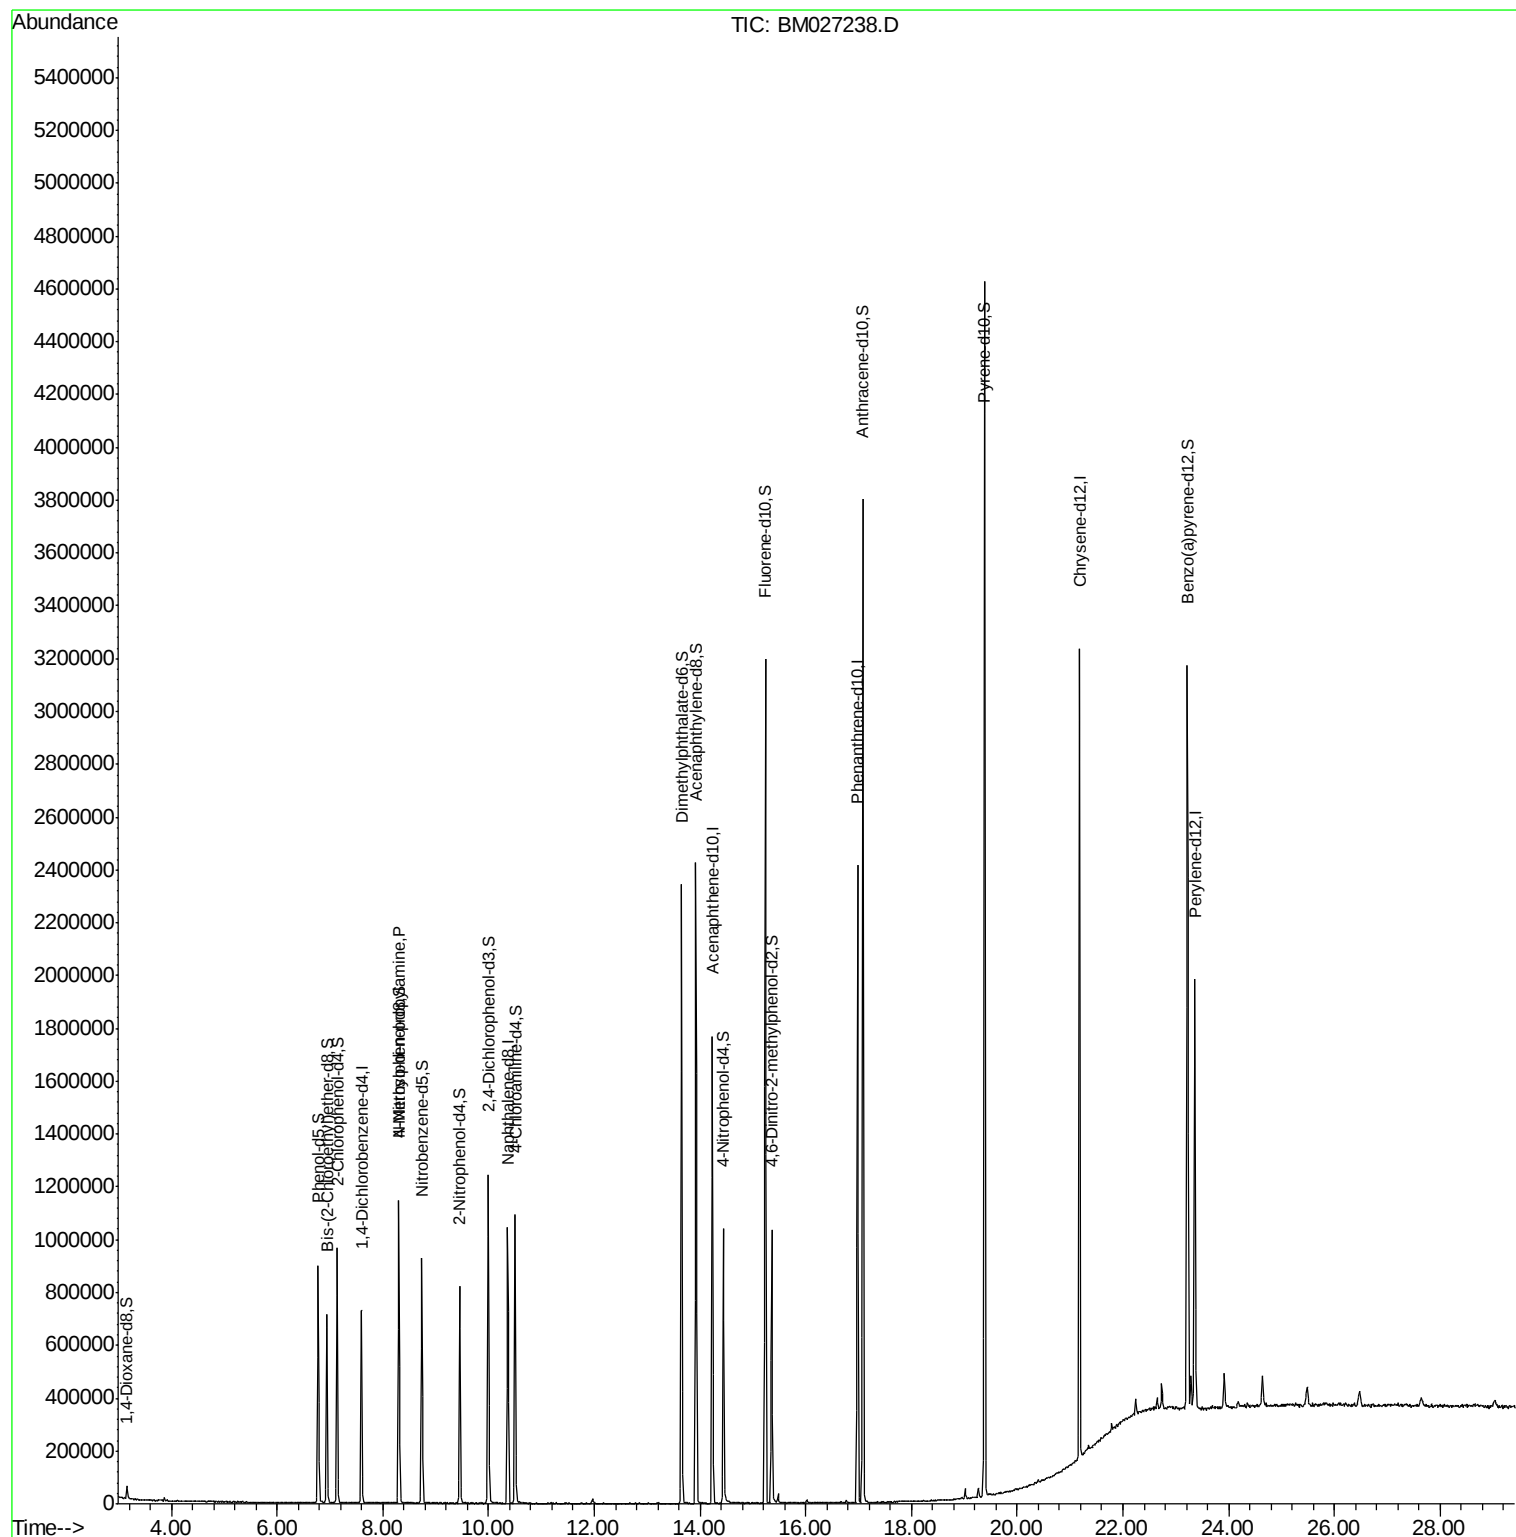

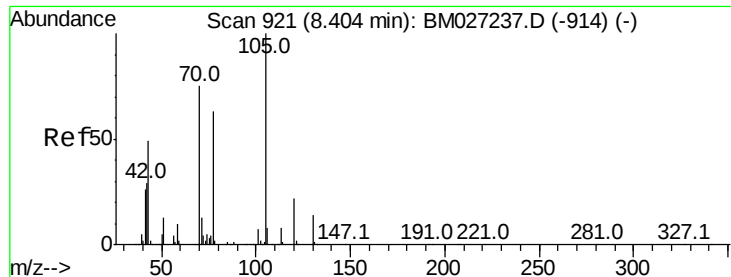

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.115 ng/ul
 RT: 8.30 min Scan# 904
 Delta R.T. -0.10 min
 Lab File: BM027238.D
 Acq: 26 Aug 2020 07:37

Instrument :
 BNA_M
 ClientSampleId :
 SBLK69

Tot Ion:	70	Resp:	13424
Ion	Ratio	Lower	Upper
70	100		
42	231.9	30.9	46.3#
101	0.0	7.4	11.2#
130	0.0	14.8	22.2#

