

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
 Data File : BM027249.D
 Acq On : 26 Aug 2020 15:24
 Operator : JU/CG
 Sample : L3613-13
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBFR2

Quant Time: Aug 26 15:55:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 25 15:35:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	182367	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.36	136	741358	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	510351	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.98	188	1147725	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	1214728	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	1005788	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	19643	6.10	ng/uL	0.00
5) Phenol-d5	6.78	99	407919	27.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	287489	30.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	327902	28.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	281858	23.74	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	169972	28.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	193656	28.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	357229	25.56	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.50	131	417376	27.72	ng/ul	-0.01
44) Dimethylphthalate-d6	13.65	166	1181873	29.19	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	1331042	27.80	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.44	143	172532	25.26	ng/ul	-0.01
58) Fluorene-d10	15.23	176	1002371	28.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	169395	22.62	ng/ul	-0.01
71) Anthracene-d10	17.08	188	1493470	27.42	ng/ul	0.00
79) Pyrene-d10	19.38	212	1802811	25.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	1618220	28.86	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	239646	5.702	ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082520\
Data File : BM027249.D
Acq On : 26 Aug 2020 15:24
Operator : JU/CG
Sample : L3613-13
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBFR2

Quant Time: Aug 26 15:55:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 25 15:35:13 2020
Response via : Initial Calibration

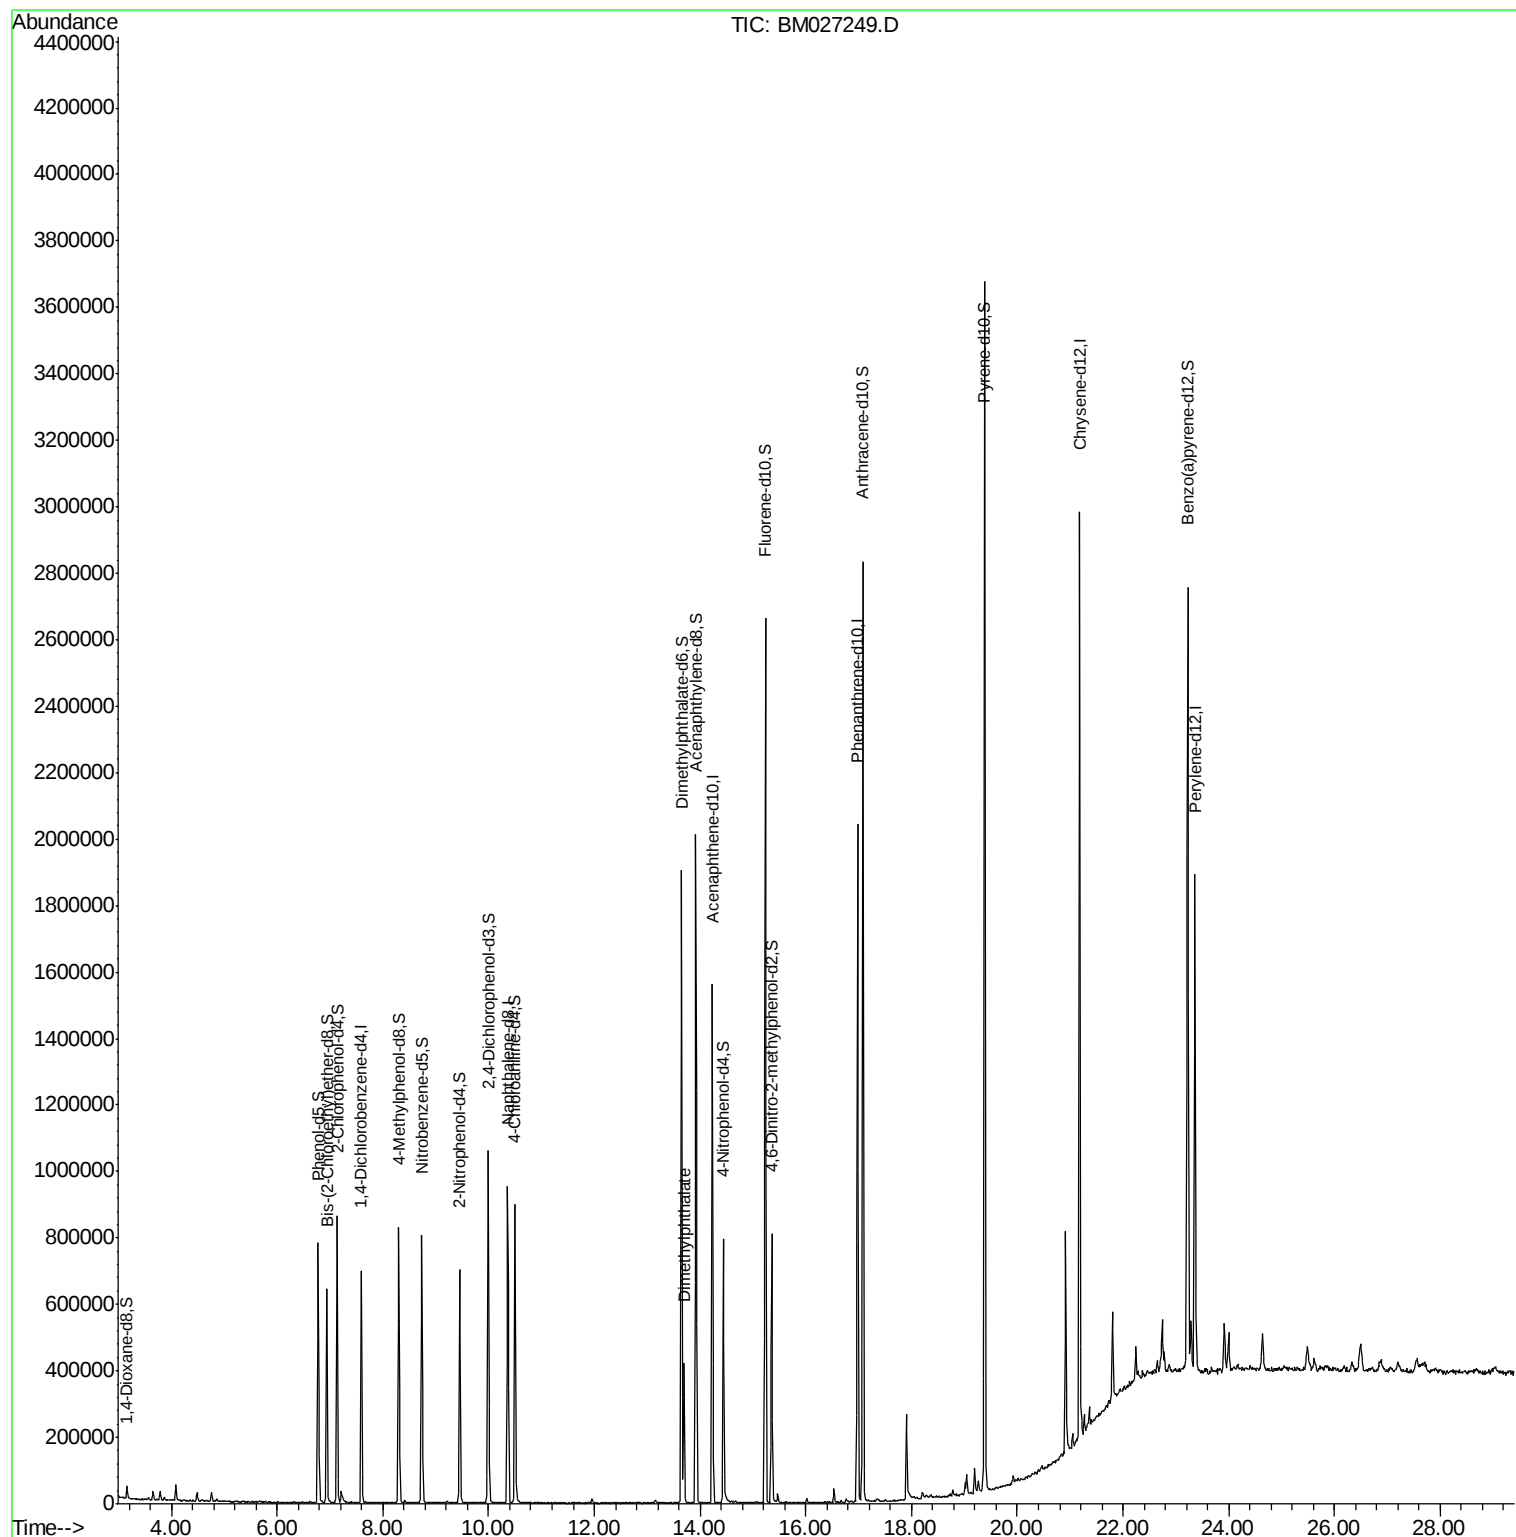

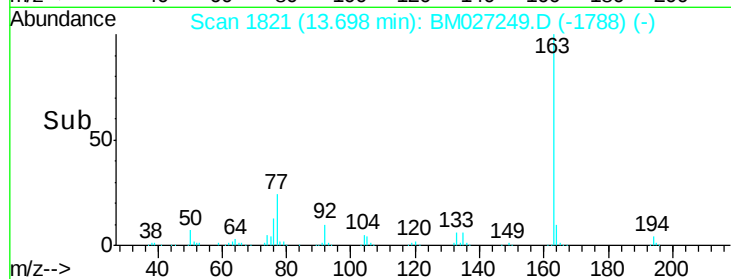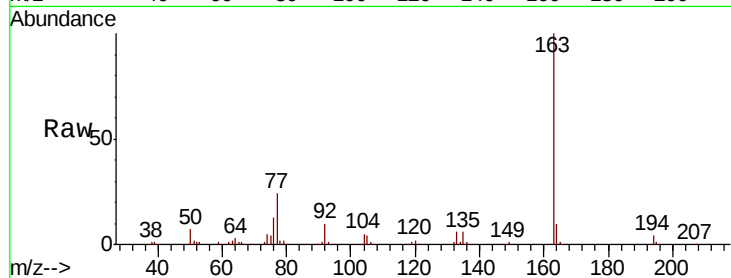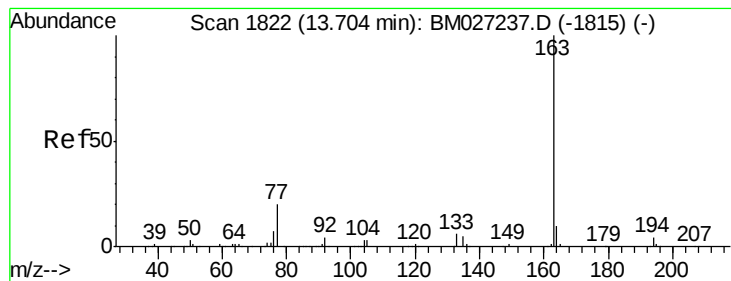

#45

Dimethylphthalate

Concen: 5.702 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM027249.D

Acq: 26 Aug 2020 15:24

Instrument :

BNA_M

ClientSampleId :

DBFR2

Tot Ion:163 Resp: 239646

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.2 8.2 12.2

