
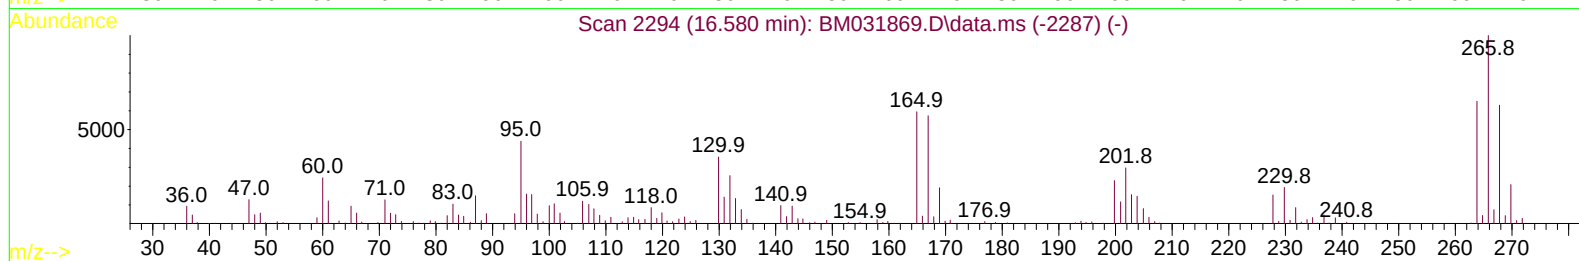
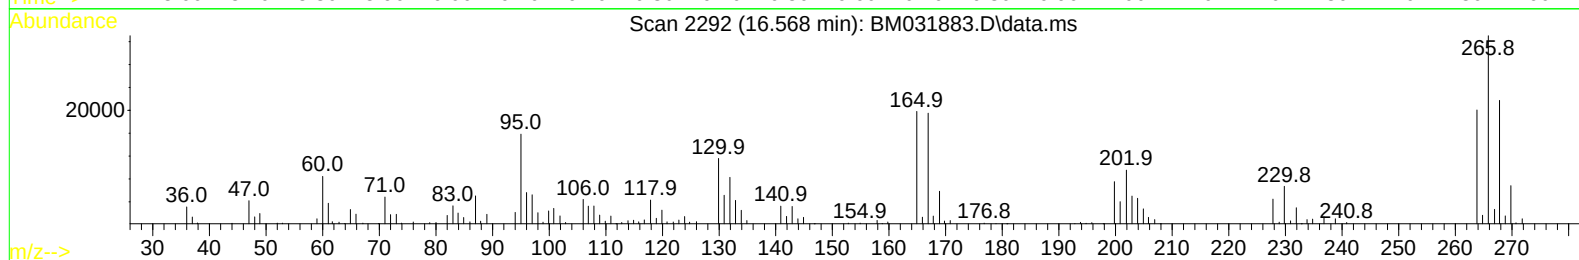


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082521\
Data File : BM031883.D
Acq On : 25 Aug 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 10:49:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 25 10:44:01 2021
Response via : Initial Calibration

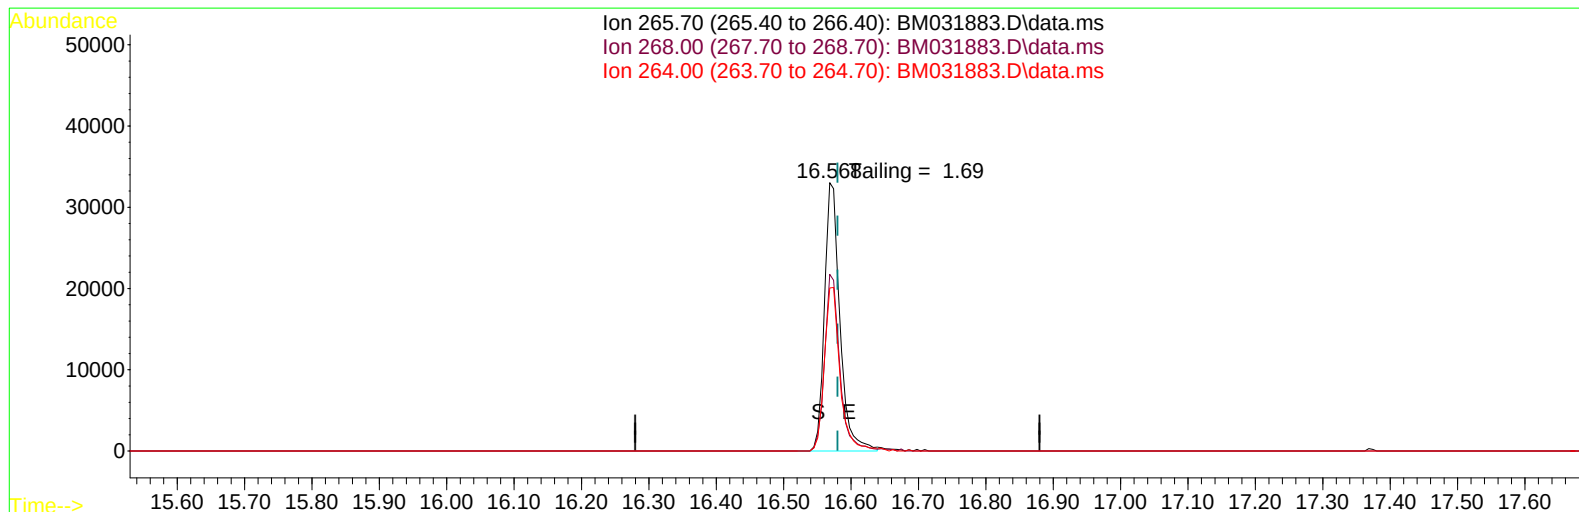

TIC: BM031883.D\data.ms

(70) Pentachlorophenol (C)




16.568min (-0.012) 0.00 ng

response **53141**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.80
264.00	65.10	60.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082521\
 Data File : BM031883.D
 Acq On : 25 Aug 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 10:49:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 25 10:44:01 2021
 Response via : Initial Calibration

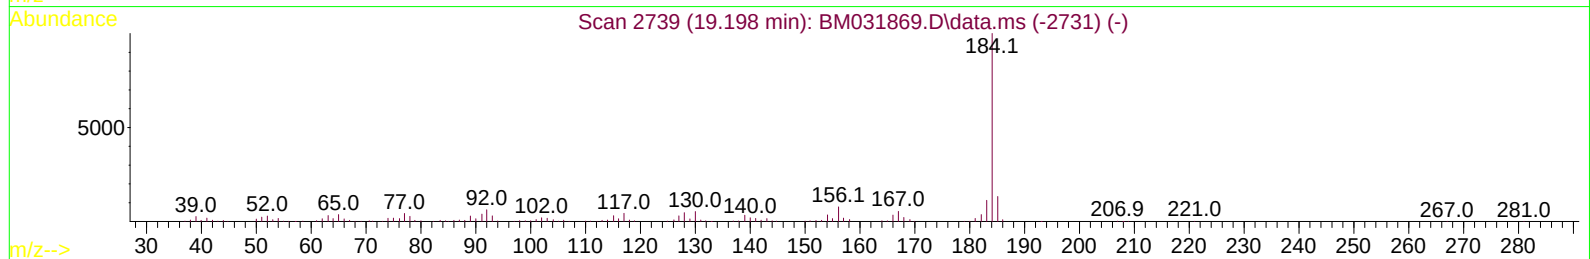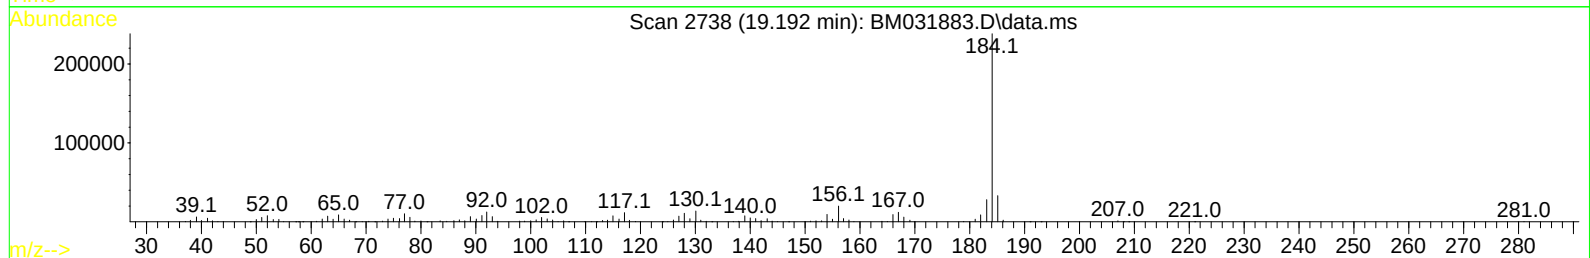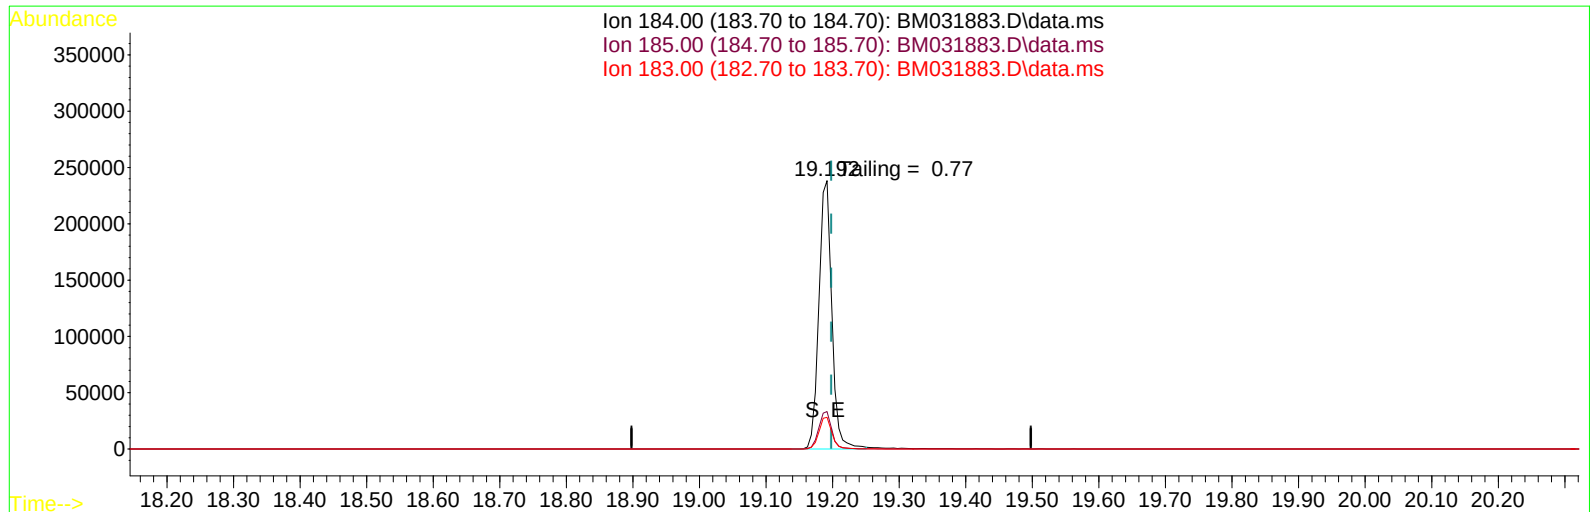

TIC: BM031883.D\data.ms

(77) Benzidine

19.192min (-0.006) 0.00 ng

response 324687

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.96
183.00	11.20	11.81
0.00	0.00	0.00