
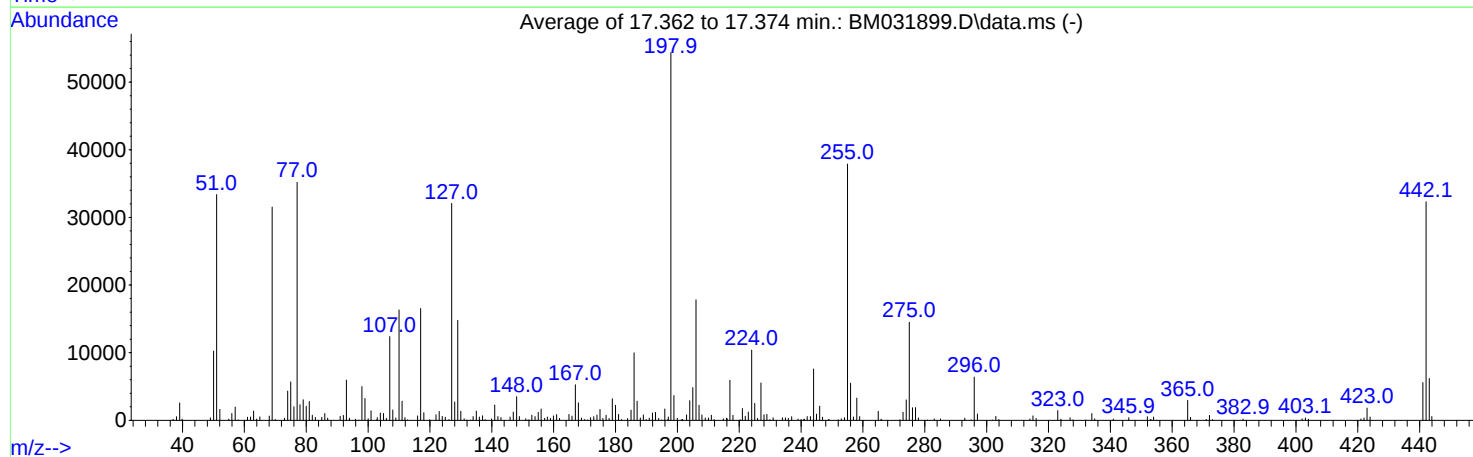


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082521\
 Data File : BM031899.D
 Acq On : 25 Aug 2021 20:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 26 12:15:55 2021

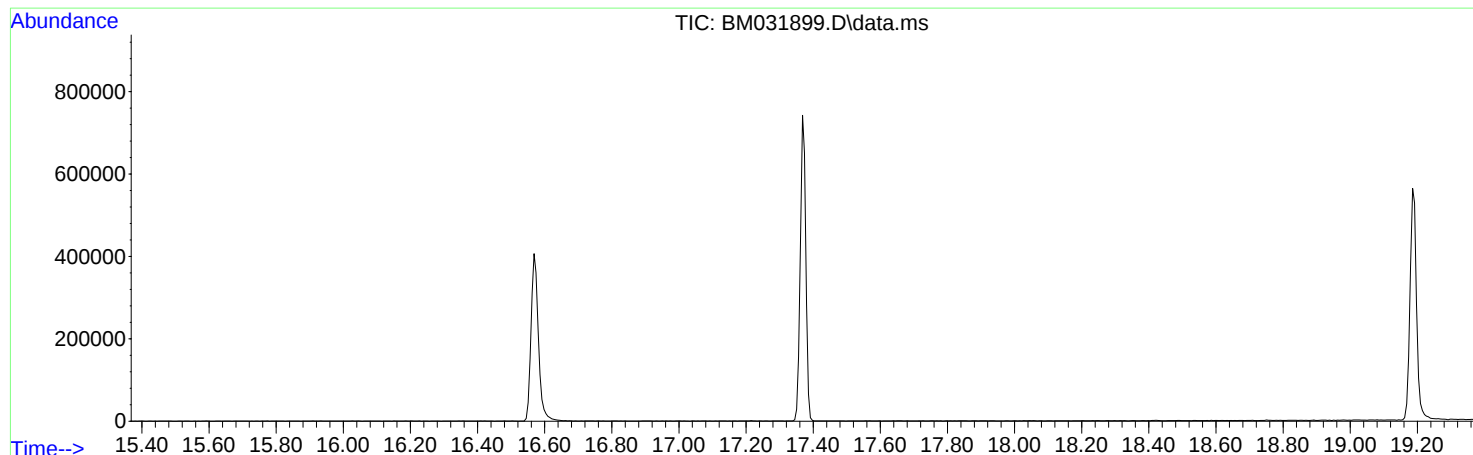




AutoFind: Scans 2427, 2428, 2429; Background Corrected with Scan 2421

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.4	33365	PASS
68	69	0.00	2	2.0	642	PASS
69	198	0.00	100	58.0	31520	PASS
70	69	0.00	2	0.4	138	PASS
127	198	10	80	59.0	32061	PASS
197	198	0.00	2	0.9	492	PASS
198	198	100	100	100.0	54376	PASS
199	198	5	9	6.8	3679	PASS
275	198	10	60	26.7	14498	PASS
365	198	1	100	5.4	2947	PASS
441	198	0.01	100	10.3	5579	PASS
442	442	50	100	100.0	32320	PASS
443	442	15	24	19.2	6201	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082521\
Data File : BM031899.D
Acq On : 25 Aug 2021 20:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 26 04:16:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 25 14:16:52 2021
Response via : Initial Calibration

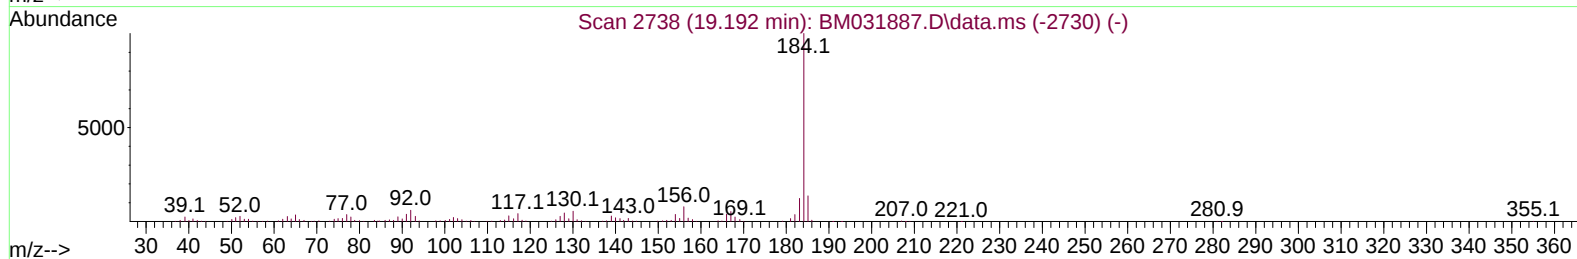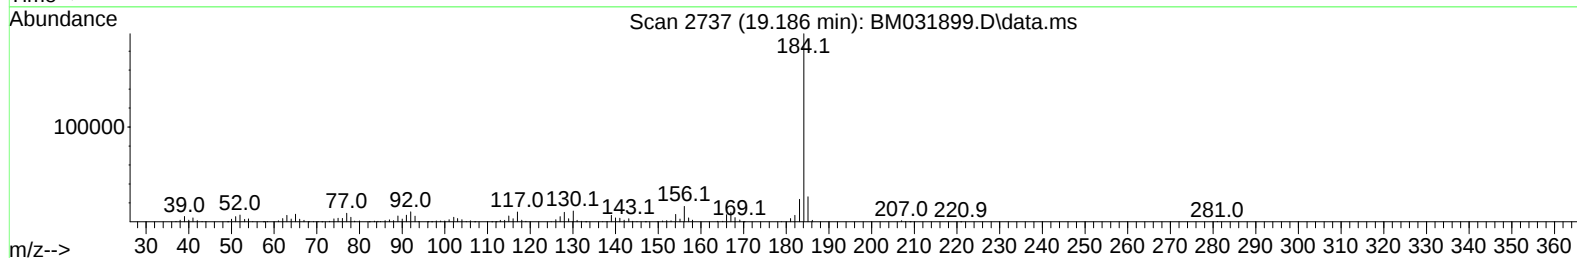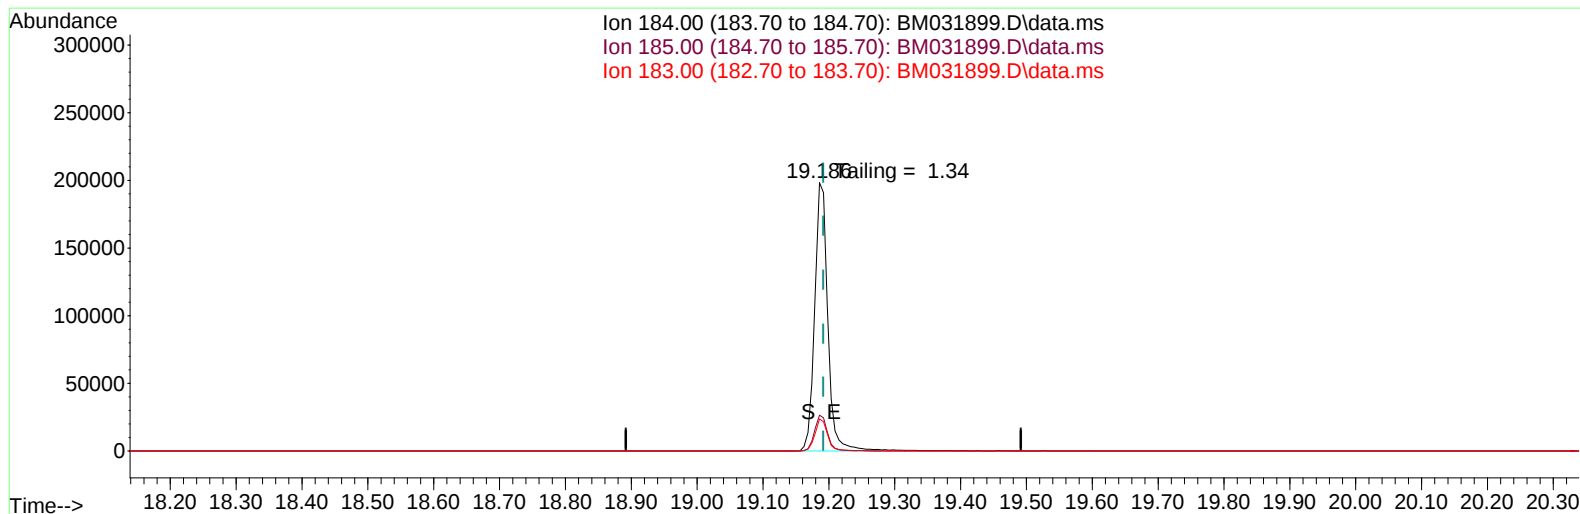

TIC: BM031899.D\data.ms

(77) Benzidine

19.186min (-0.006) 0.00 ng




response 275376

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.38
183.00	11.20	11.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082521\
Data File : BM031899.D
Acq On : 25 Aug 2021 20:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 26 04:16:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 25 14:16:52 2021
Response via : Initial Calibration

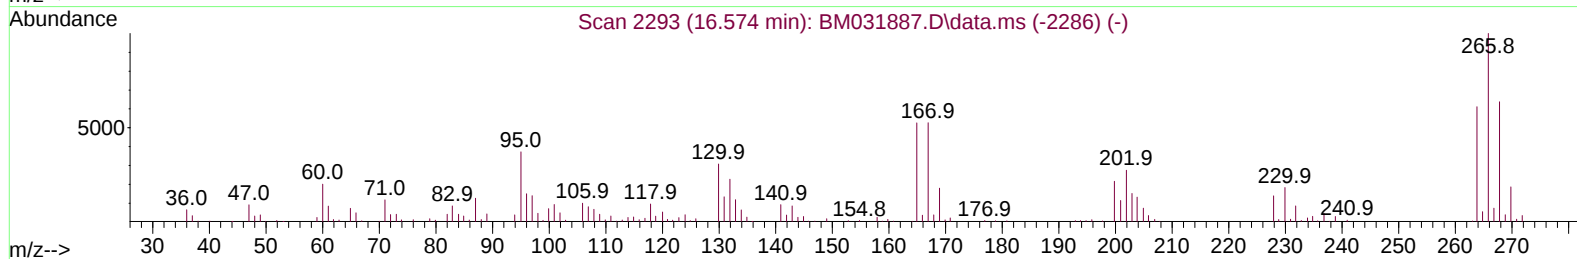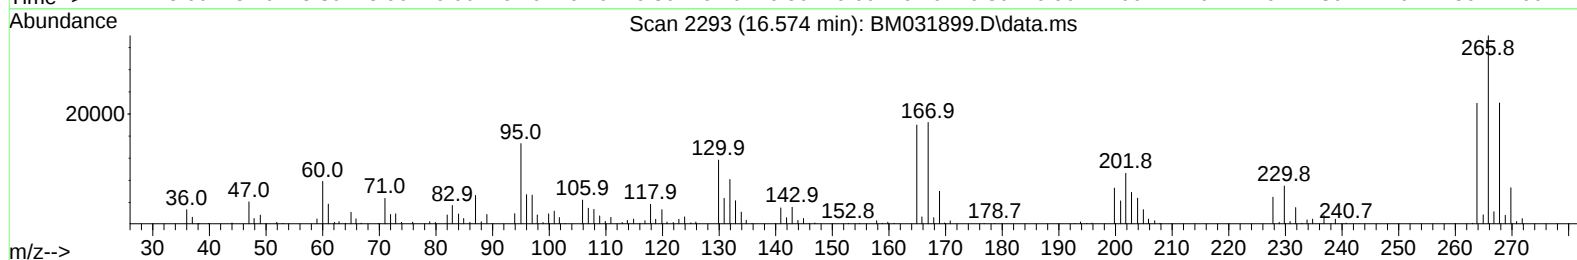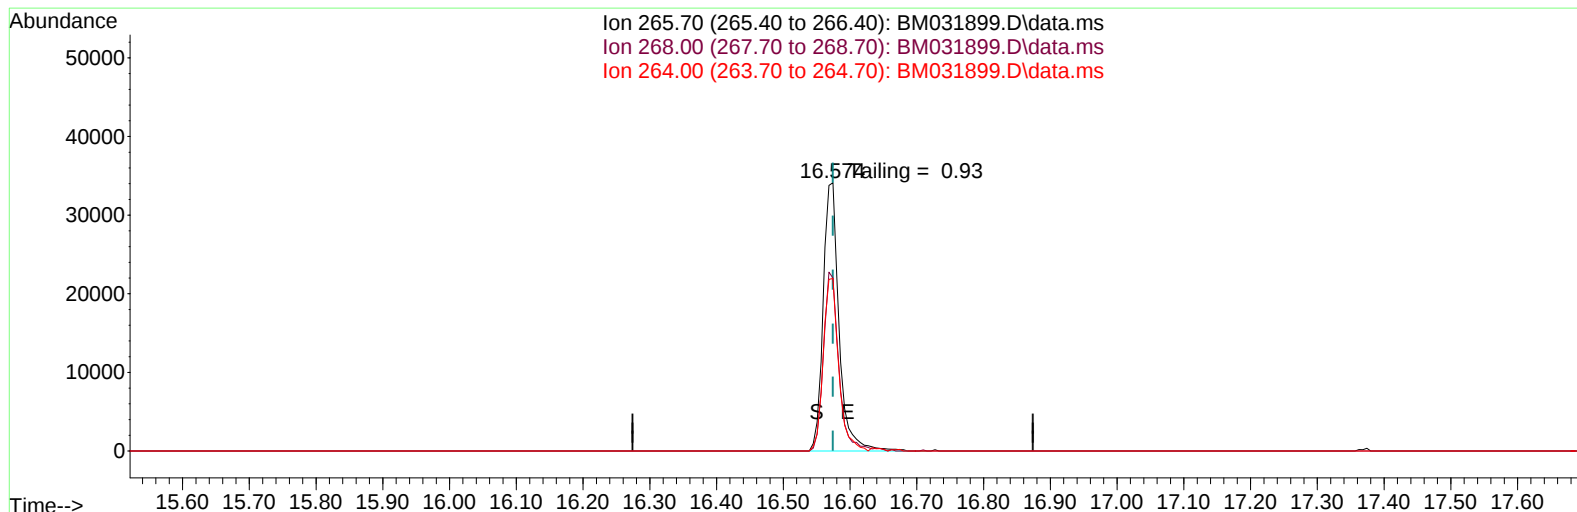

TIC: BM031899.D\data.ms

(70) Pentachlorophenol (C)

16.574min (+ 0.000) 0.00 ng

response 56584

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.42
264.00	65.10	64.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_M	<u>BM031899.D</u>
Compound Name	Response	Retention Time
DDT	160548	20.415
DDD	2102	19.98
DDE	141	19.468
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2243	162791	1.38

Instrument :
BNA_M
ClientSampleId :
DFTPP