
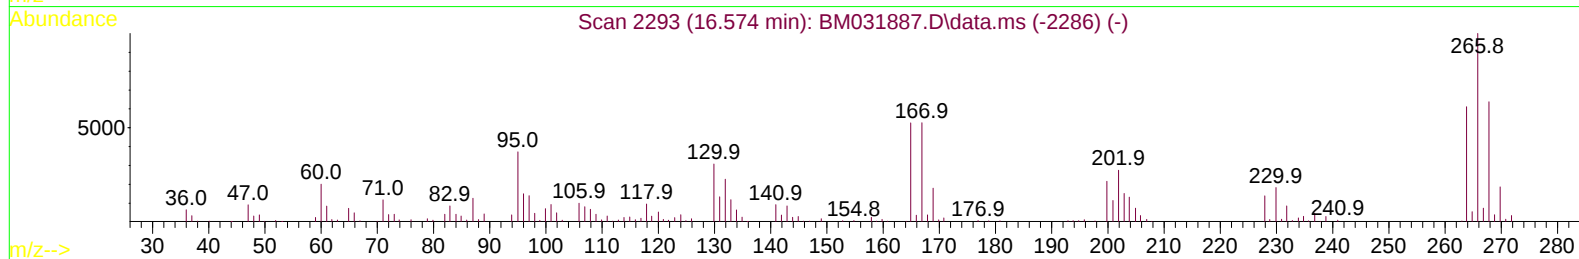
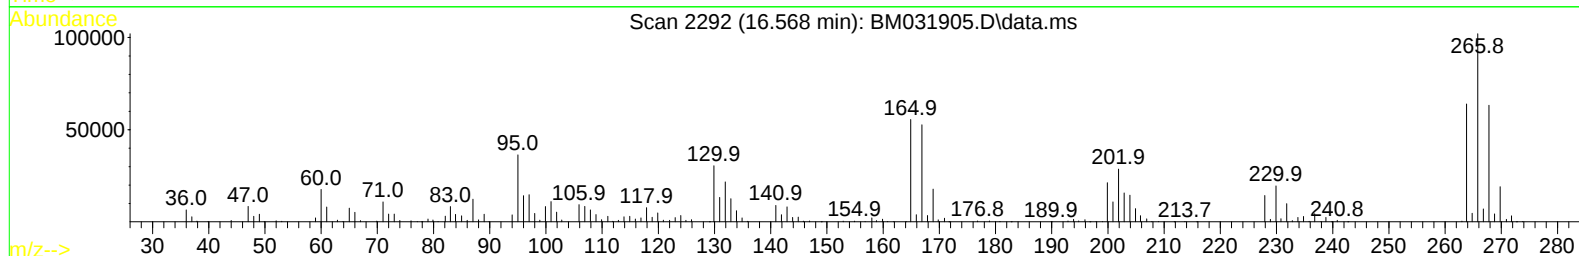


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031905.D
 Acq On : 26 Aug 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 11:04:20 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 10:59:02 2021
 Response via : Initial Calibration

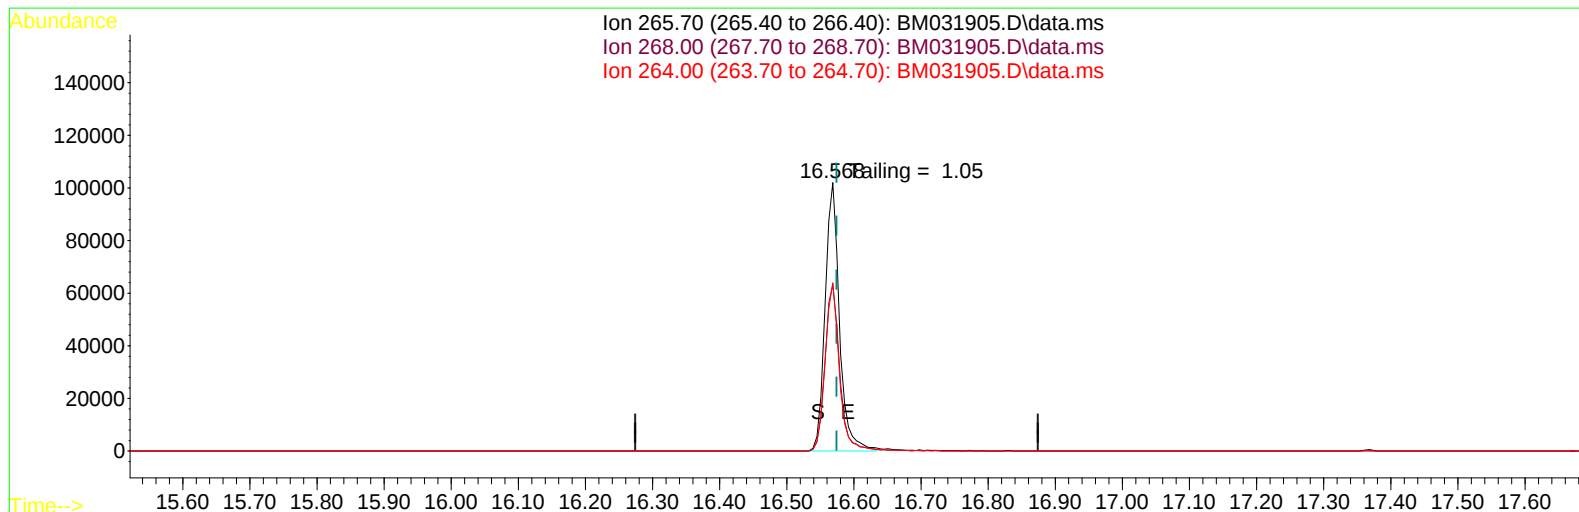

TIC: BM031905.D\data.ms

(70) Pentachlorophenol (C)




16.568min (-0.006) 0.00 ng

response 152869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.03
264.00	65.10	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031905.D
 Acq On : 26 Aug 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 11:04:20 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 10:59:02 2021
 Response via : Initial Calibration

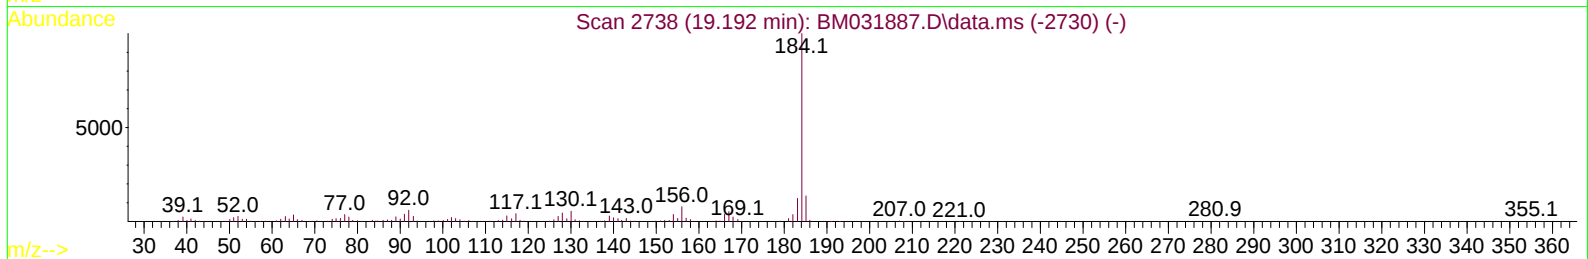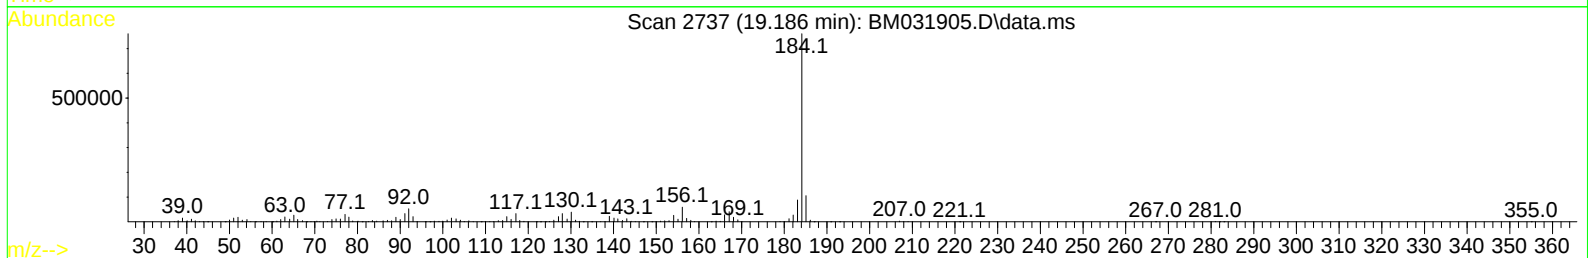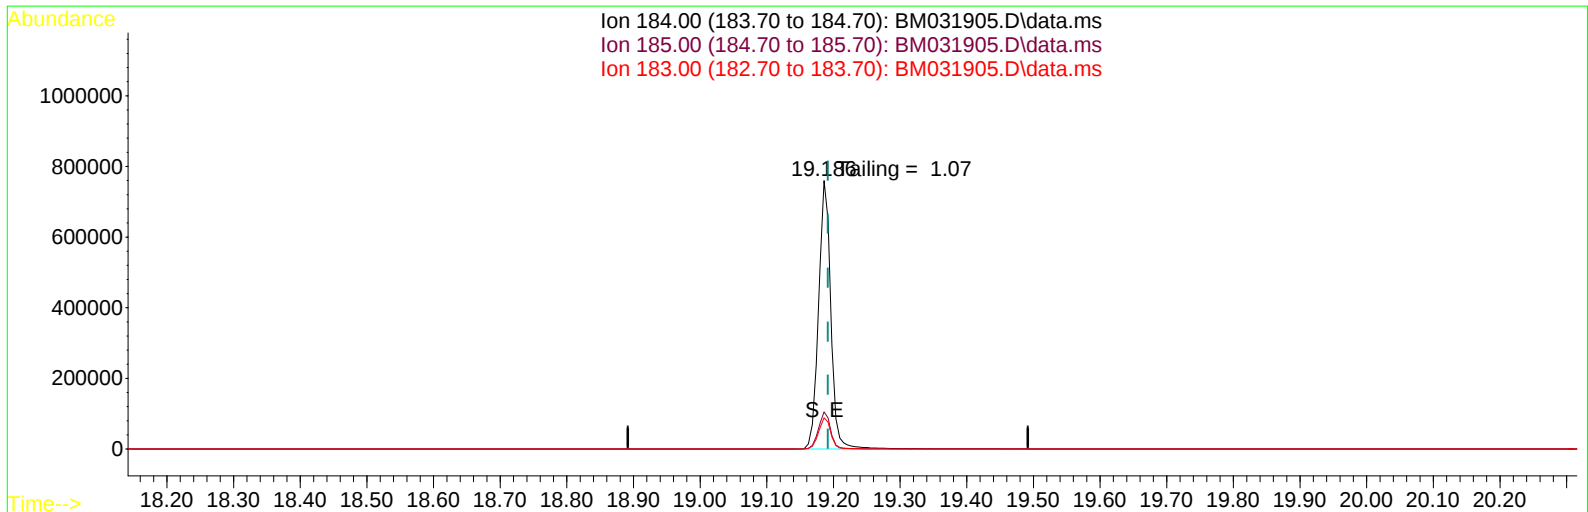

TIC: BM031905.D\data.ms

(77) Benzidine

19.186min (-0.006) 0.00 ng

response 971485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.85
183.00	11.20	11.62
0.00	0.00	0.00