

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031919.D
 Acq On : 26 Aug 2021 18:21
 Operator : CG/JU
 Sample : PB138117BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138117BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	346	352	363	rBV	1592858	2243861	74.49%	13.101%
2	6.716	609	617	638	rBV	1463648	2324344	77.16%	13.571%
3	7.516	746	753	763	rBV	260330	405022	13.44%	2.365%
4	8.669	942	949	968	rBV	858873	1437455	47.72%	8.393%
5	10.275	1215	1222	1236	rBV	310479	544527	18.08%	3.179%
6	12.769	1639	1646	1661	rBV	2070885	3012465	100.00%	17.589%
7	14.157	1876	1882	1901	rBV	433891	661895	21.97%	3.865%
8	15.657	2131	2137	2160	rBV	1341632	2008556	66.67%	11.727%
9	16.915	2344	2351	2365	rBV	432159	670855	22.27%	3.917%
10	19.562	2795	2801	2811	rBV	2361155	2903620	96.39%	16.953%
11	21.115	3060	3065	3074	rBV	341116	475832	15.80%	2.778%
12	23.256	3423	3429	3441	rBV2	228643	438781	14.57%	2.562%




Sum of corrected areas: 17127213

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031919.D
Acq On : 26 Aug 2021 18:21
Operator : CG/JU
Sample : PB138117BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138117BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

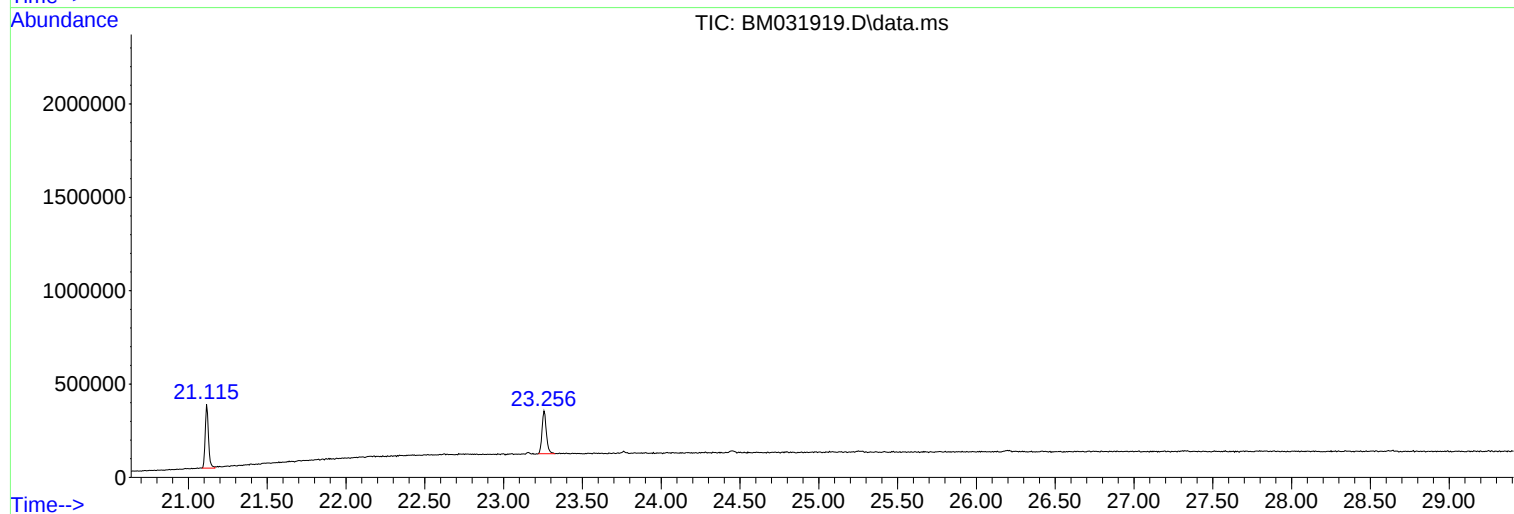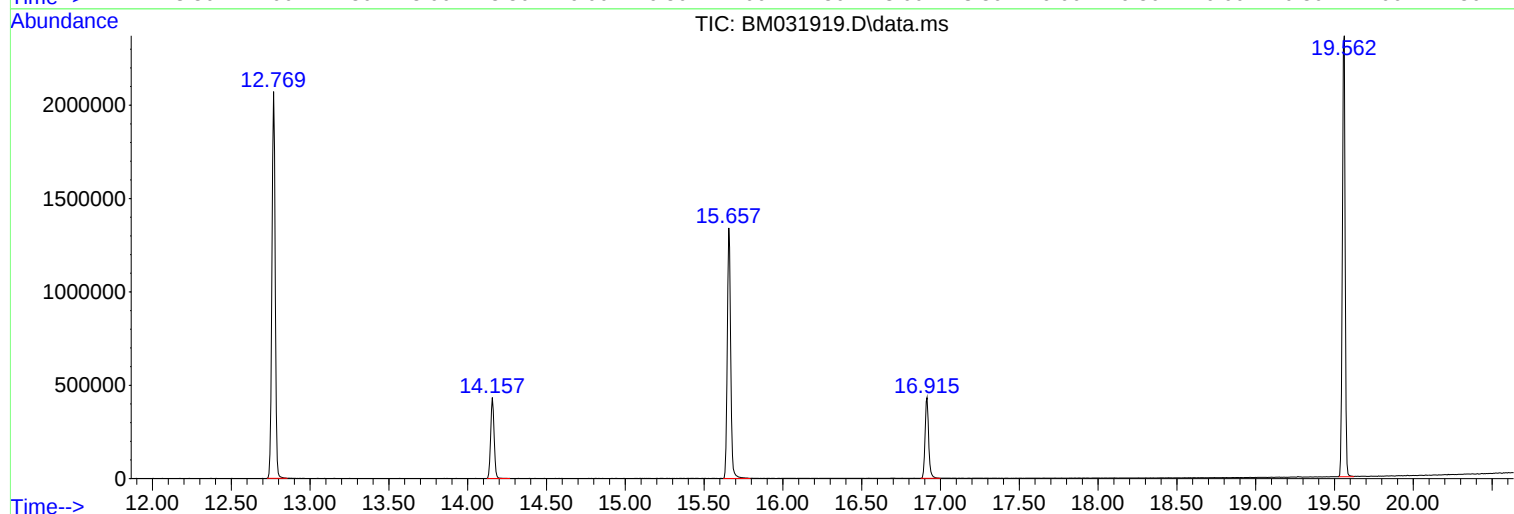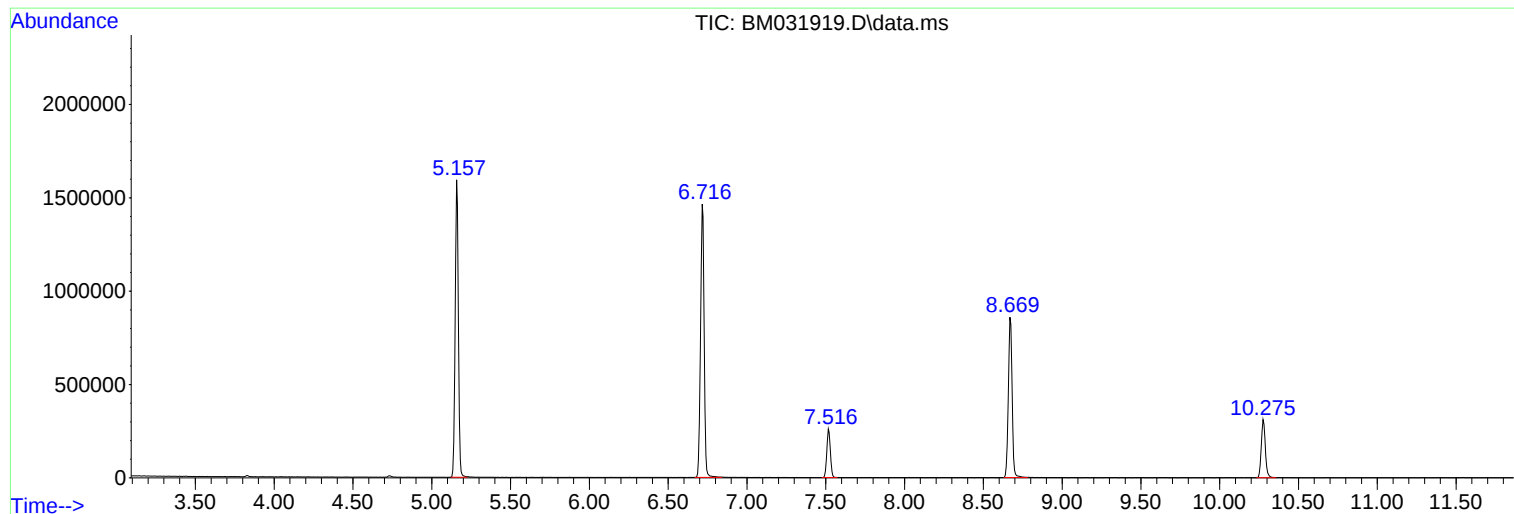

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031919.D
Acq On : 26 Aug 2021 18:21
Operator : CG/JU
Sample : PB138117BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138117BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031919.D
Acq On : 26 Aug 2021 18:21
Operator : CG/JU
Sample : PB138117BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138117BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------