

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031920.D
 Acq On : 26 Aug 2021 18:59
 Operator : CG/JU
 Sample : PB138118BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138118BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	346	352	364	rBV	1553666	2131724	56.22%	11.860%
2	6.716	610	617	640	rBV	1397350	2228578	58.77%	12.399%
3	7.516	747	753	761	rBV	244073	375937	9.91%	2.092%
4	8.669	942	949	968	rBV	823168	1362246	35.93%	7.579%
5	10.275	1215	1222	1241	rBV	295575	512304	13.51%	2.850%
6	12.769	1639	1646	1660	rBV	2032047	2929983	77.27%	16.301%
7	14.157	1875	1882	1890	rBV	422273	646117	17.04%	3.595%
8	15.657	2131	2137	2155	rBV	1463893	2135883	56.33%	11.883%
9	16.909	2344	2350	2364	rBV	458678	725232	19.13%	4.035%
10	19.562	2795	2801	2811	rBV	3206466	3791848	100.00%	21.096%
11	21.115	3060	3065	3074	rBV	437586	622954	16.43%	3.466%
12	23.256	3424	3429	3439	rBV	274603	511557	13.49%	2.846%




Sum of corrected areas: 17974363

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031920.D
Acq On : 26 Aug 2021 18:59
Operator : CG/JU
Sample : PB138118BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

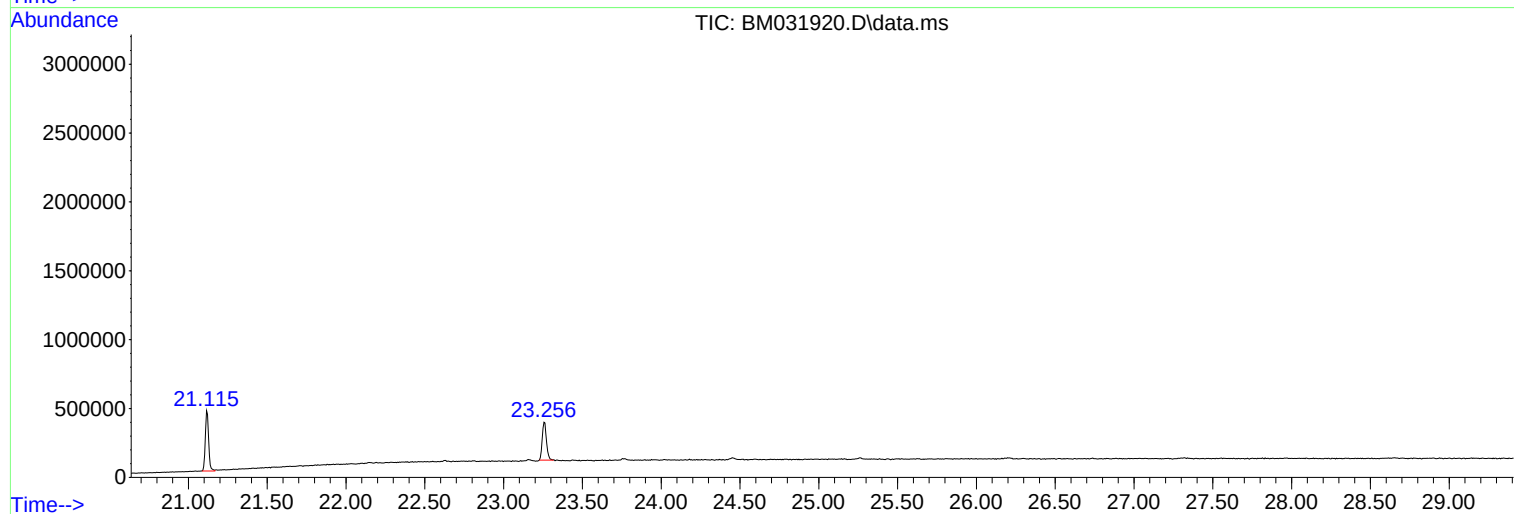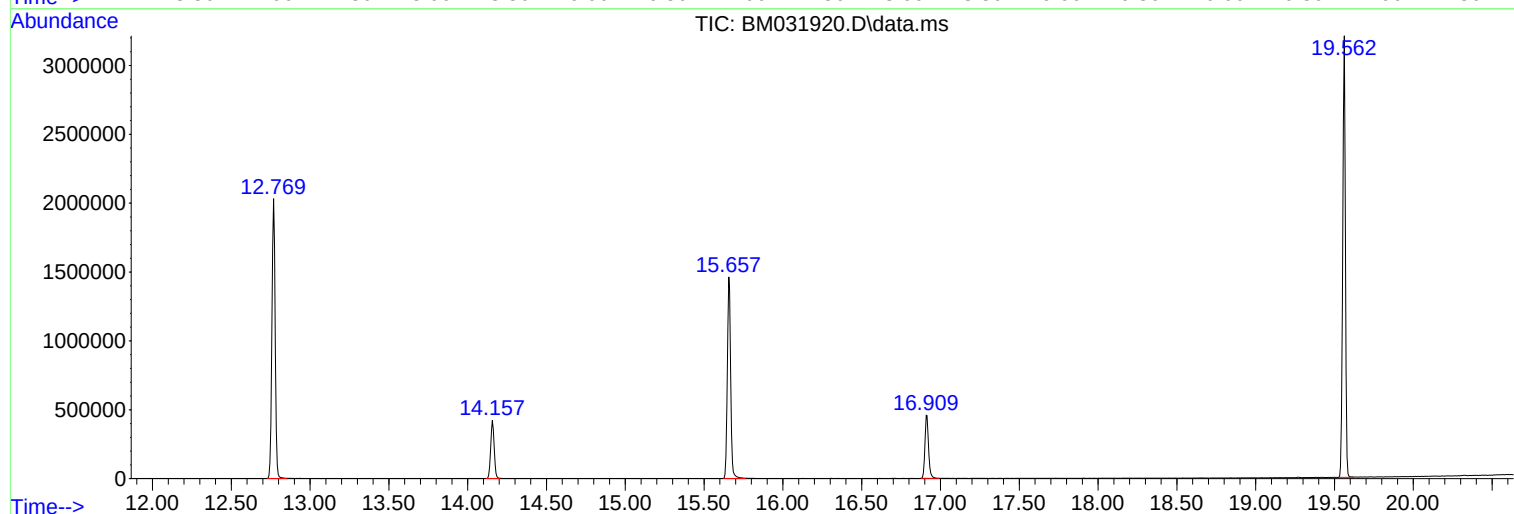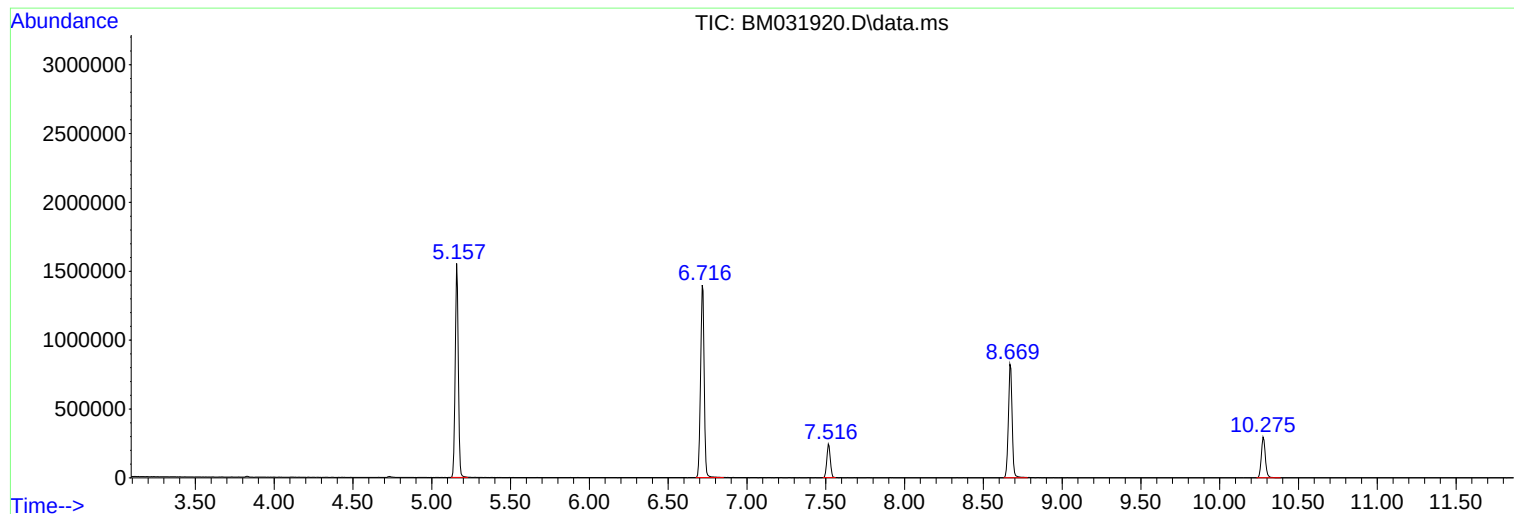

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031920.D
Acq On : 26 Aug 2021 18:59
Operator : CG/JU
Sample : PB138118BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
Data File : BM031920.D
Acq On : 26 Aug 2021 18:59
Operator : CG/JU
Sample : PB138118BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------