
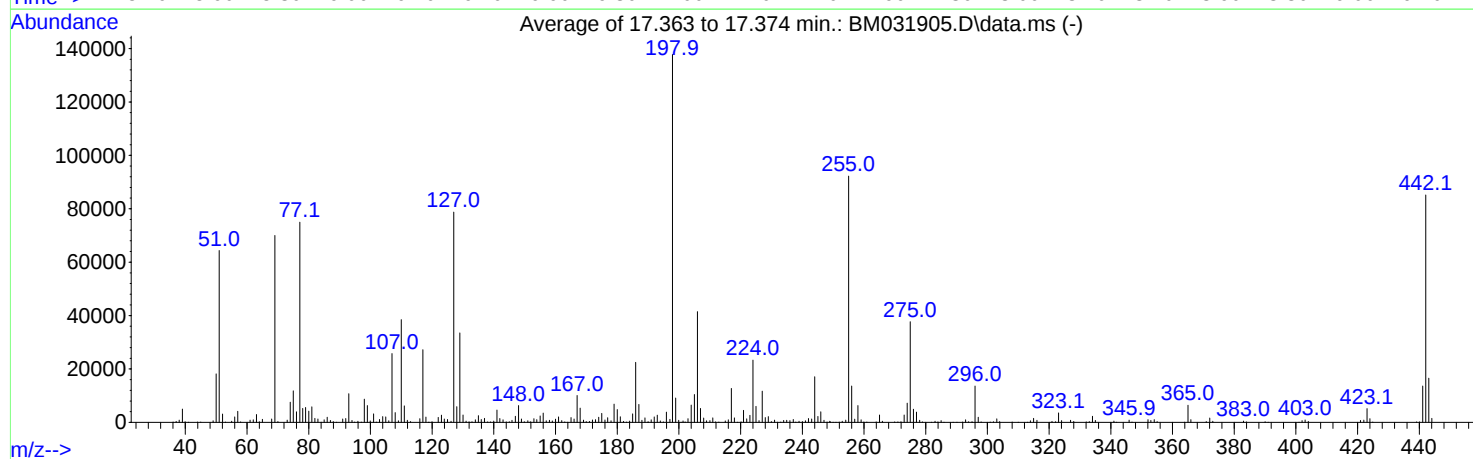


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031905.D
 Acq On : 26 Aug 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 26 14:24:44 2021

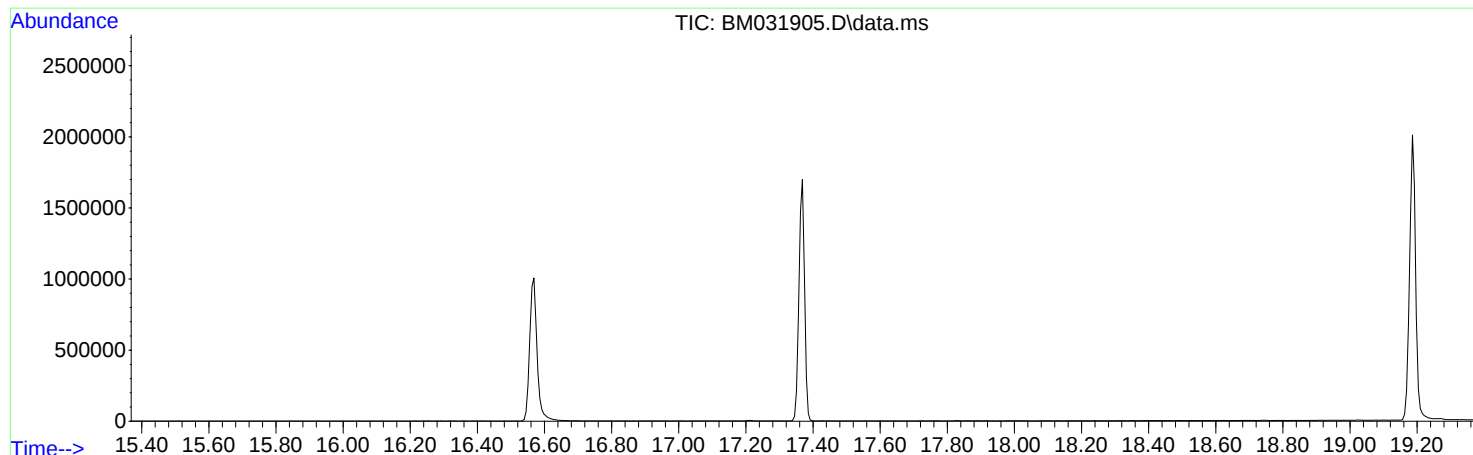




AutoFind: Scans 2427, 2428, 2429; Background Corrected with Scan 2420

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	64355	PASS
68	69	0.00	2	1.8	1245	PASS
69	198	0.00	100	50.8	69997	PASS
70	69	0.00	2	0.5	328	PASS
127	198	10	80	57.1	78741	PASS
197	198	0.00	2	0.8	1139	PASS
198	198	100	100	100.0	137789	PASS
199	198	5	9	6.6	9142	PASS
275	198	10	60	27.4	37733	PASS
365	198	1	100	4.7	6424	PASS
441	198	0.01	100	9.9	13615	PASS
442	442	50	100	100.0	85168	PASS
443	442	15	24	19.4	16545	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031905.D
 Acq On : 26 Aug 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 11:04:20 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 10:59:02 2021
 Response via : Initial Calibration

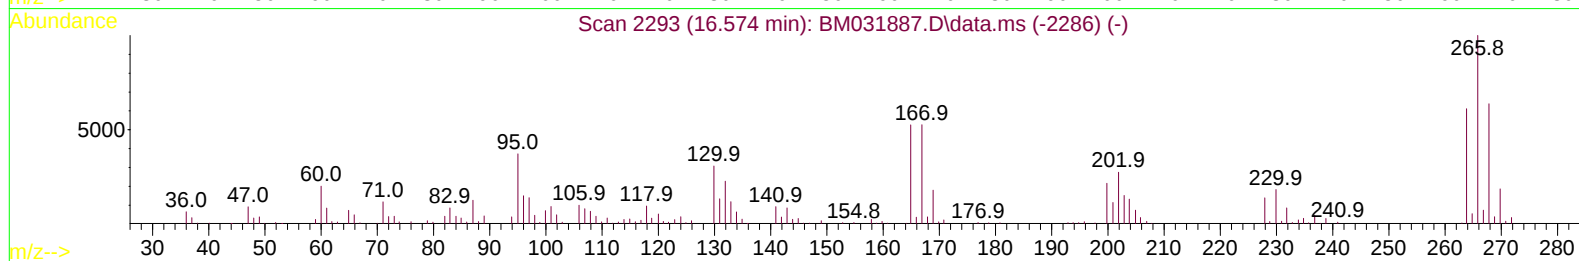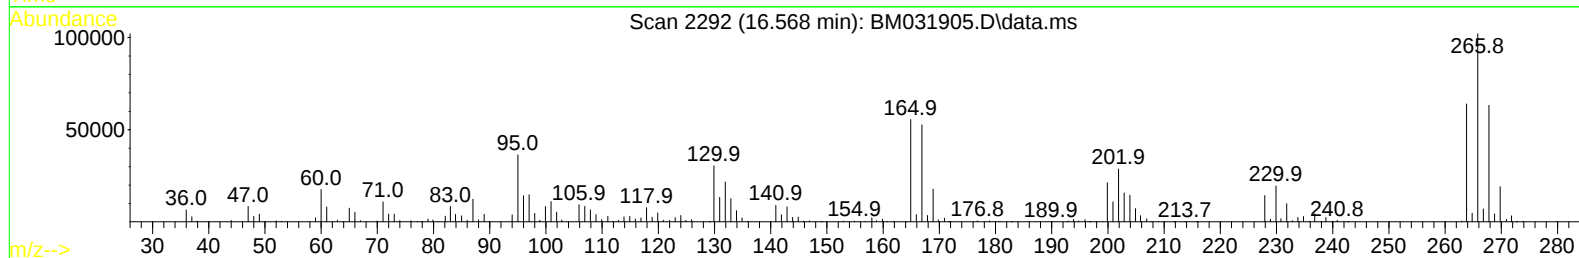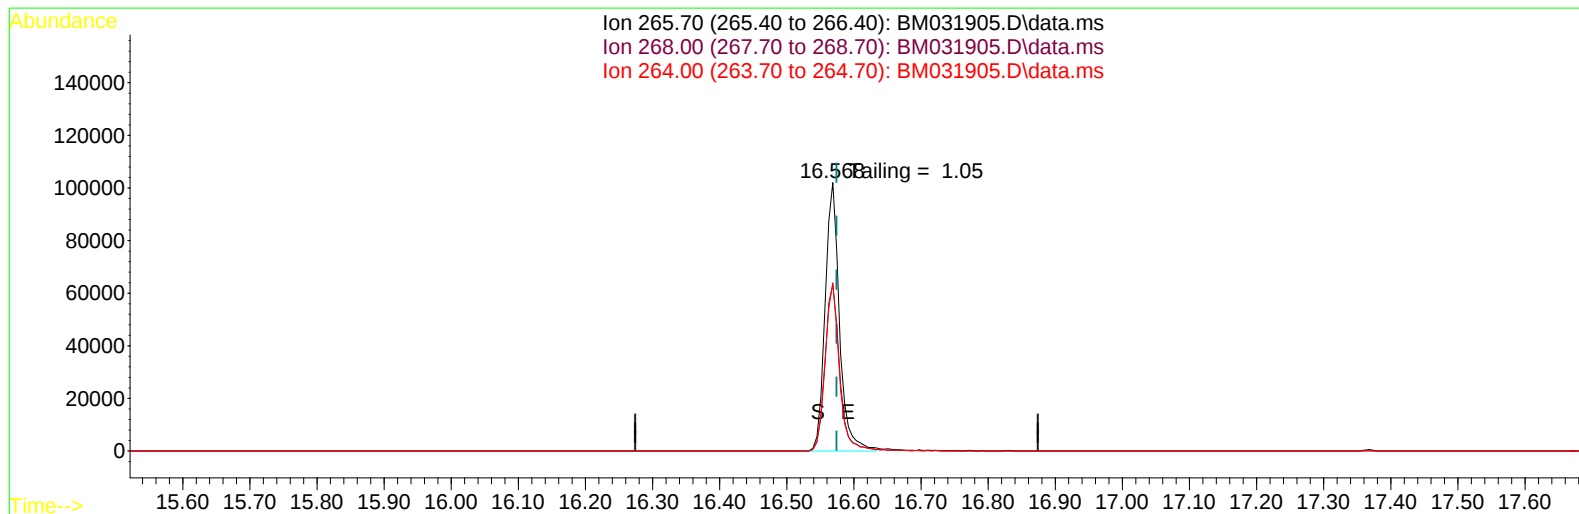

TIC: BM031905.D\data.ms

(70) Pentachlorophenol (C)

16.568min (-0.006) 0.00 ng




response 152869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.03
264.00	65.10	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082621\
 Data File : BM031905.D
 Acq On : 26 Aug 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 11:04:20 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 26 10:59:02 2021
 Response via : Initial Calibration

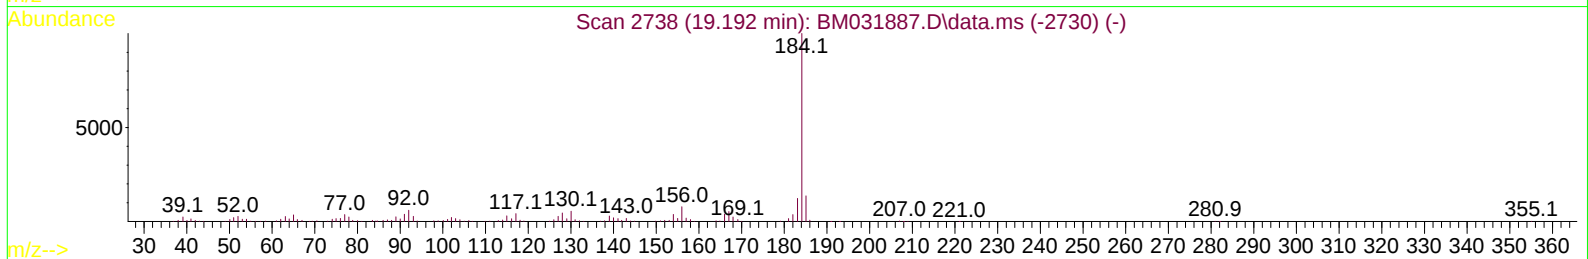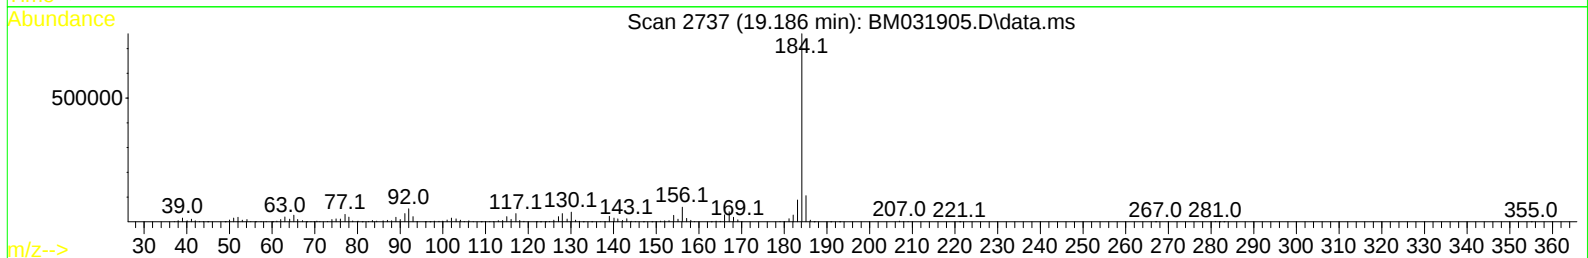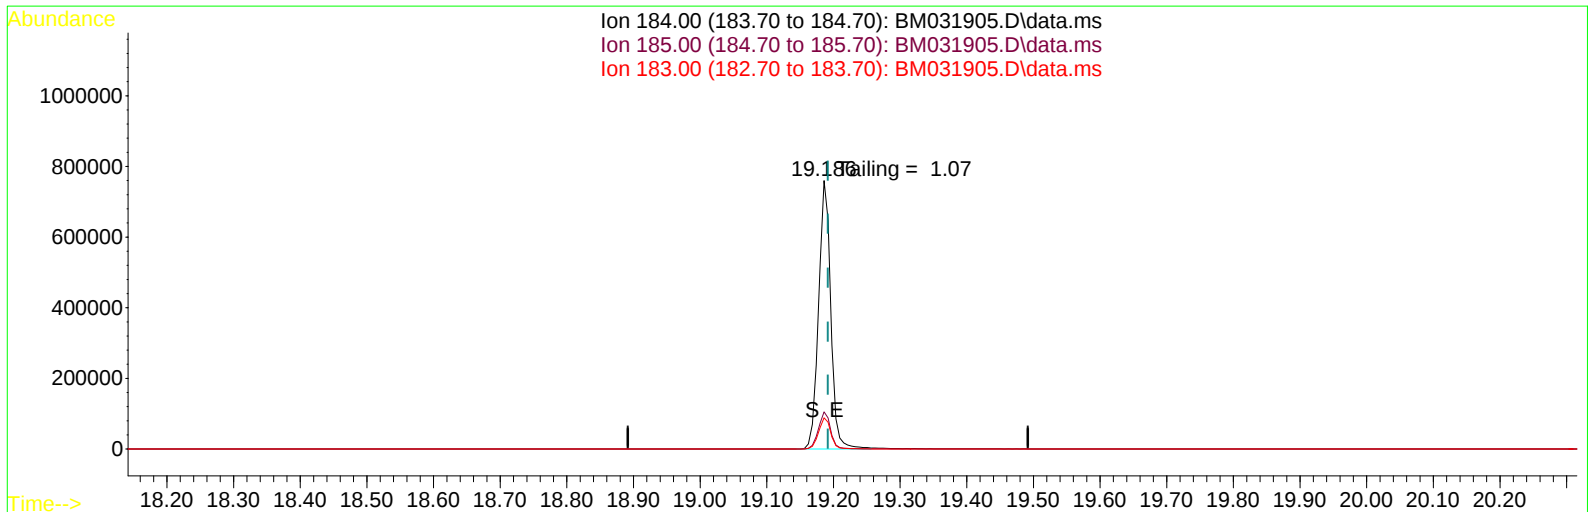

TIC: BM031905.D\data.ms

(77) Benzidine

19.186min (-0.006) 0.00 ng

response 971485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.85
183.00	11.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/26/2021	BNA_M	<u>BM031905.D</u>
Compound Name	Response	Retention Time
DDT	507951	20.41
DDD	4198	19.98
DDE	771	19.46
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4969	512920	0.97