

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082622\
 Data File : BM036427.D
 Acq On : 26 Aug 2022 15:59
 Operator : CG/JU
 Sample : N4349-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN62

Quant Time: Aug 26 23:08:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM082622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 26 14:26:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.791	152	5081	0.400	ng/ul	0.00
4) Naphthalene-d8	10.589	136	20362	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.432	164	12559	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.175	188	27855	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	45055	0.400	ng/ul #	0.00
23) Perylene-d12	23.688	264	30765	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	30991	4.529	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.189	152	8891	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.206	212	27946	0.502	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.239	88	7454	1.154	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082622\
Data File : BM036427.D
Acq On : 26 Aug 2022 15:59
Operator : CG/JU
Sample : N4349-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN62


Quant Time: Aug 26 23:08:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 26 14:26:34 2022
Response via : Initial Calibration

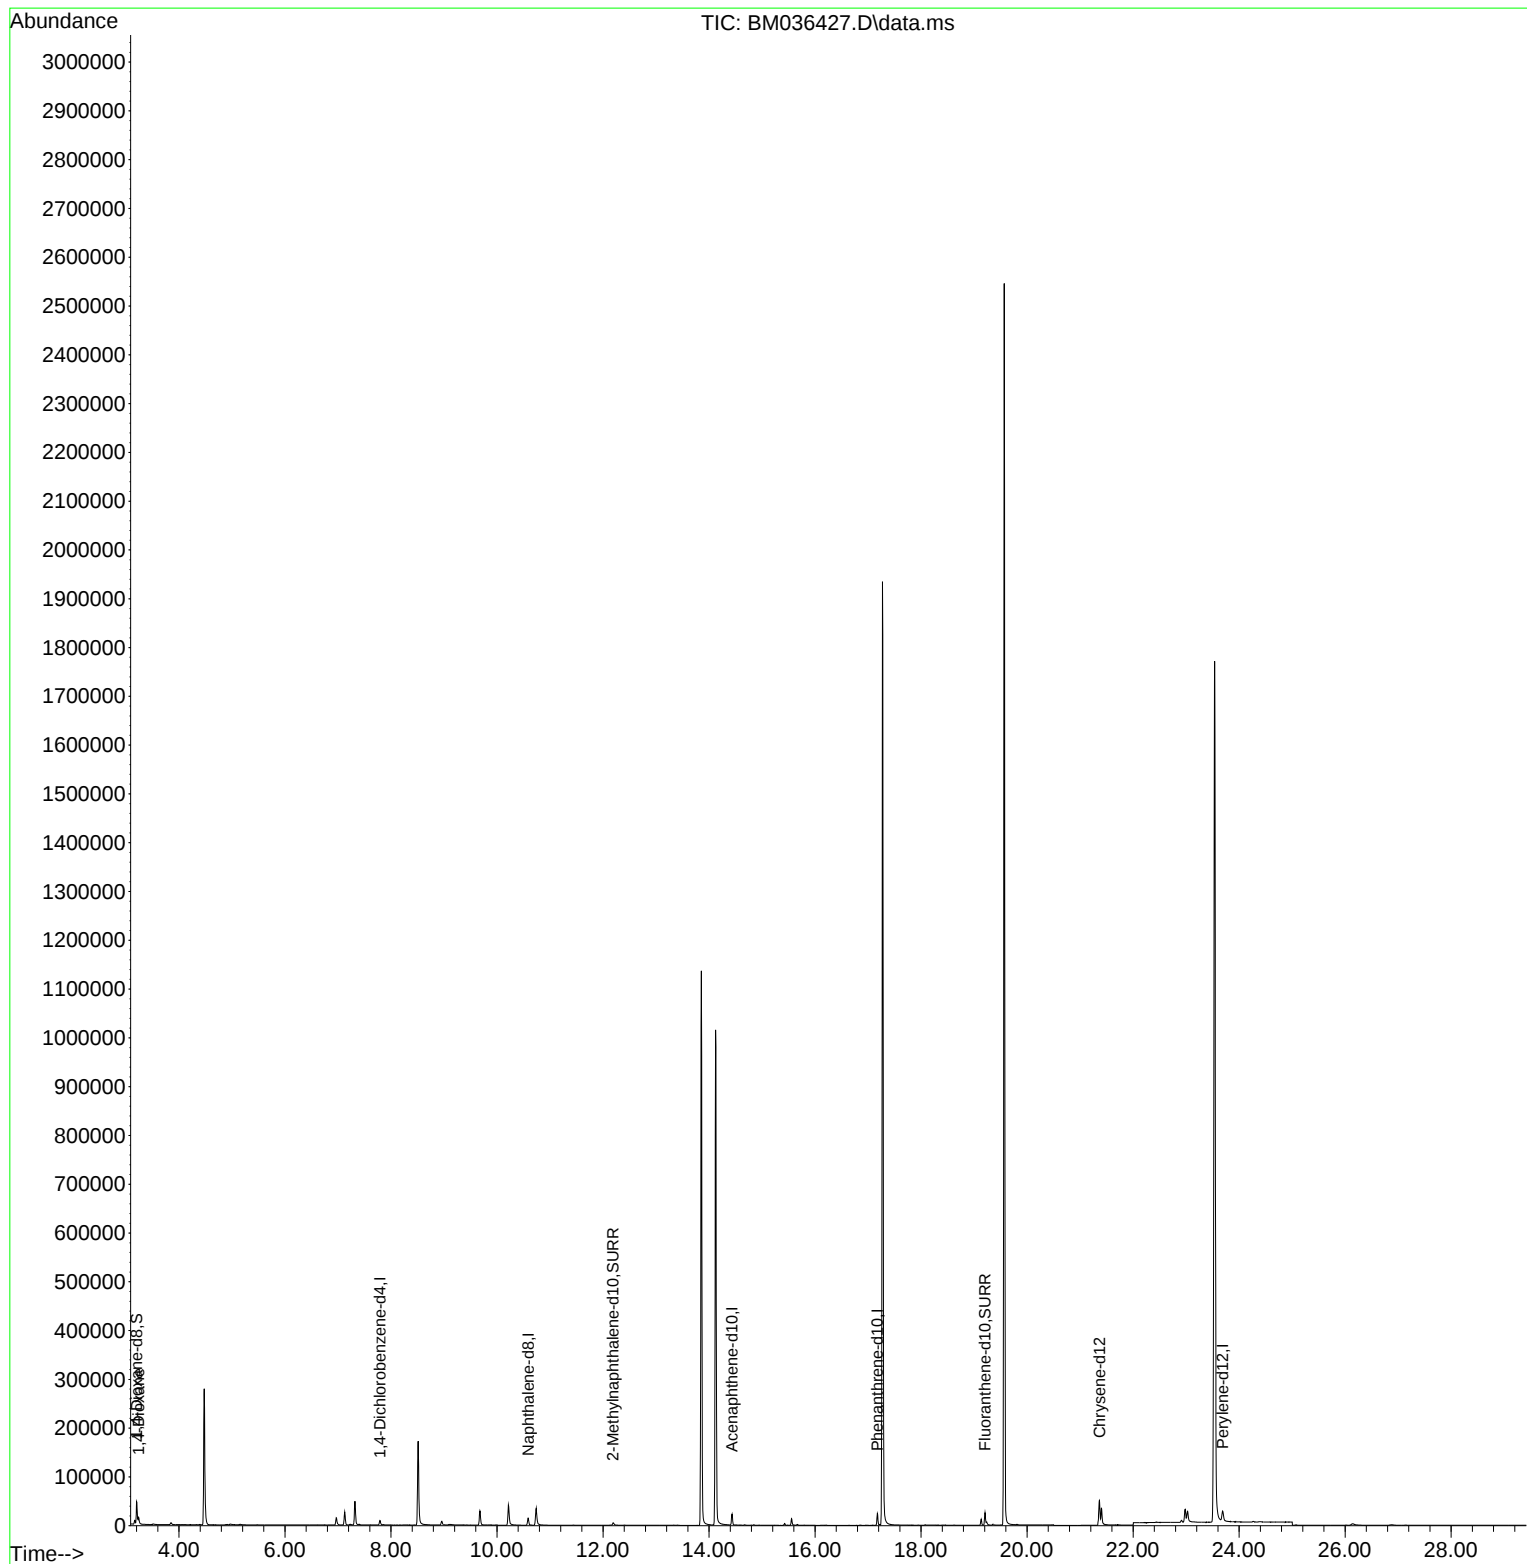


Abundance Scan 38 (3.243 min): BM036421.D\data.ms (-31)

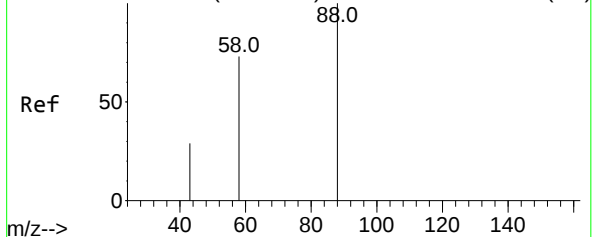

Abundance Scan 37 (3.239 min): BM036427.D\data.ms

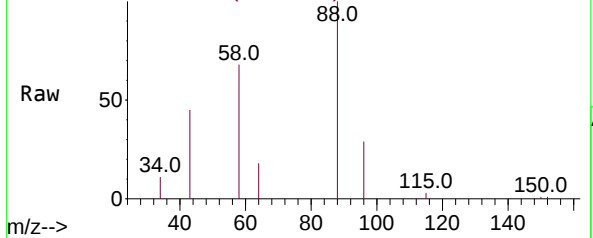

Abundance Scan 37 (3.239 min): BM036427.D\data.ms (-26)

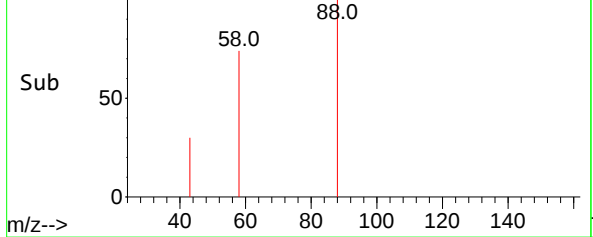

#2
1,4-Dioxane
Concen: 1.154 ng/ul
RT: 3.239 min Scan# 31
Delta R.T. -0.004 min
Lab File: BM036427.D
Acq: 26 Aug 2022 15:59

Instrument :
BNA_M
ClientSampleId :
BGN62

Tgt Ion: 88 Resp: 7454
Ion Ratio Lower Upper
88 100
43 44.6 37.8 56.6
58 68.5 42.6 63.8#

