

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082622\
 Data File : BM036429.D
 Acq On : 26 Aug 2022 17:13
 Operator : CG/JU
 Sample : N4349-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGN64

Quant Time: Aug 26 23:08:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM082622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 26 14:26:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	4270	0.400	ng/ul	0.00
4) Naphthalene-d8	10.594	136	17049	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.432	164	10472	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.178	188	22559	0.400	ng/ul	0.00
17) Chrysene-d12	21.368	240	31587	0.400	ng/ul	# 0.00
23) Perylene-d12	23.689	264	23978	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	25196	4.382	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.200	152	7600	0.279	ng/ul	0.01
18) Fluoranthene-d10	19.205	212	21510	0.551	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.238	88	1963	0.362	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082622\
Data File : BM036429.D
Acq On : 26 Aug 2022 17:13
Operator : CG/JU
Sample : N4349-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGN64


Quant Time: Aug 26 23:08:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM082622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 26 14:26:34 2022
Response via : Initial Calibration

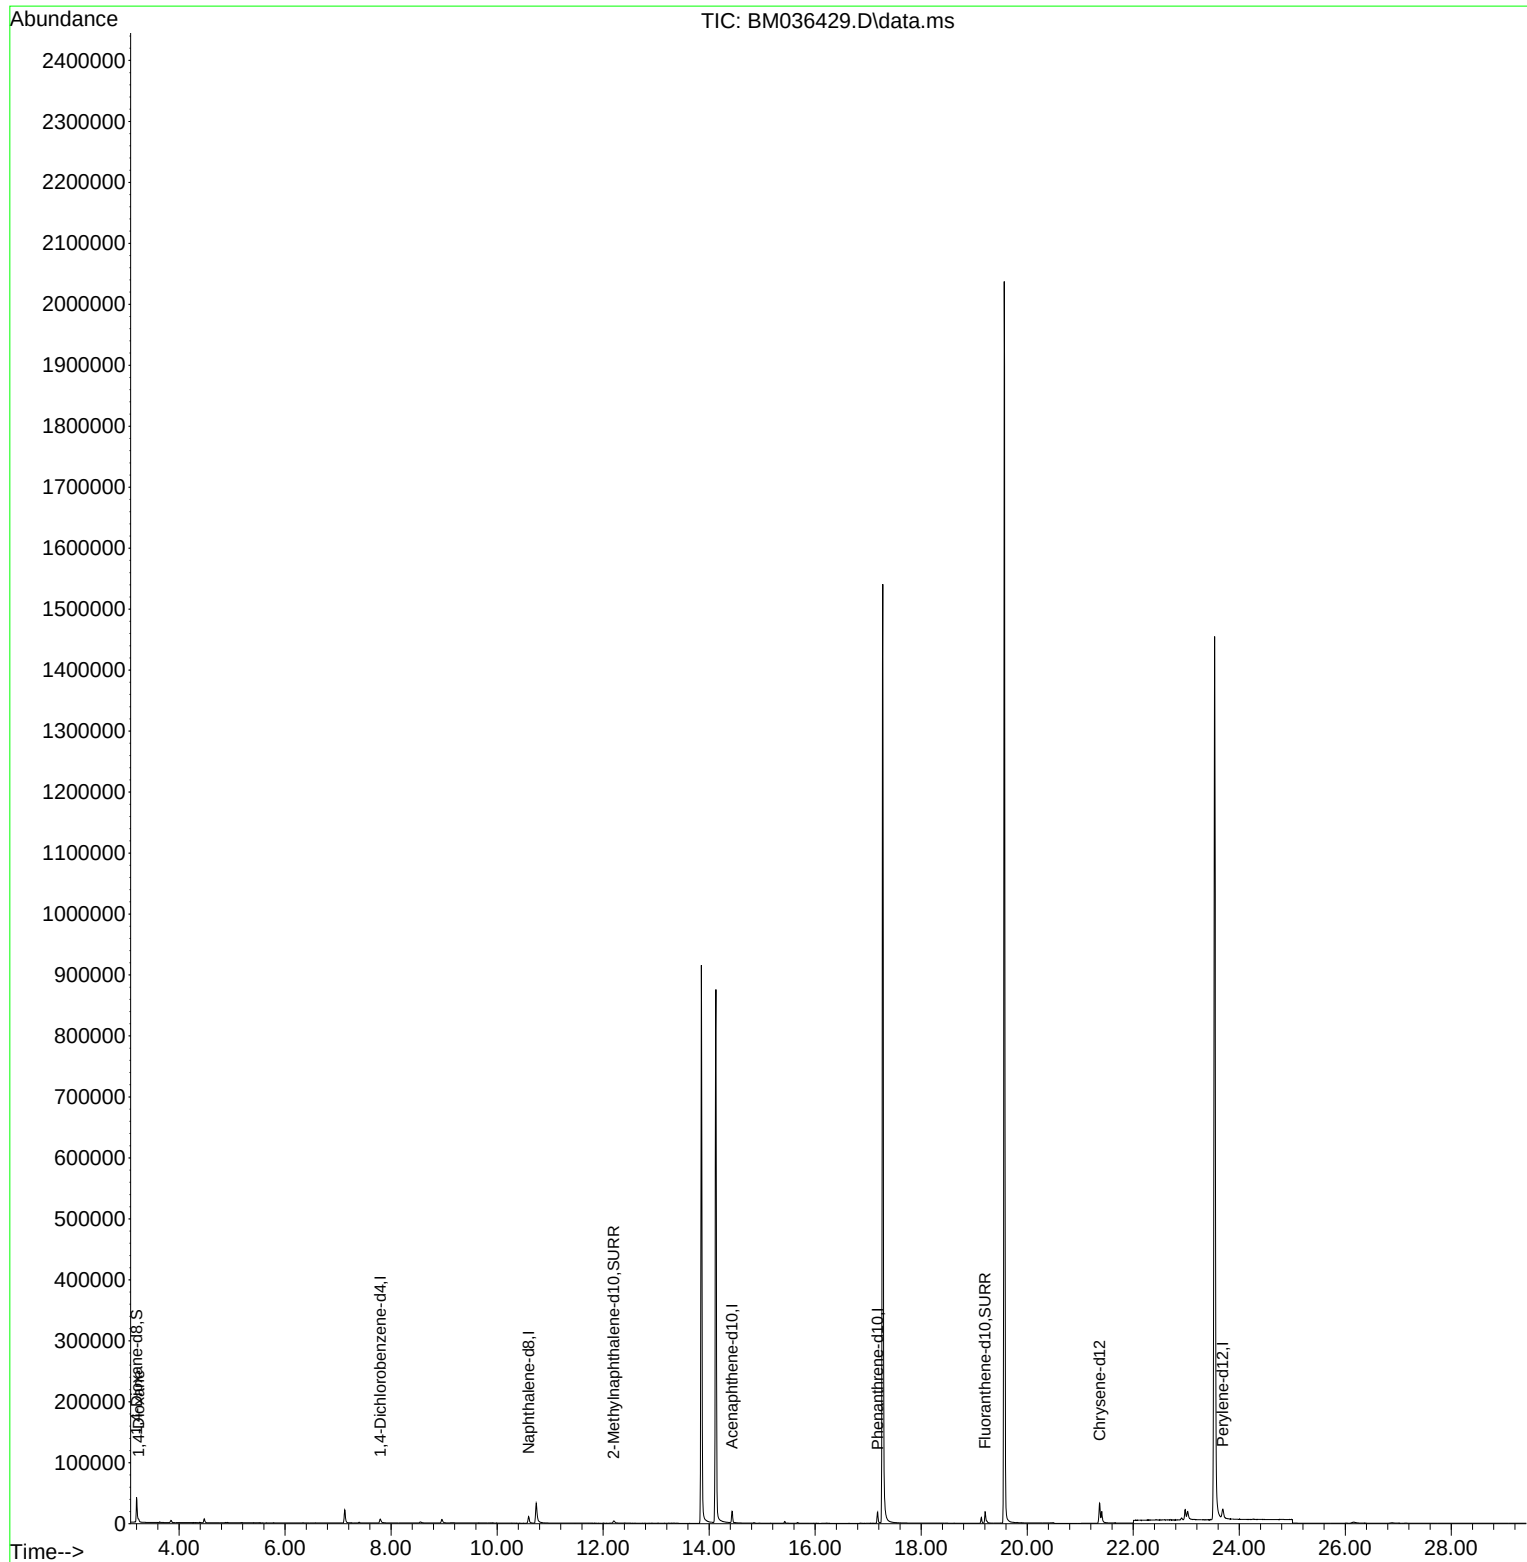

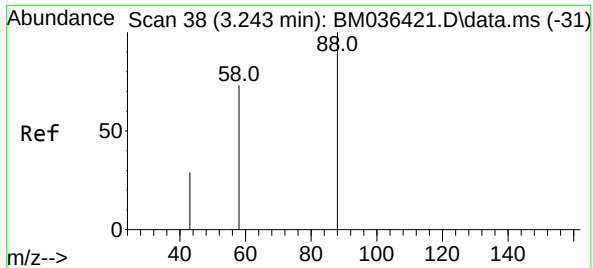

#2
 1,4-Dioxane
 Concen: 0.362 ng/ul
 RT: 3.238 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM036429.D
 Acq: 26 Aug 2022 17:13

Instrument :
 BNA_M
 ClientSampleId :
 BGN64

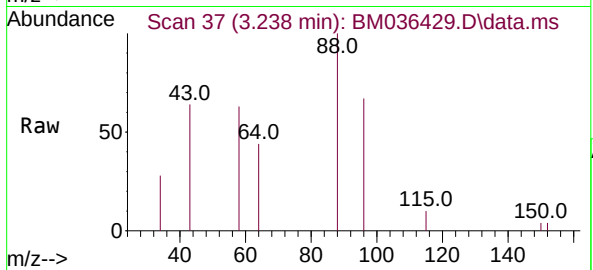

Tgt Ion:	88	Resp:	1963
Ion	Ratio	Lower	Upper
88	100		
43	63.7	37.8	56.6#
58	63.3	42.6	63.8

