
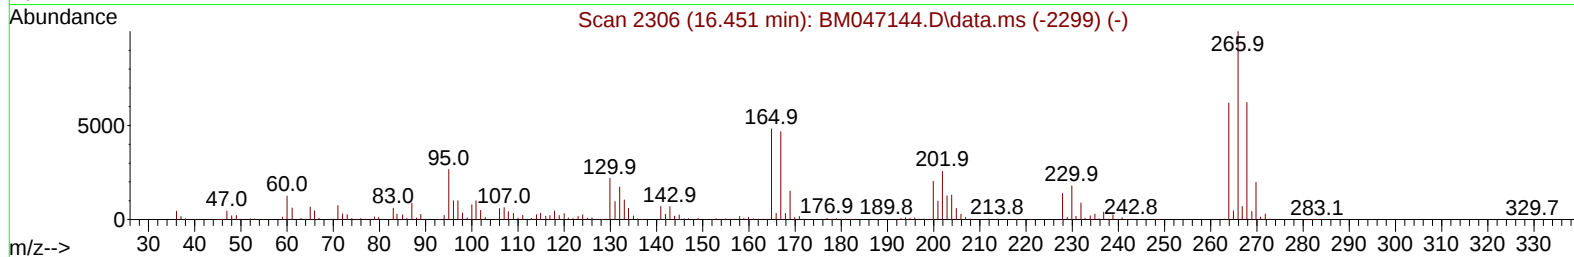
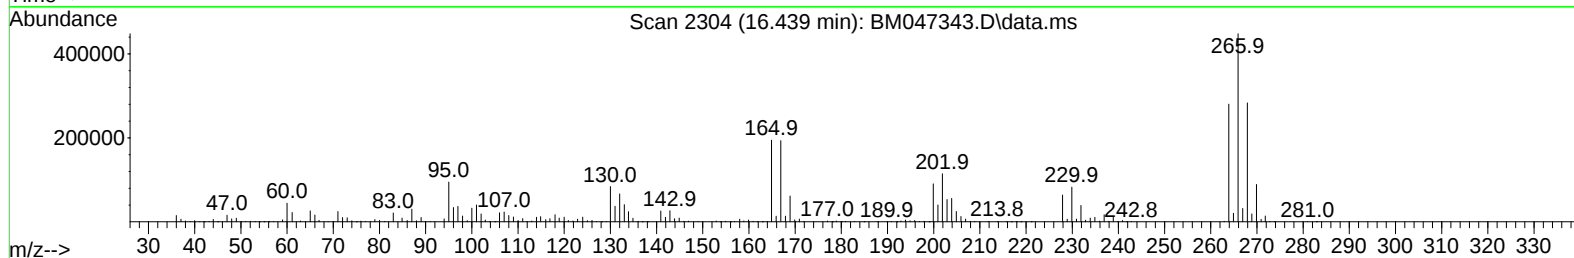


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082624\
Data File : BM047343.D
Acq On : 26 Aug 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 14:56:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 14:47:08 2024
Response via : Initial Calibration

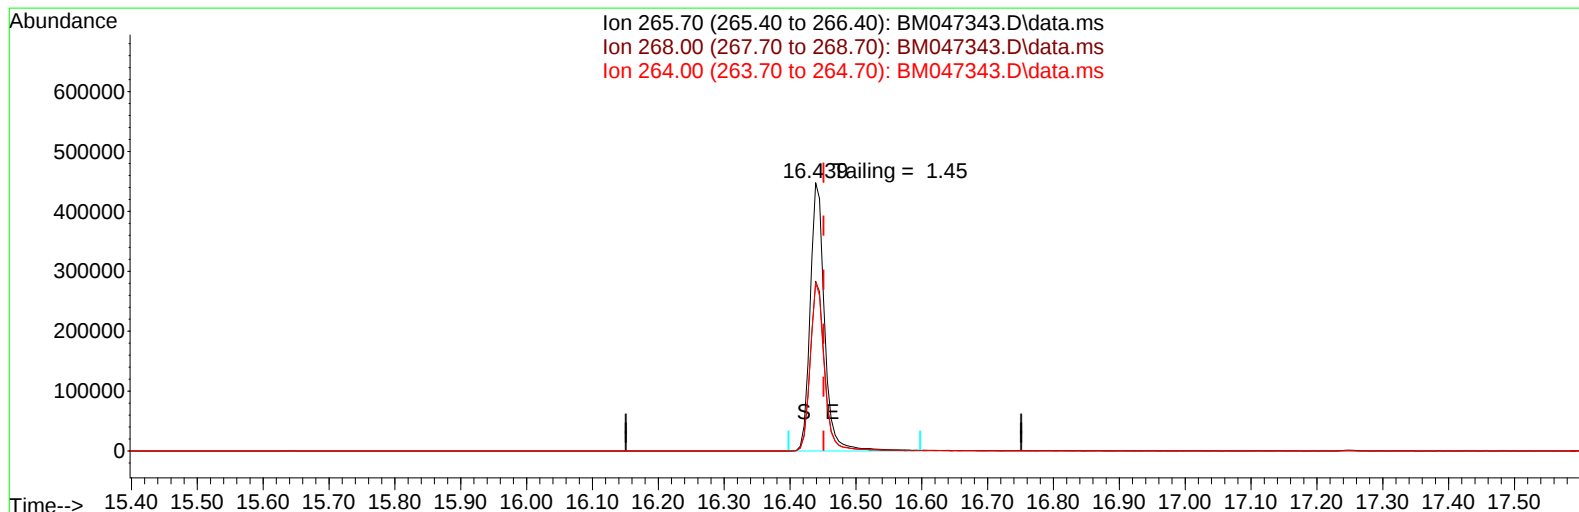

TIC: BM047343.D\data.ms

(70) Pentachlorophenol (C)




16.439min (-0.012) 0.00 ng

response 681726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.24
264.00	62.00	62.59
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082624\  
Data File : BM047343.D  
Acq On    : 26 Aug 2024  11:43  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Aug 26 14:56:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 14:47:08 2024
Response via : Initial Calibration

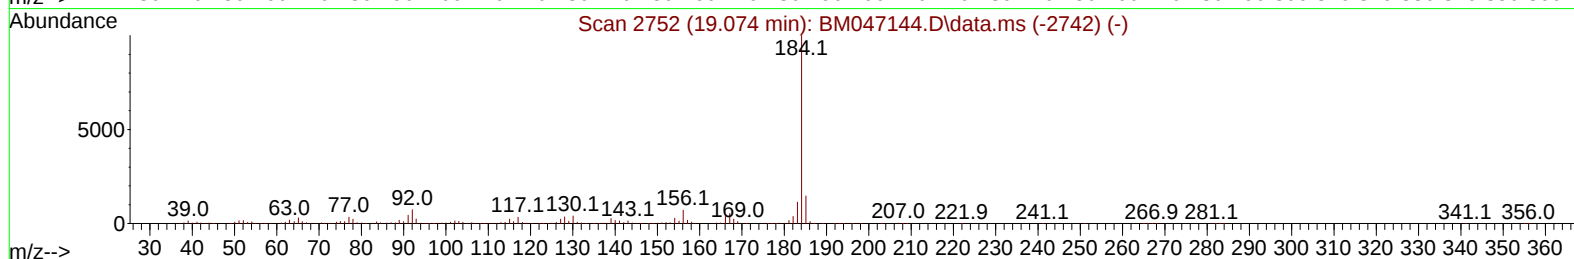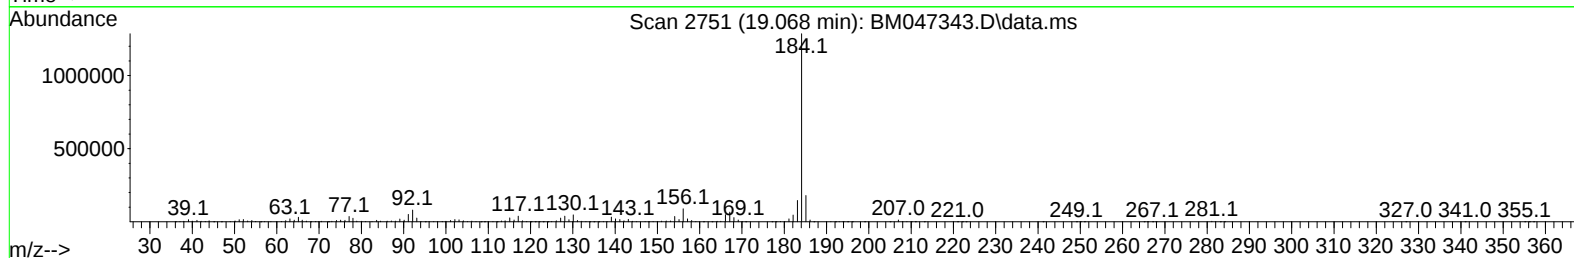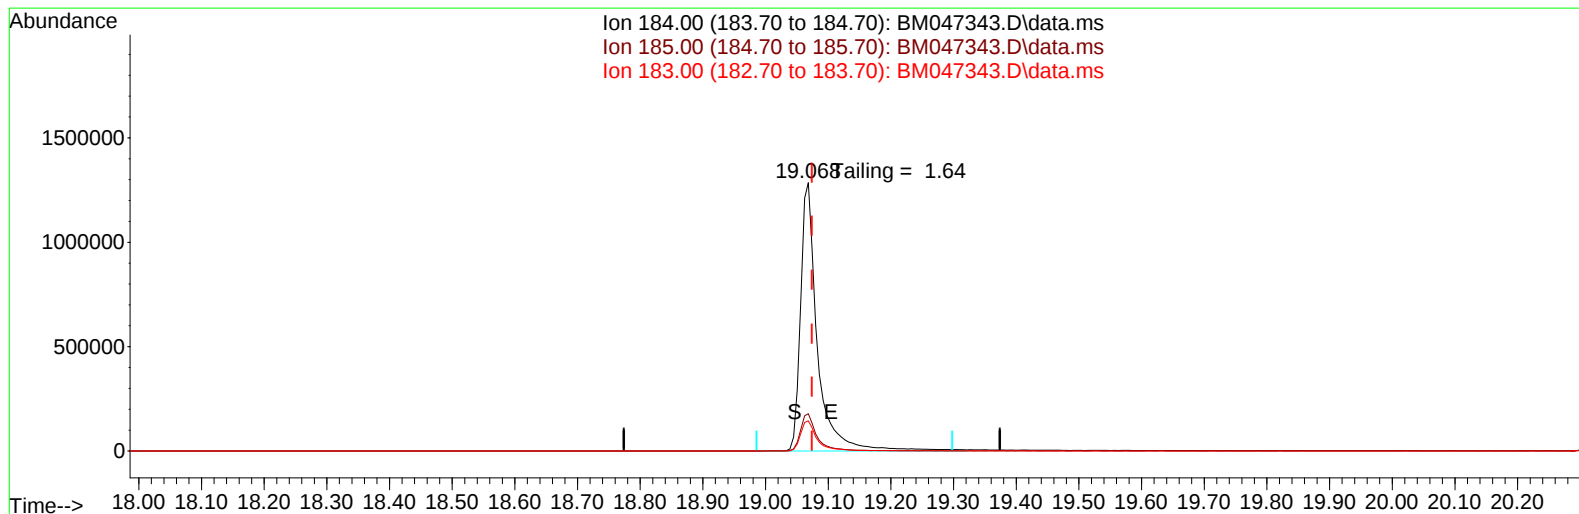

TIC: BM047343.D\data.ms

(77) Benzidine

19.068min (-0.006) 305816.37 ng

response **2411571**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.70	13.93
--------	-------	-------

183.00	11.30	11.30
--------	-------	-------

0.00 0.00 0.00