


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082624\
Data File : BM047343.D
Acq On : 26 Aug 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

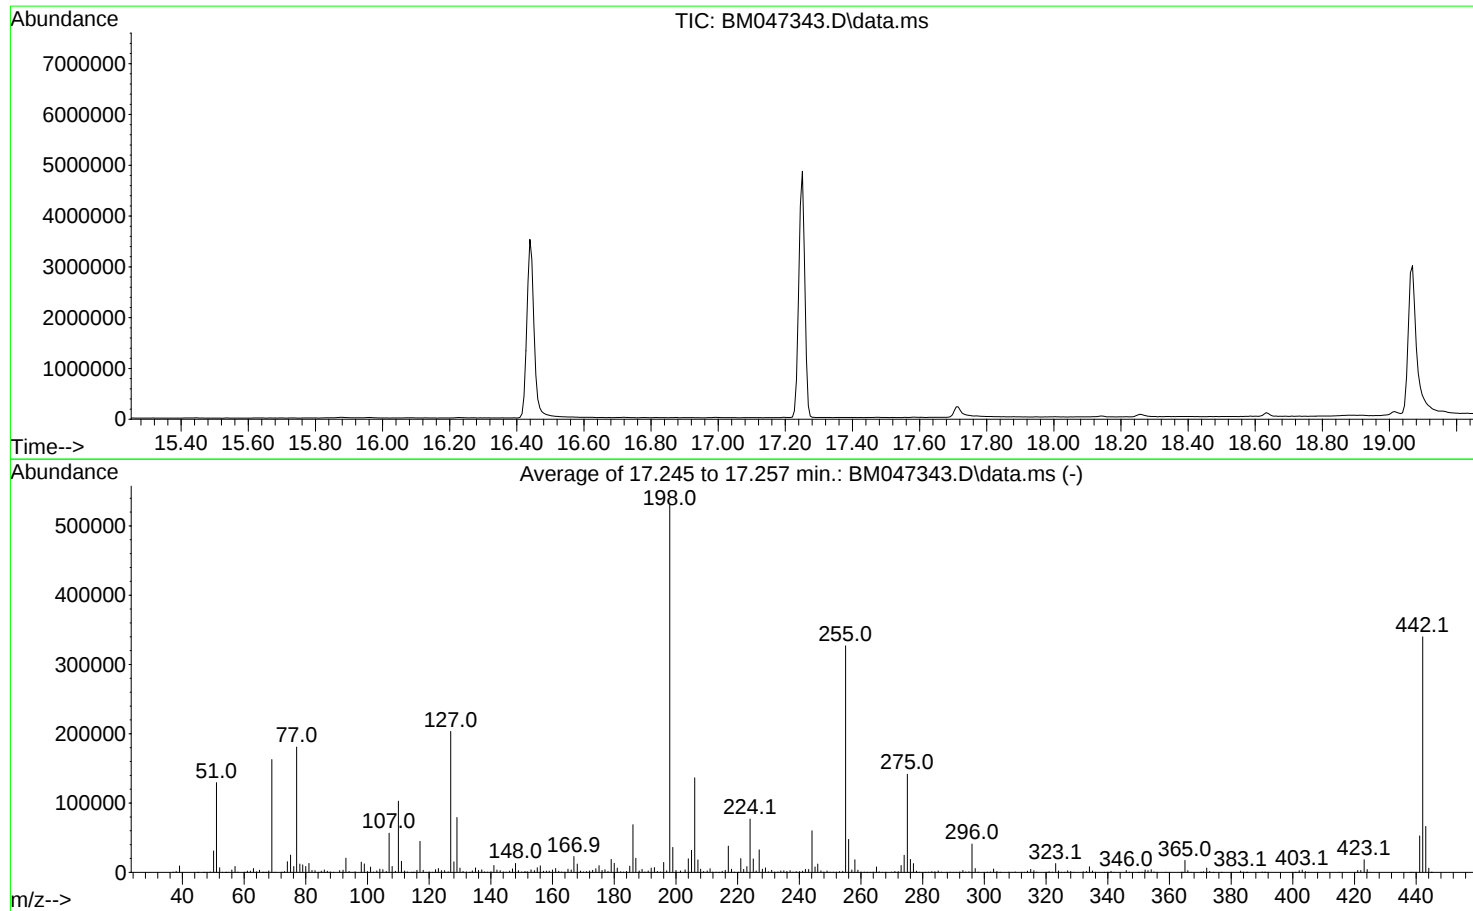

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	129515	PASS
68	69	0.00	2	1.3	2088	PASS
69	198	0.00	100	30.7	162802	PASS
70	69	0.00	2	0.2	329	PASS
127	198	10	80	38.3	203371	PASS
197	198	0.00	2	0.4	2232	PASS
198	198	100	100	100.0	530923	PASS
199	198	5	9	6.8	36136	PASS
275	198	10	60	26.7	141501	PASS
365	198	1	100	3.2	17232	PASS
441	198	0.01	100	9.9	52792	PASS
442	442	50	100	100.0	340032	PASS
443	442	15	24	19.5	66371	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2024	BNA_M	<u>BM047343.D</u>
Compound Name	Response	Retention Time
DDT	1787330	20.309
DDD	20153	19.909
DDE	464	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20617	1807947	1.14

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082624\
Data File : BM047343.D
Acq On : 26 Aug 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 26 14:56:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 14:47:08 2024
Response via : Initial Calibration

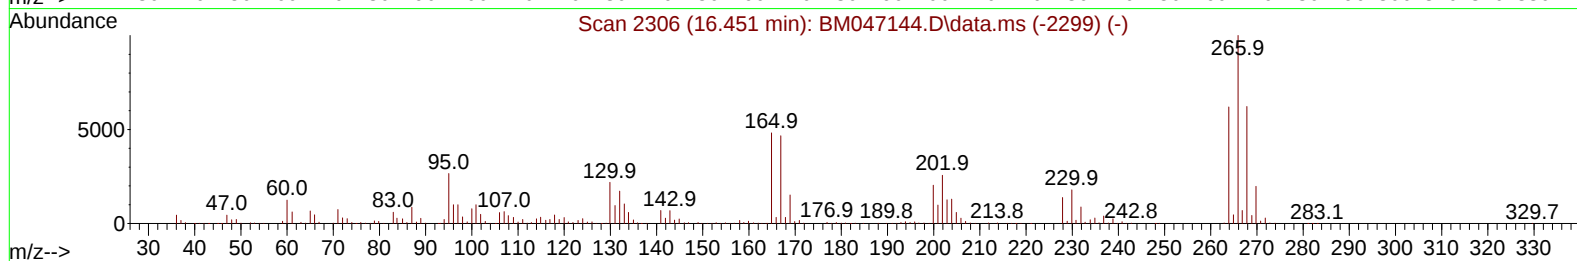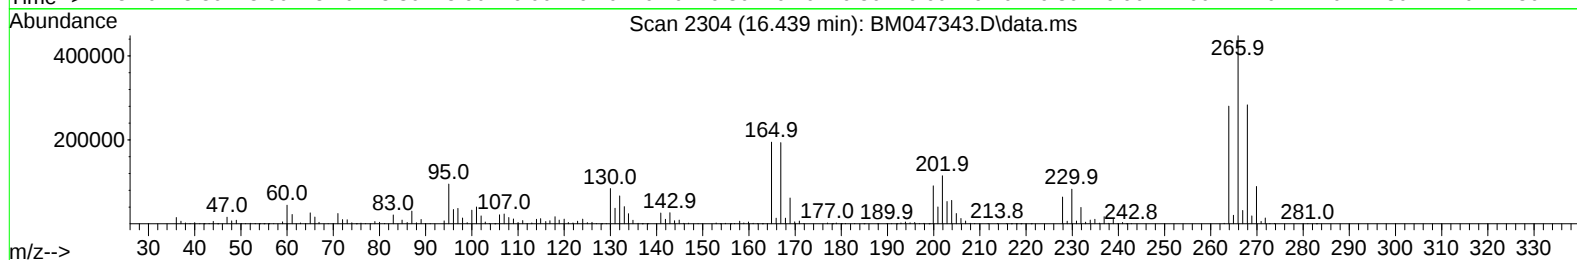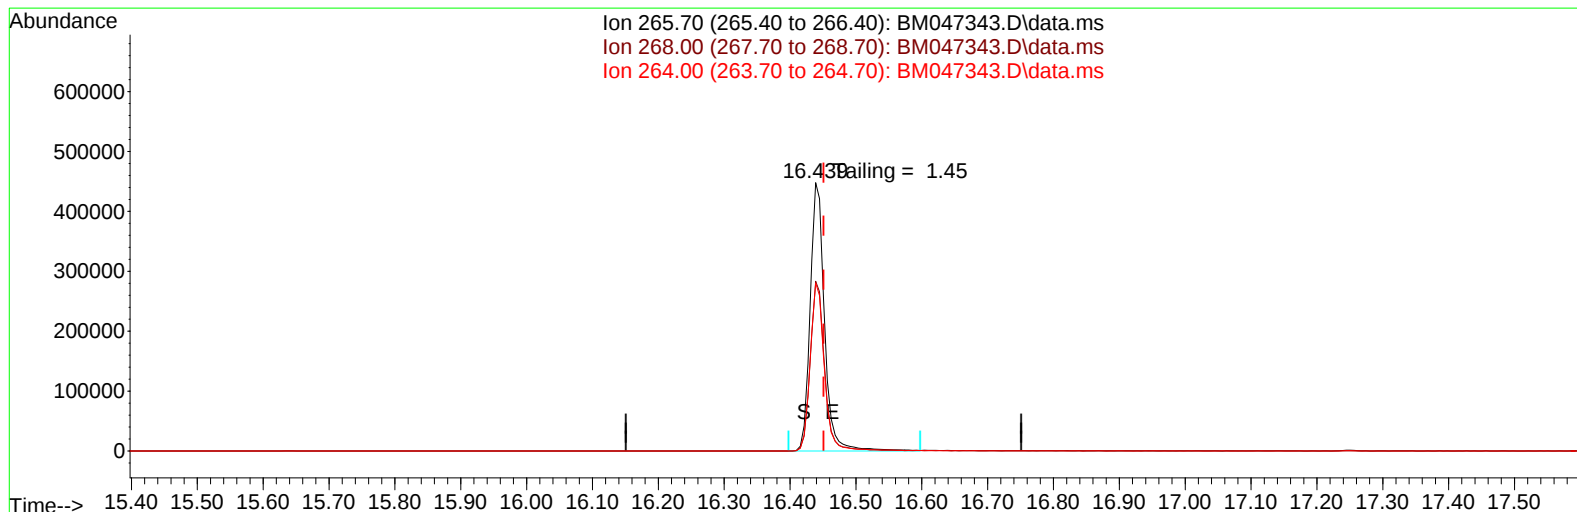

TIC: BM047343.D\data.ms

(70) Pentachlorophenol (C)

16.439min (-0.012) 0.00 ng




response 681726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.24
264.00	62.00	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082624\
Data File : BM047343.D
Acq On : 26 Aug 2024 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 26 14:56:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 14:47:08 2024
Response via : Initial Calibration

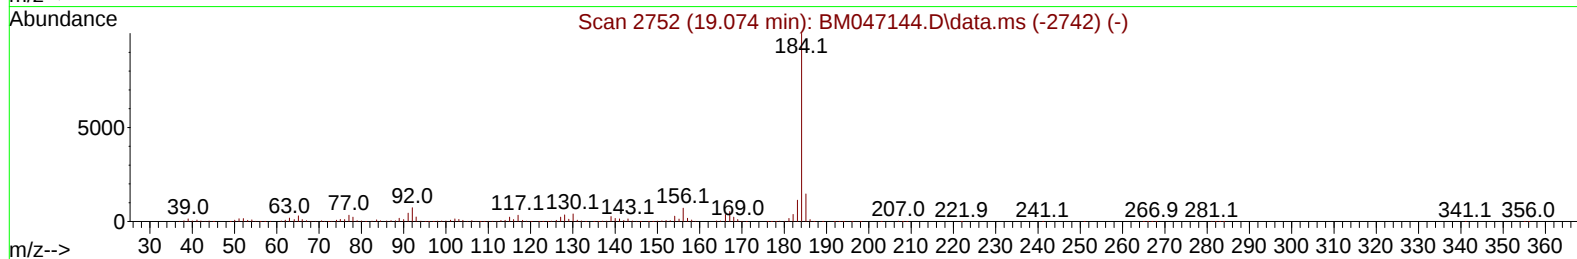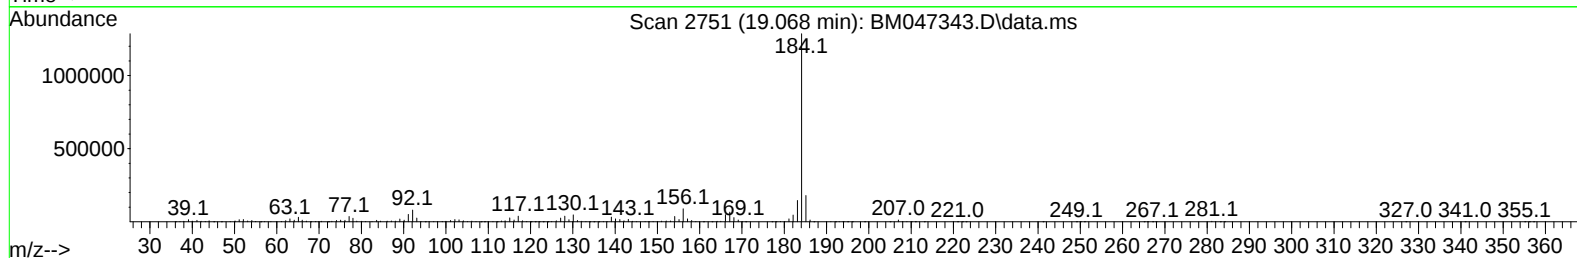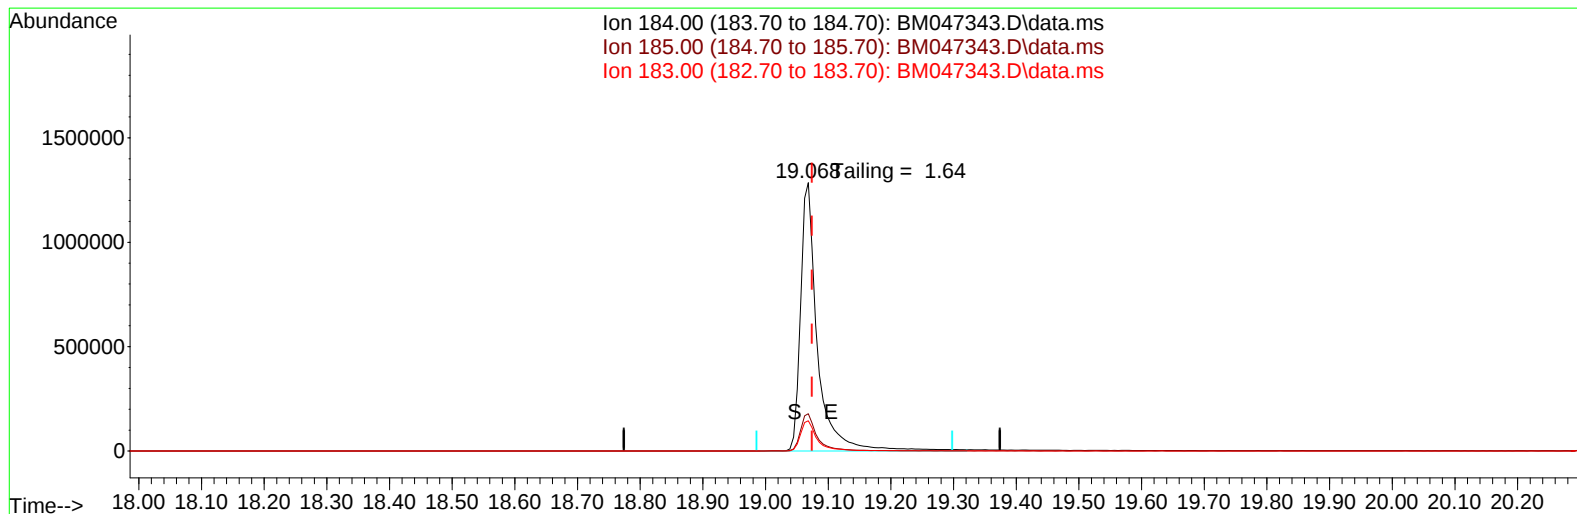

TIC: BM047343.D\data.ms

(77) Benzidine

19.068min (-0.006) 305816.37 ng

response 2411571

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.93
183.00	11.30	11.30
0.00	0.00	0.00