
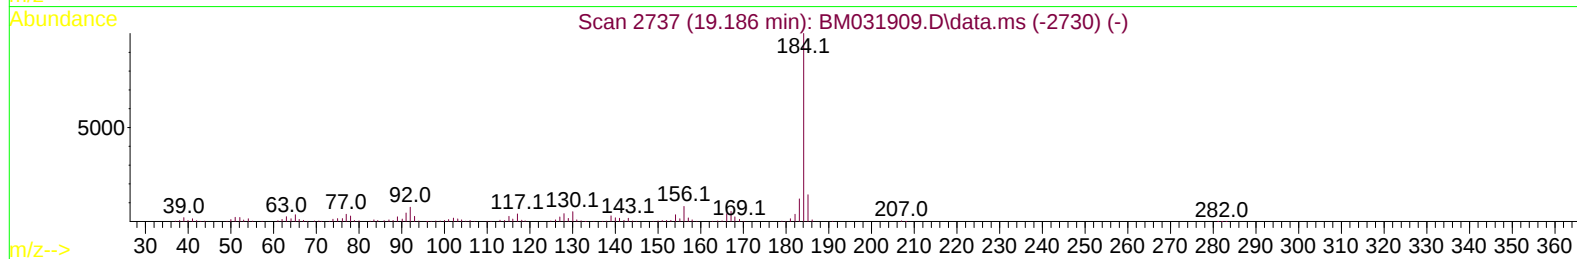
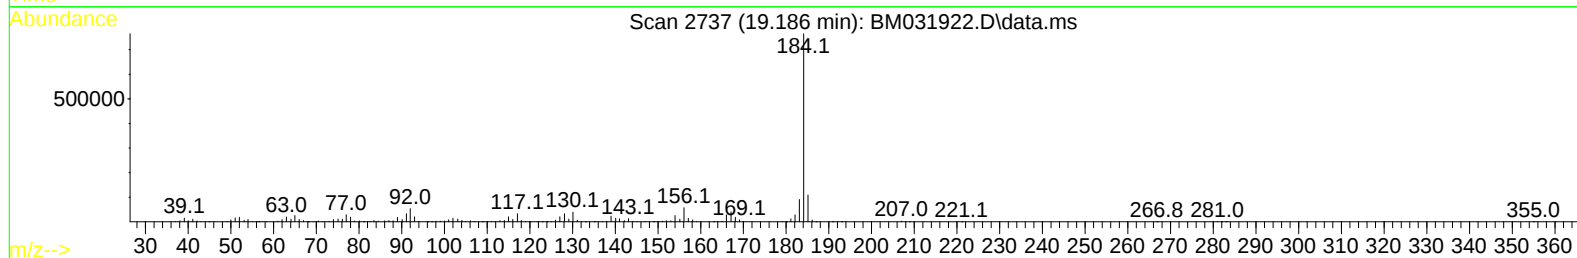


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031922.D
Acq On : 27 Aug 2021 08:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 10:57:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 14:24:44 2021
Response via : Initial Calibration

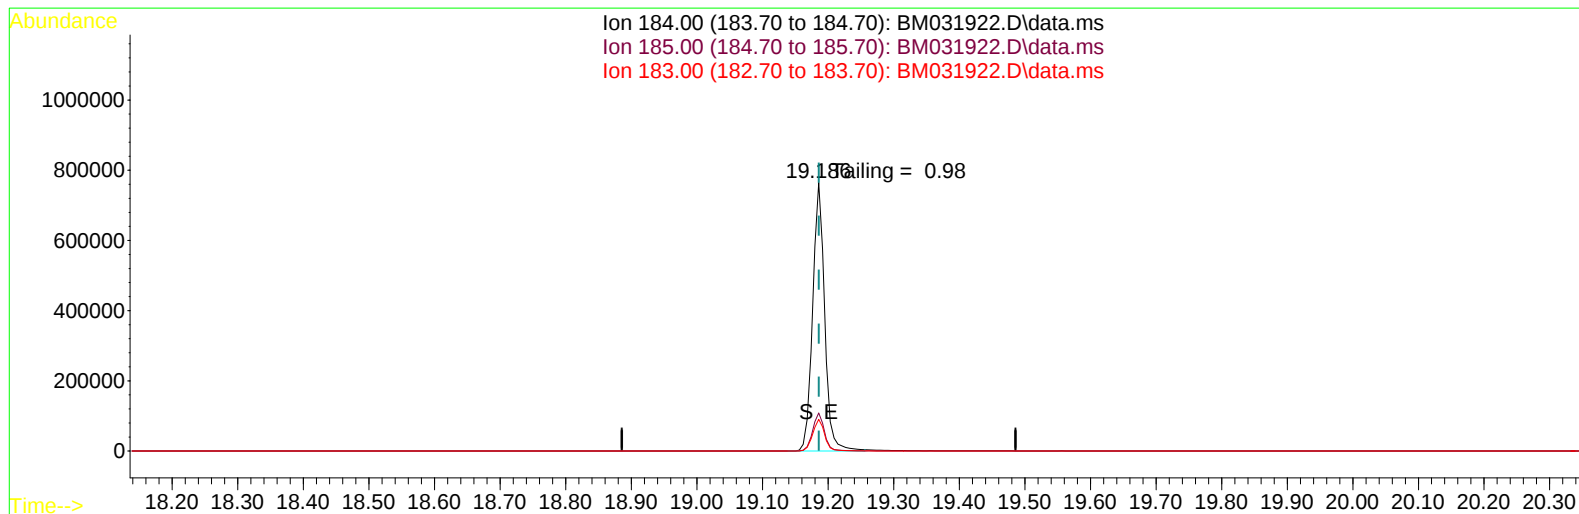




TIC: BM031922.D\data.ms

(77) Benzidine**19.186min (-0.000) 11608.64 ng****response 985170**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.24
183.00	11.20	11.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031922.D
Acq On : 27 Aug 2021 08:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 10:57:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 14:24:44 2021
Response via : Initial Calibration

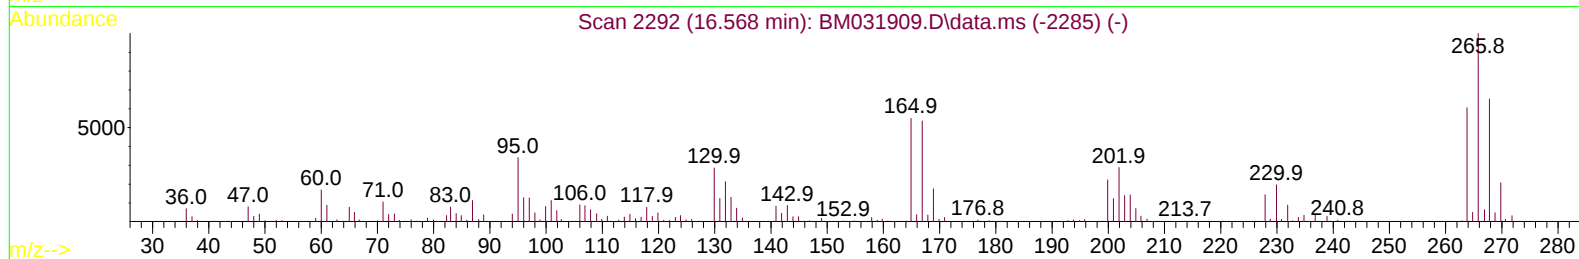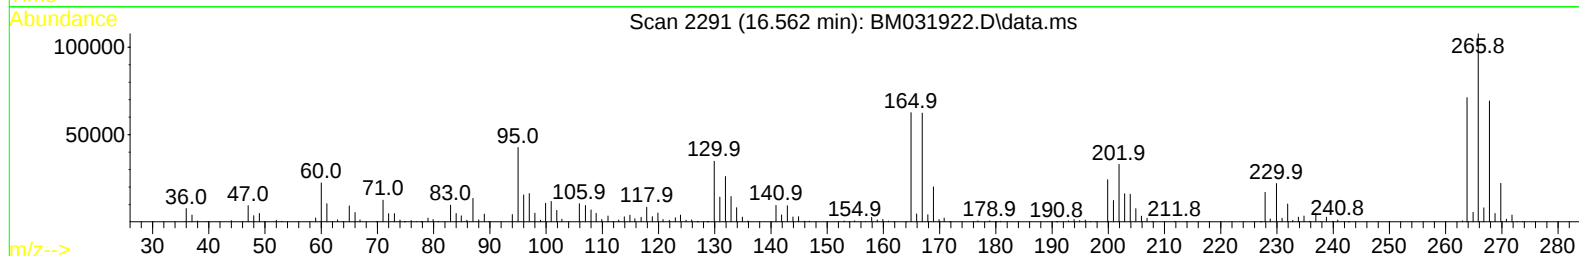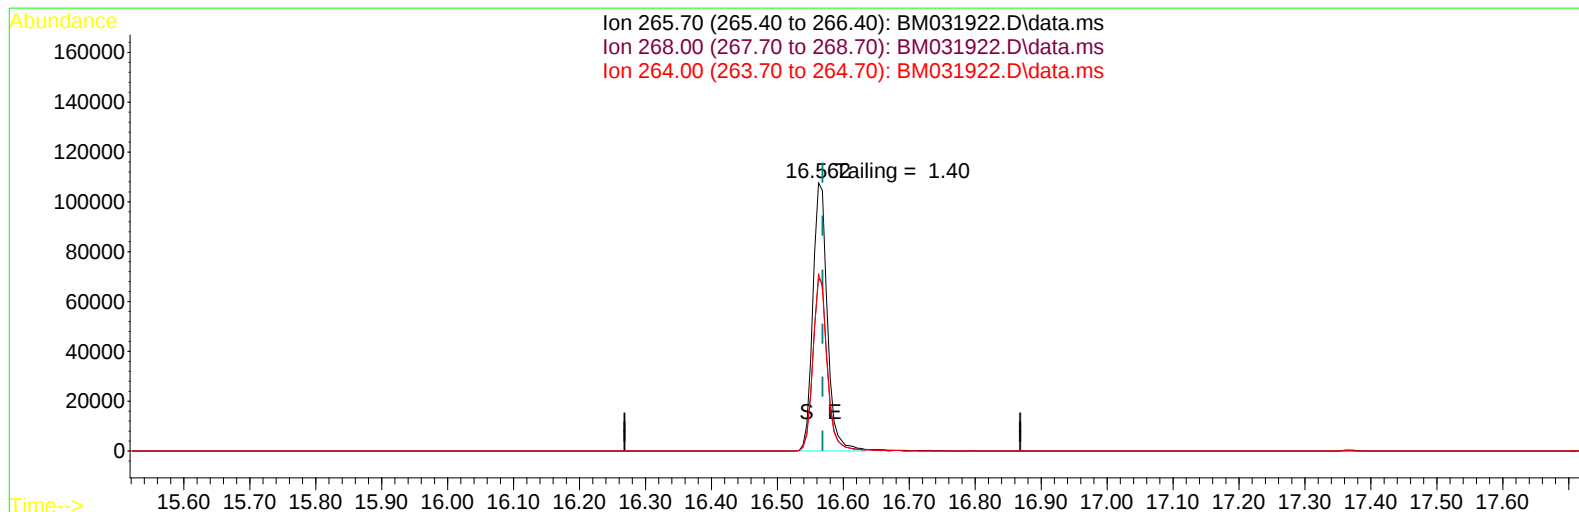

TIC: BM031922.D\data.ms

(70) Pentachlorophenol (C)

16.562min (-0.006) 42890.14 ng

response 166215

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.35
264.00	65.10	66.09
0.00	0.00	0.00