

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
 Data File : BM031924.D
 Acq On : 27 Aug 2021 12:34
 Operator : CG/JU
 Sample : PB138731BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138731BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.152	345	351	366	rBV	1823784	2574610	44.99%	10.788%
2	6.716	609	617	631	rBV	1716333	2715199	47.44%	11.377%
3	7.510	745	752	764	rBV	270480	424611	7.42%	1.779%
4	8.669	940	949	965	rBV	999858	1683224	29.41%	7.053%
5	10.269	1214	1221	1234	rBV	330819	586453	10.25%	2.457%
6	12.763	1638	1645	1660	rBV	2519771	3788984	66.21%	15.876%
7	14.151	1875	1881	1893	rVB	509653	778789	13.61%	3.263%
8	15.657	2130	2137	2158	rBV	2176815	2969098	51.88%	12.440%
9	16.910	2344	2350	2362	rBV	614593	915181	15.99%	3.835%
10	19.562	2795	2801	2806	rBV	4914618	5723041	100.00%	23.979%
11	21.115	3060	3065	3075	rBV	639130	895525	15.65%	3.752%
12	23.262	3424	3430	3440	rVB	439464	811820	14.19%	3.401%




Sum of corrected areas: 23866535

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031924.D
Acq On : 27 Aug 2021 12:34
Operator : CG/JU
Sample : PB138731BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138731BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

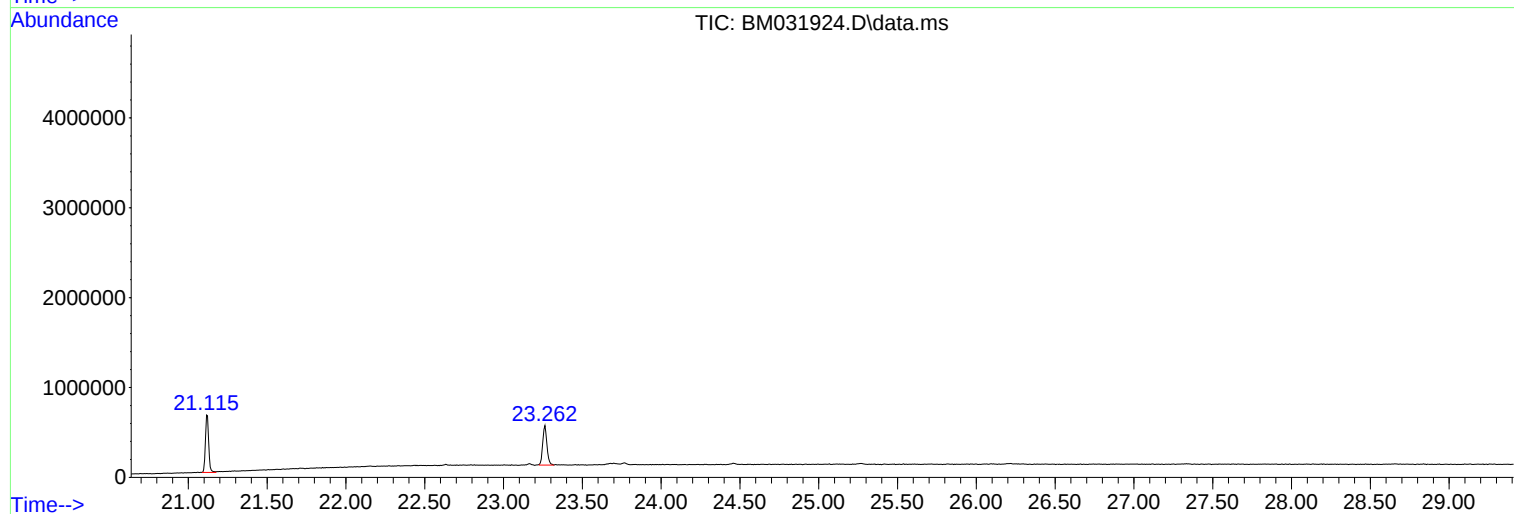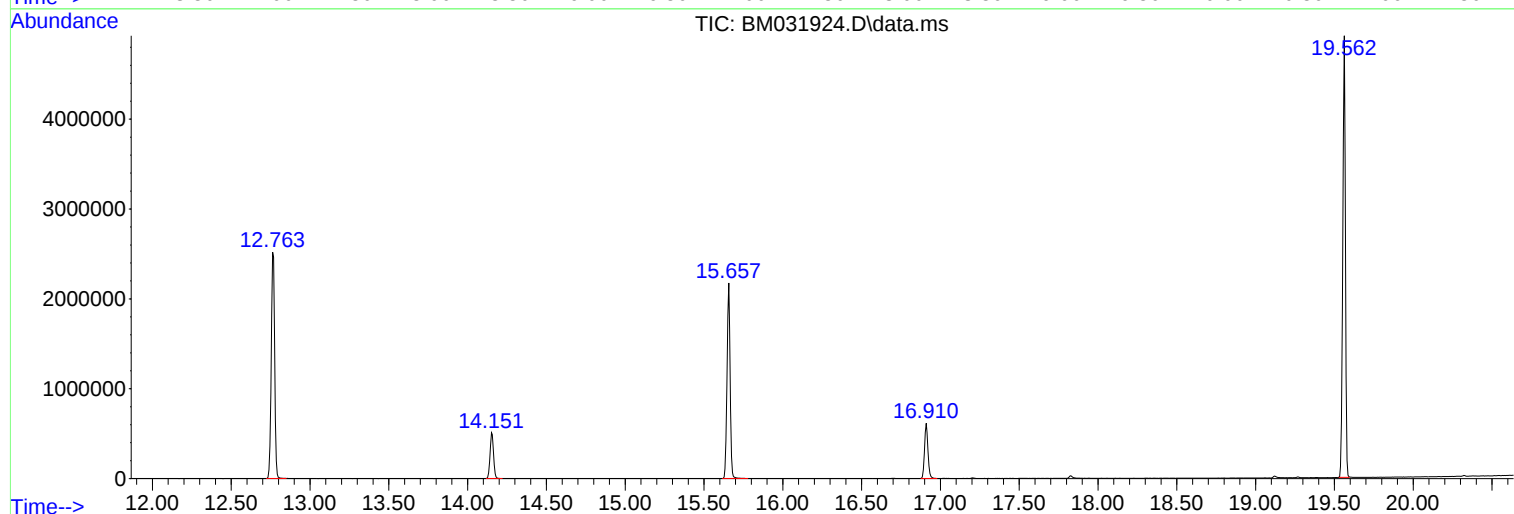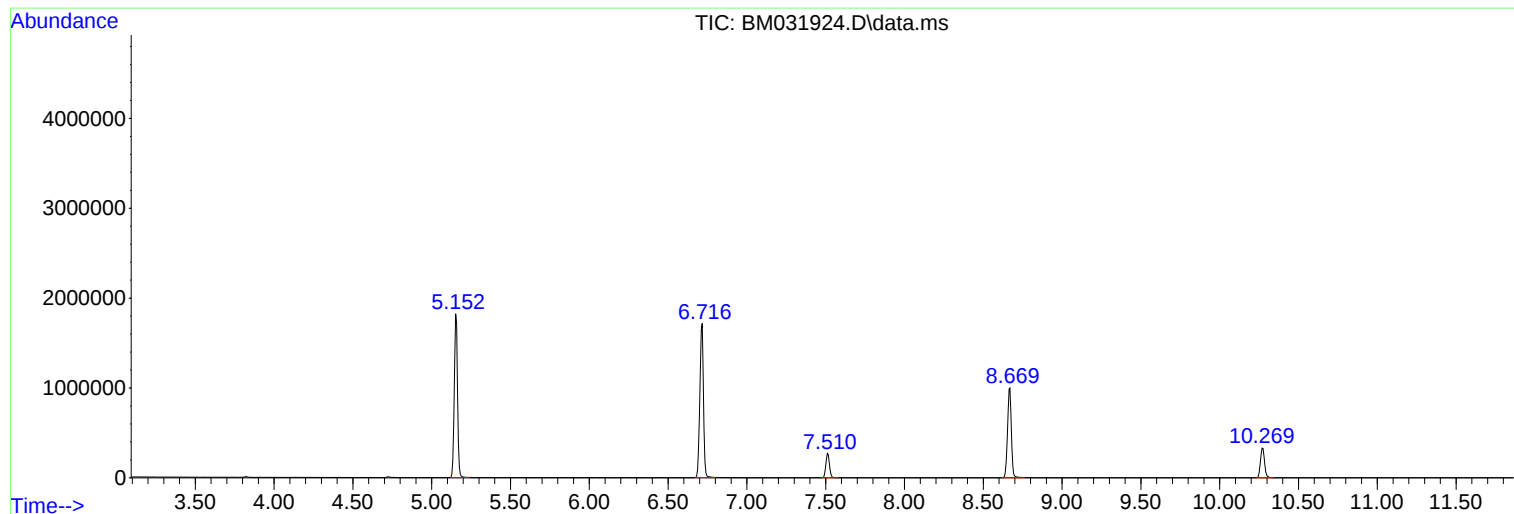

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031924.D
Acq On : 27 Aug 2021 12:34
Operator : CG/JU
Sample : PB138731BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138731BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031924.D
Acq On : 27 Aug 2021 12:34
Operator : CG/JU
Sample : PB138731BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138731BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------