
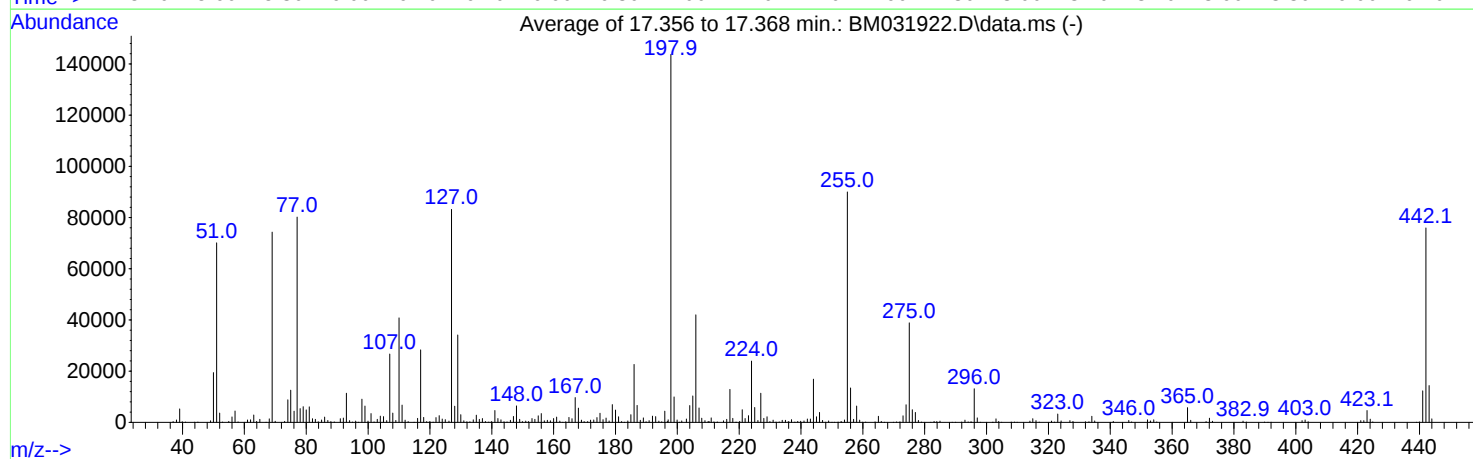


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
 Data File : BM031922.D
 Acq On : 27 Aug 2021 08:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 26 14:24:44 2021

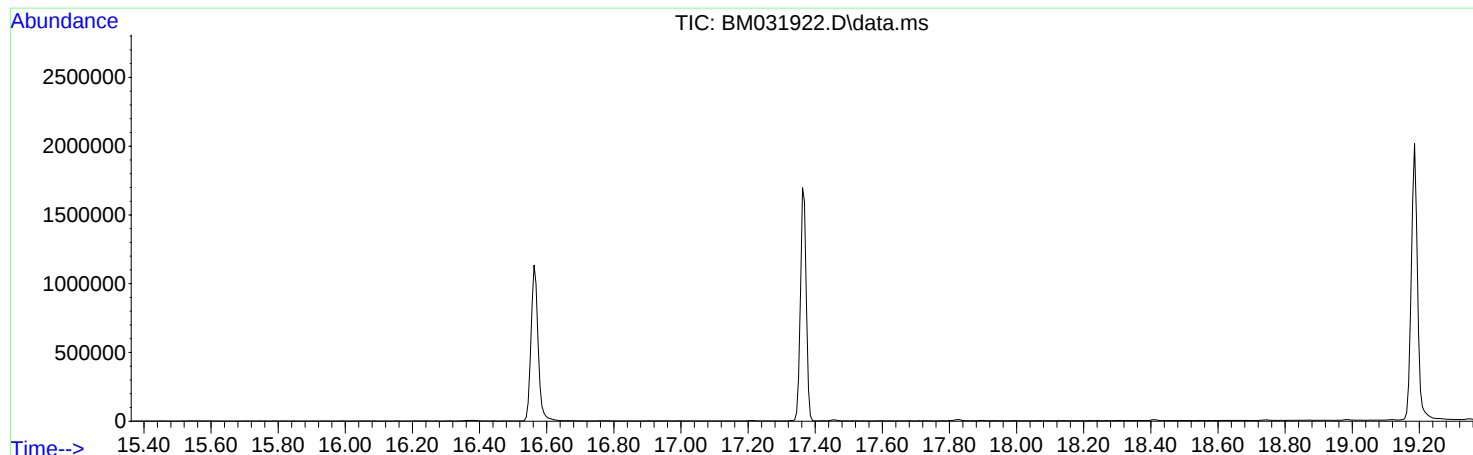




AutoFind: Scans 2426, 2427, 2428; Background Corrected with Scan 2420

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	70125	PASS
68	69	0.00	2	1.8	1354	PASS
69	198	0.00	100	51.7	74312	PASS
70	69	0.00	2	0.6	436	PASS
127	198	10	80	57.9	83203	PASS
197	198	0.00	2	0.7	1022	PASS
198	198	100	100	100.0	143667	PASS
199	198	5	9	6.9	9931	PASS
275	198	10	60	27.0	38853	PASS
365	198	1	100	4.0	5758	PASS
441	198	0.01	100	8.6	12292	PASS
442	442	50	100	100.0	75909	PASS
443	442	15	24	18.9	14349	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031922.D
Acq On    : 27 Aug 2021  08:22
Operator  : CG/JU
Sample    : DFTPP
Misc      :
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 27 10:57:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 14:24:44 2021
Response via : Initial Calibration

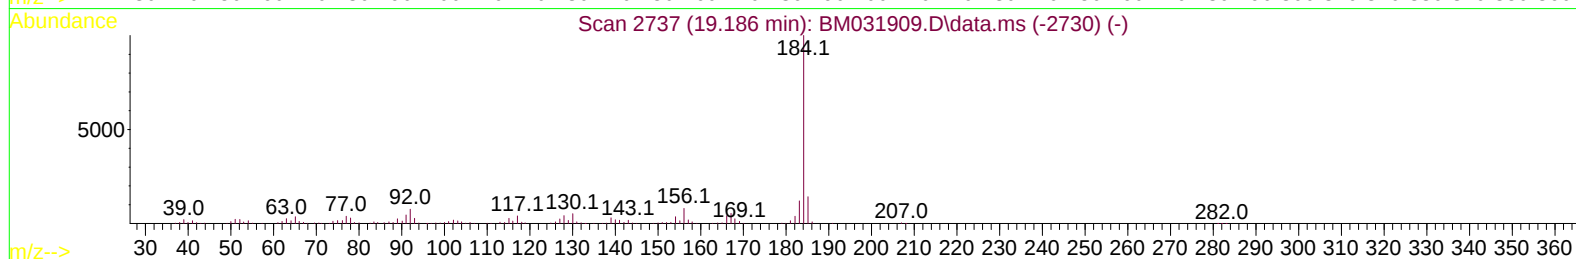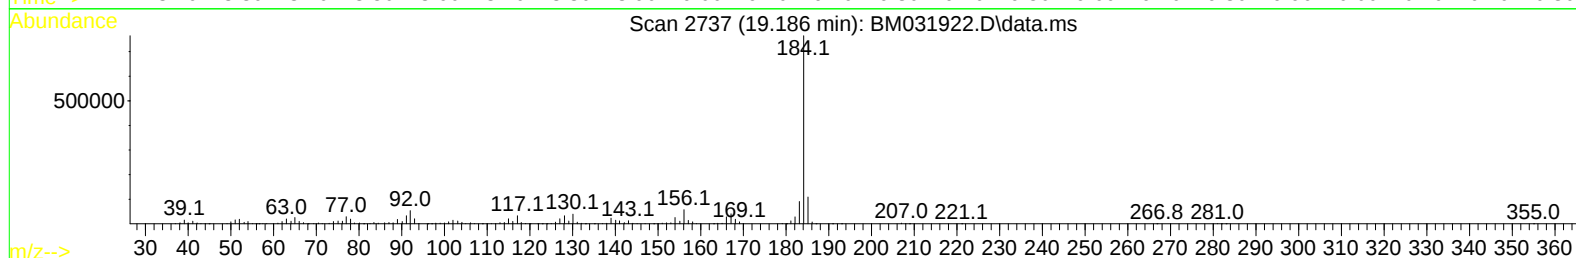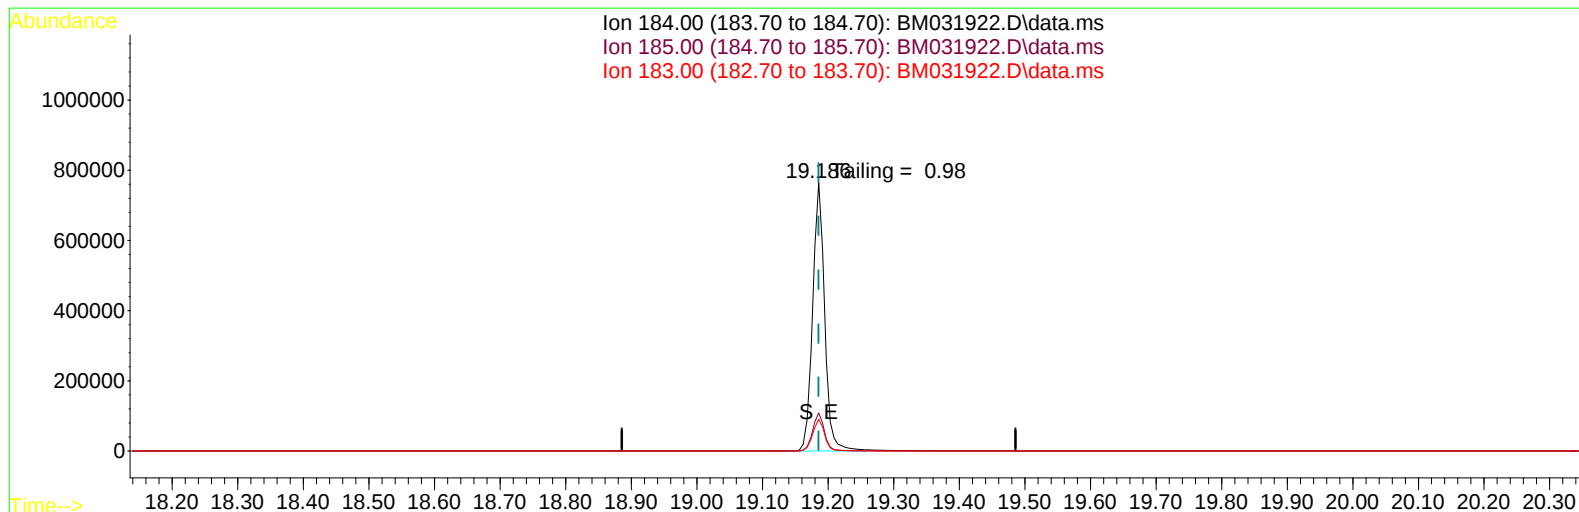

TIC: BM031922.D\data.ms

(77) Benzidine

19.186min (-0.000) 11608.64 ng

response **985170**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	13.30	14.24
--------	-------	-------




183.00	11.20	11.81
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082721\
Data File : BM031922.D
Acq On : 27 Aug 2021 08:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 27 10:57:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 26 14:24:44 2021
Response via : Initial Calibration

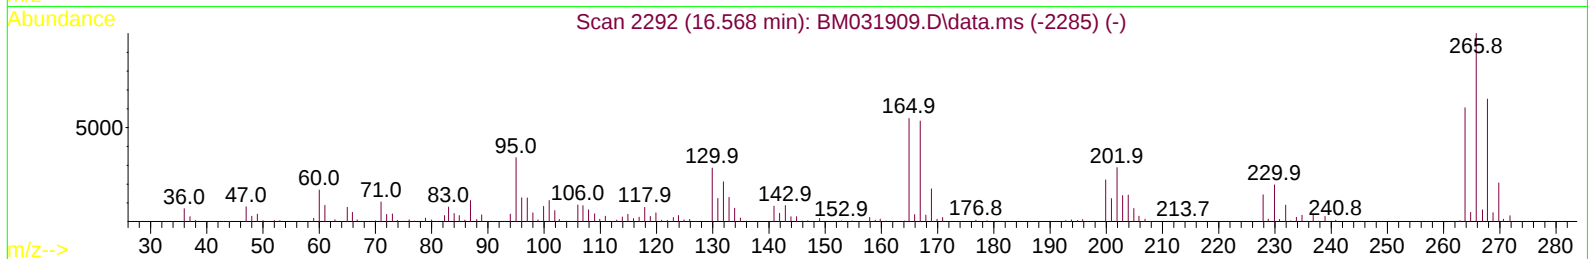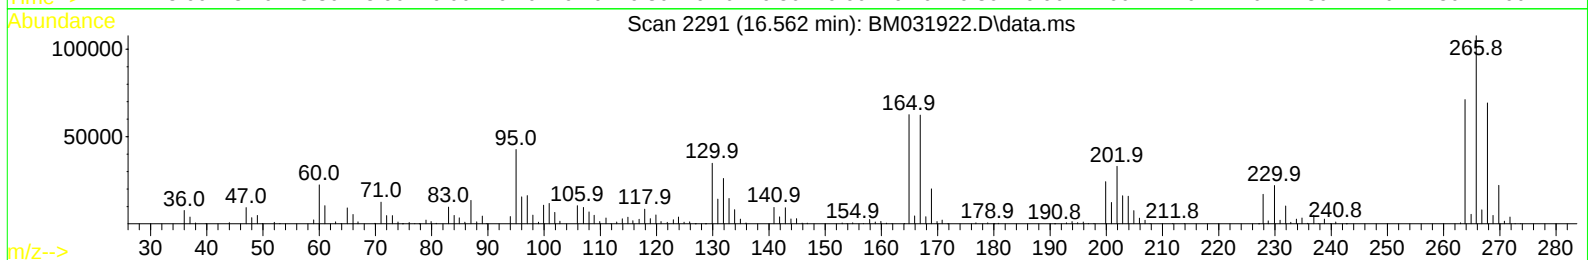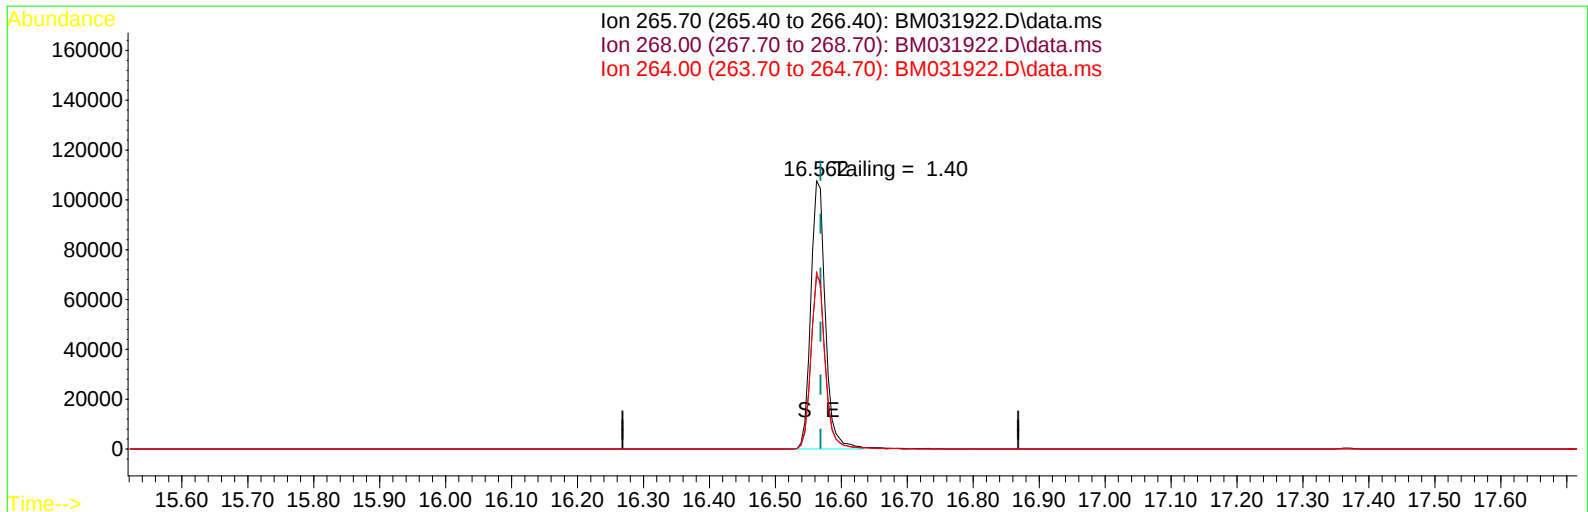

TIC: BM031922.D\data.ms

(70) Pentachlorophenol (C)

16.562min (-0.006) 42890.14 ng

response 166215

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.35
264.00	65.10	66.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/27/2021	BNA_M	<u>BM031922.D</u>
Compound Name	Response	Retention Time
DDT	526761	20.41
DDD	5953	19.98
DDE	1250	19.46
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7203	533964	1.35