
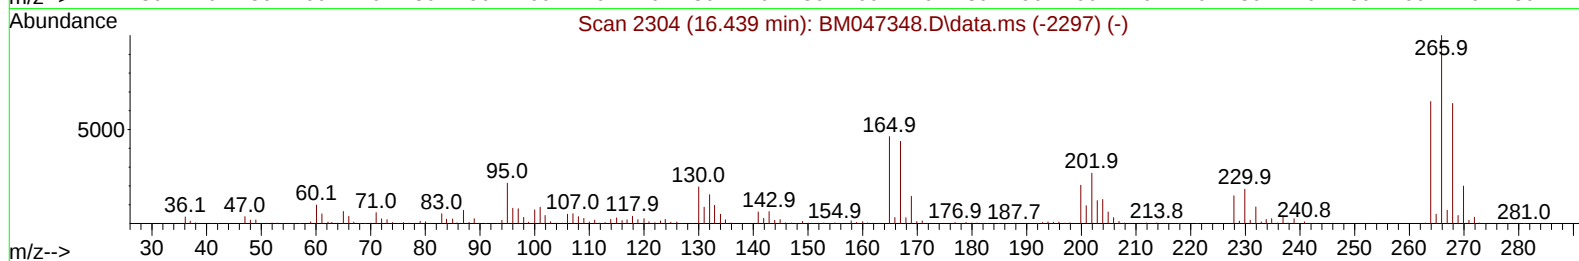
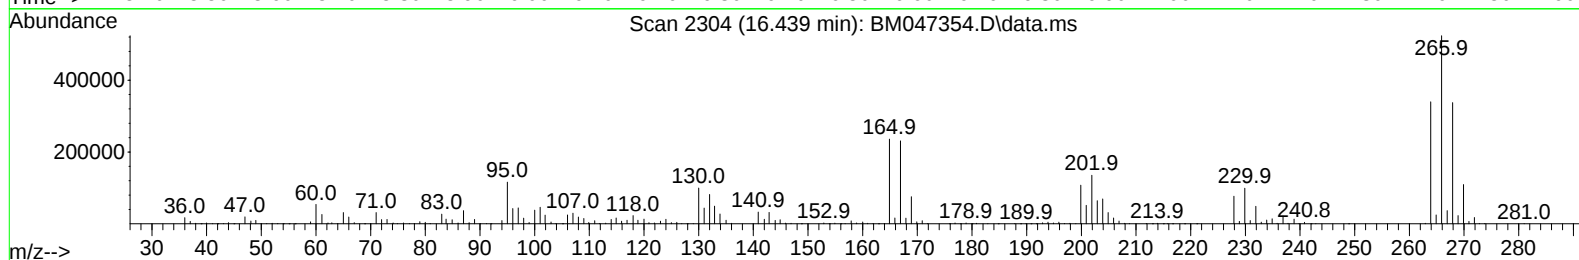


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082724\
Data File : BM047354.D
Acq On : 27 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 11:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

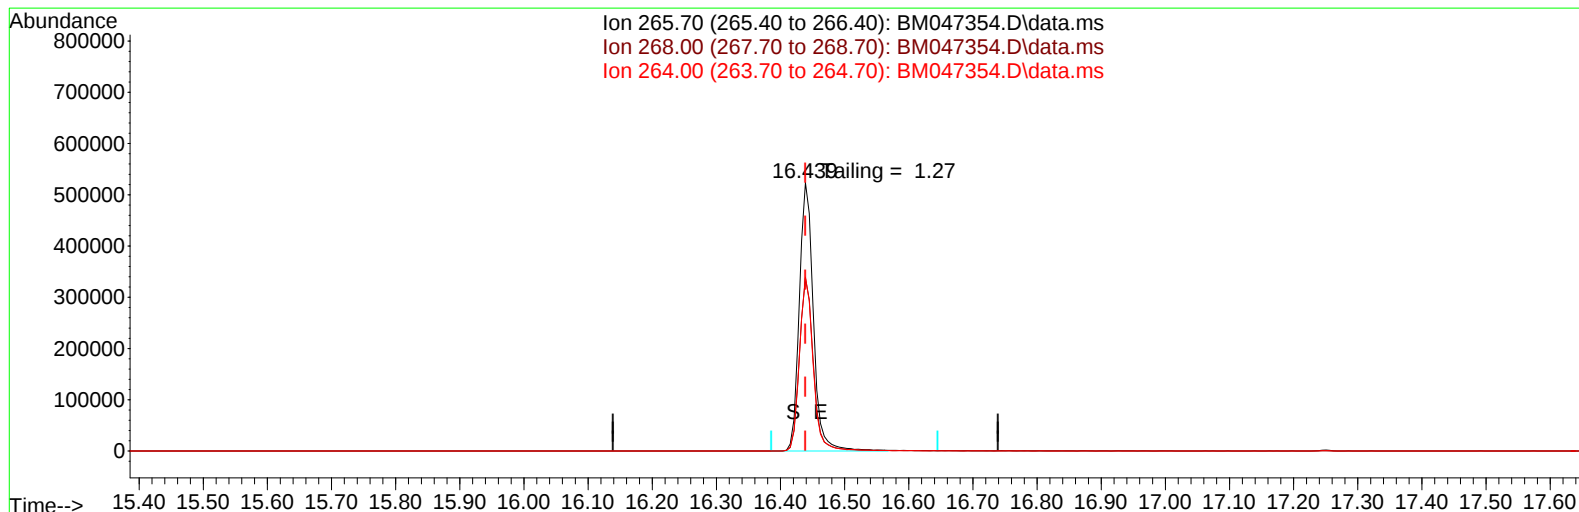

TIC: BM047354.D\data.ms

(70) Pentachlorophenol (C)




16.439min (-0.000) 214021.70 ng m

response 797479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.45
264.00	64.90	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082724\
Data File : BM047354.D
Acq On : 27 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 11:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

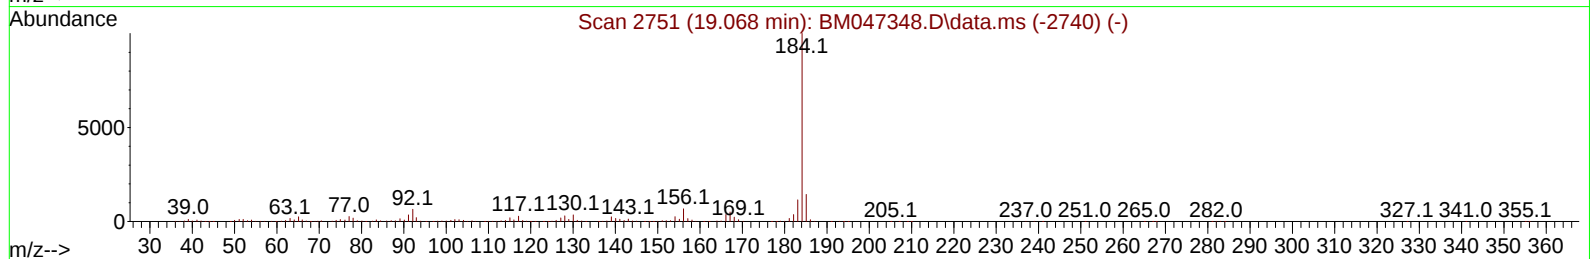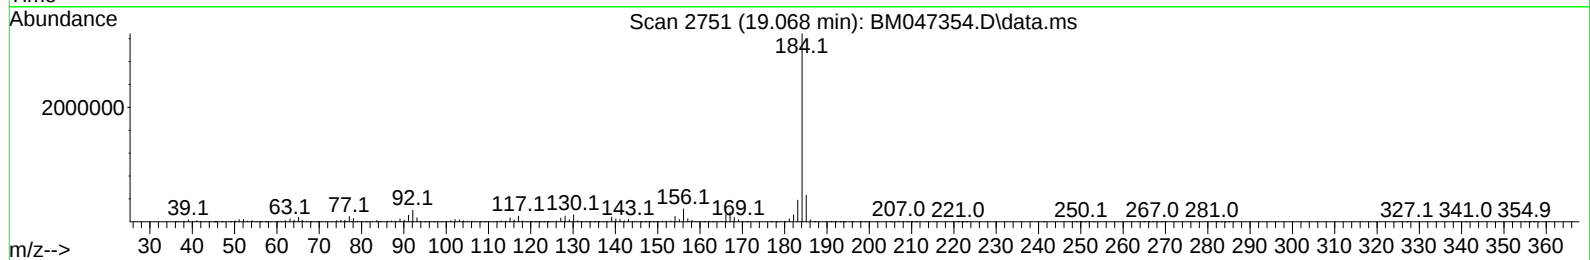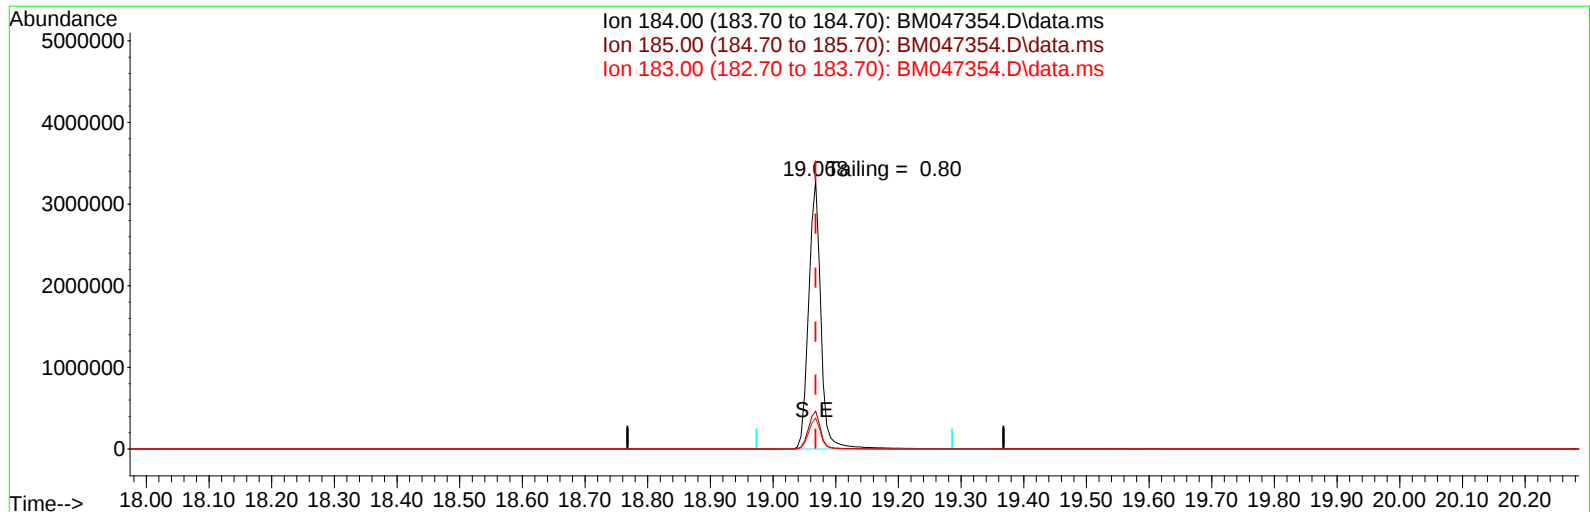

TIC: BM047354.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 7735.93 ng

response 4463653

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.50	11.51
0.00	0.00	0.00