
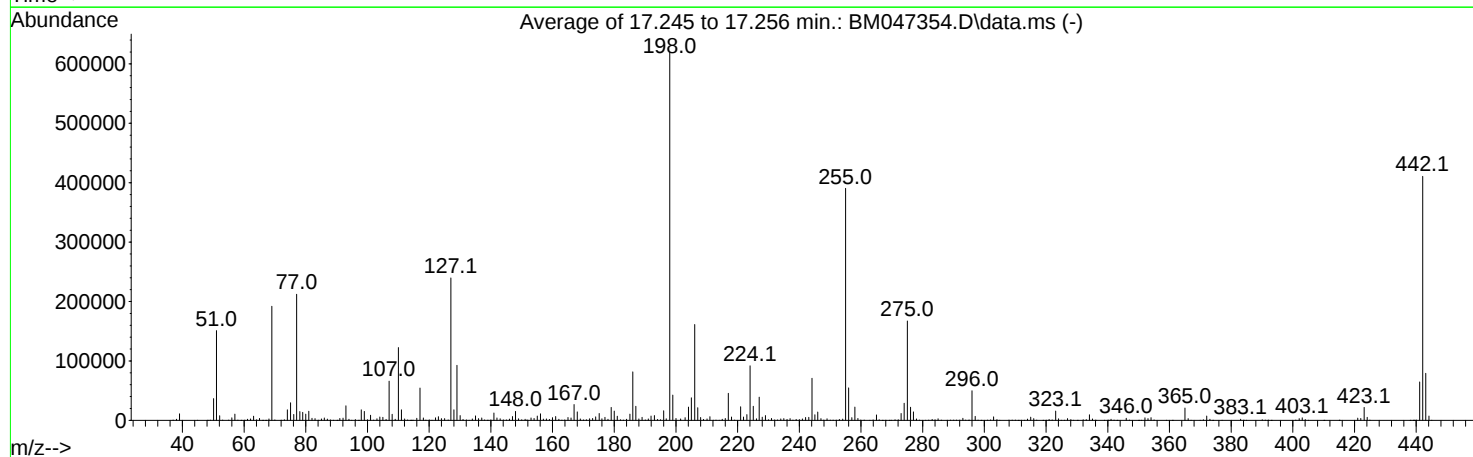


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082724\
Data File : BM047354.D
Acq On : 27 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 26 18:11:40 2024

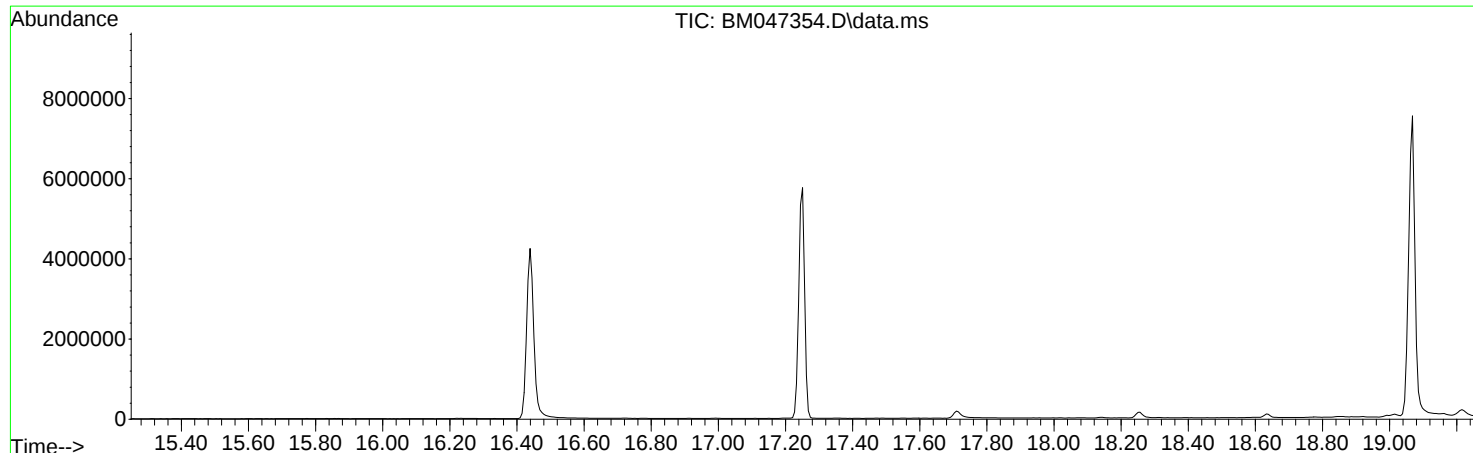

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	150964	PASS
68	69	0.00	2	1.3	2490	PASS
69	198	0.00	100	31.0	191997	PASS
70	69	0.00	2	0.4	716	PASS
127	198	10	80	38.7	239637	PASS
197	198	0.00	2	0.4	2666	PASS
198	198	100	100	100.0	619115	PASS
199	198	5	9	6.9	42691	PASS
275	198	10	60	27.0	167229	PASS
365	198	1	100	3.4	20821	PASS
441	198	0.01	100	10.4	64547	PASS
442	442	50	100	100.0	410731	PASS
443	442	15	24	19.3	79144	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/27/2024	BNA_M	<u>BM047354.D</u>
Compound Name	Response	Retention Time
DDT	2245651	20.309
DDD	35318	19.915
DDE	2238	19.35
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37556	2283207	1.64

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082724\
Data File : BM047354.D
Acq On : 27 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

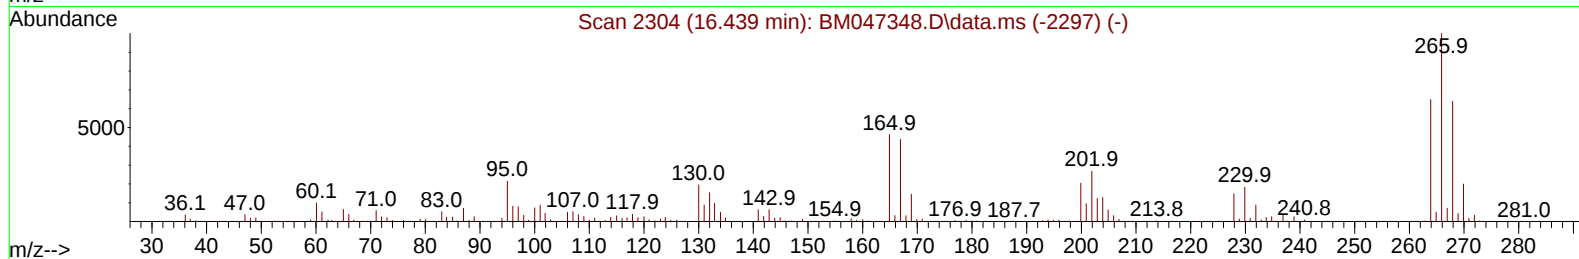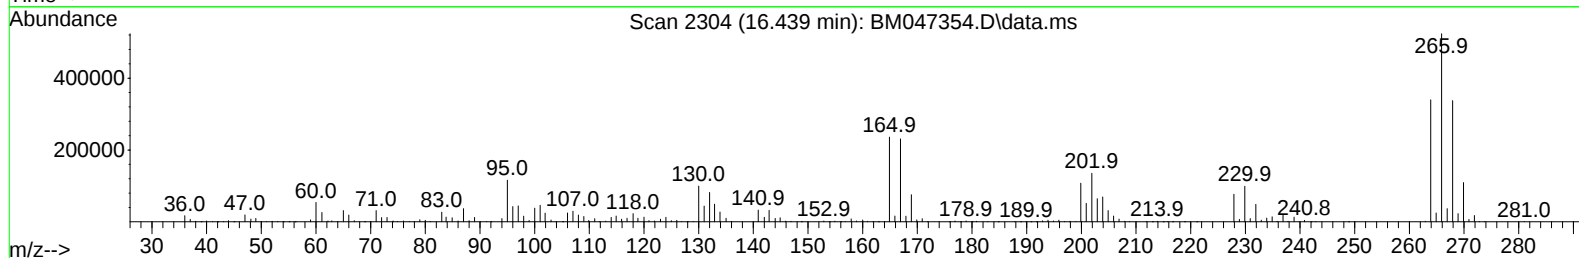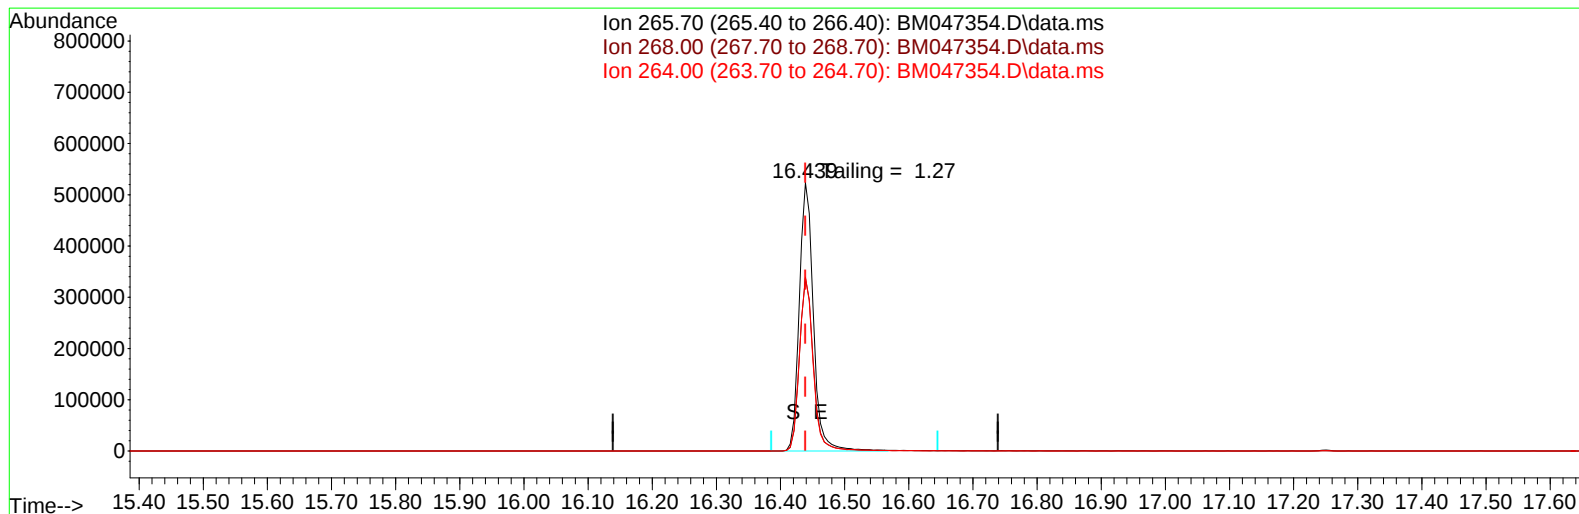

TIC: BM047354.D\data.ms

(70) Pentachlorophenol (C)

16.439min (-0.000) 214021.70 ng m




response 797479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.45
264.00	64.90	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082724\
Data File : BM047354.D
Acq On : 27 Aug 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 27 11:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

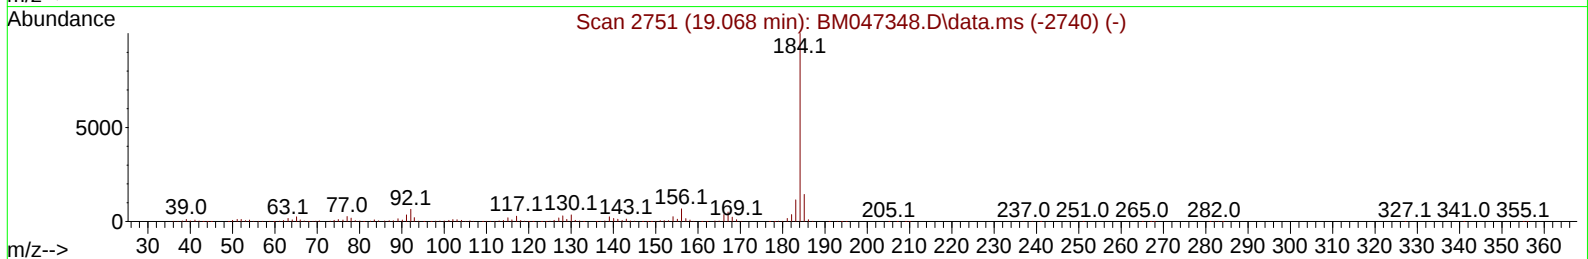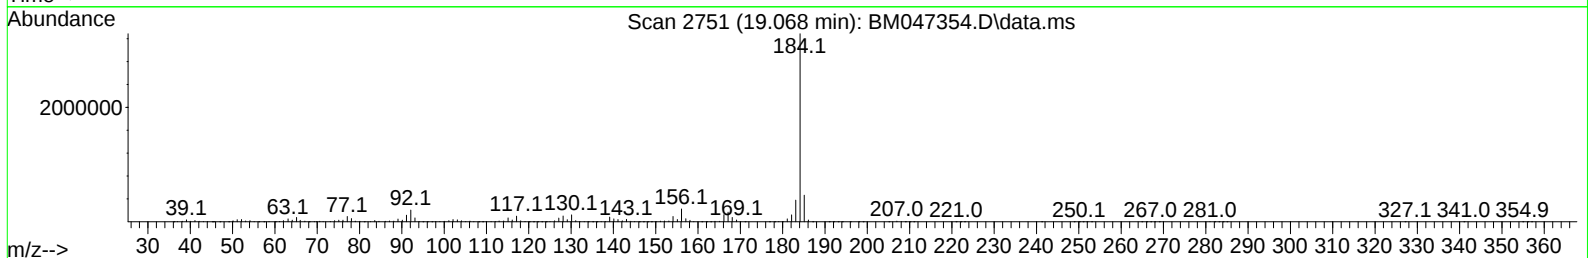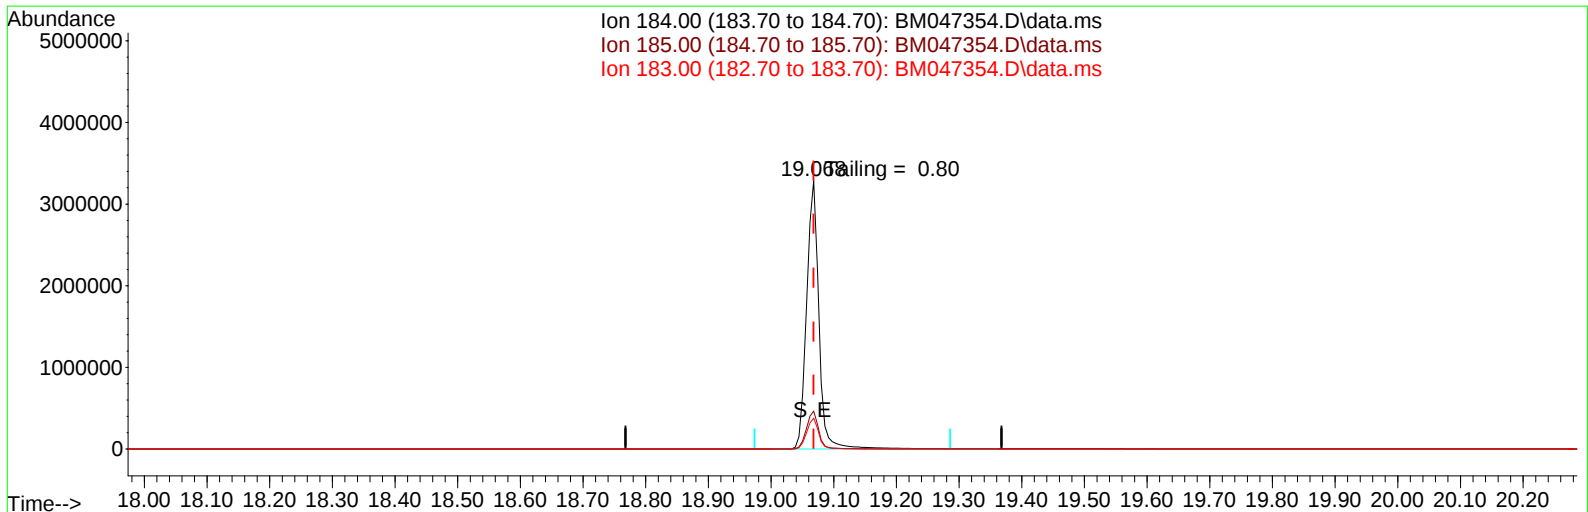

TIC: BM047354.D\data.ms

(77) Benzidine

19.068min (+ 0.000) 7735.93 ng

response 4463653

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.50	11.51
0.00	0.00	0.00