


Data Path : Z:\HPCHEM1\BNA M\DATA\BM082817\
 Data File : BM011357.D
 Acq On : 28 Aug 2017 12:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM082817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 28 17:45:40 2017

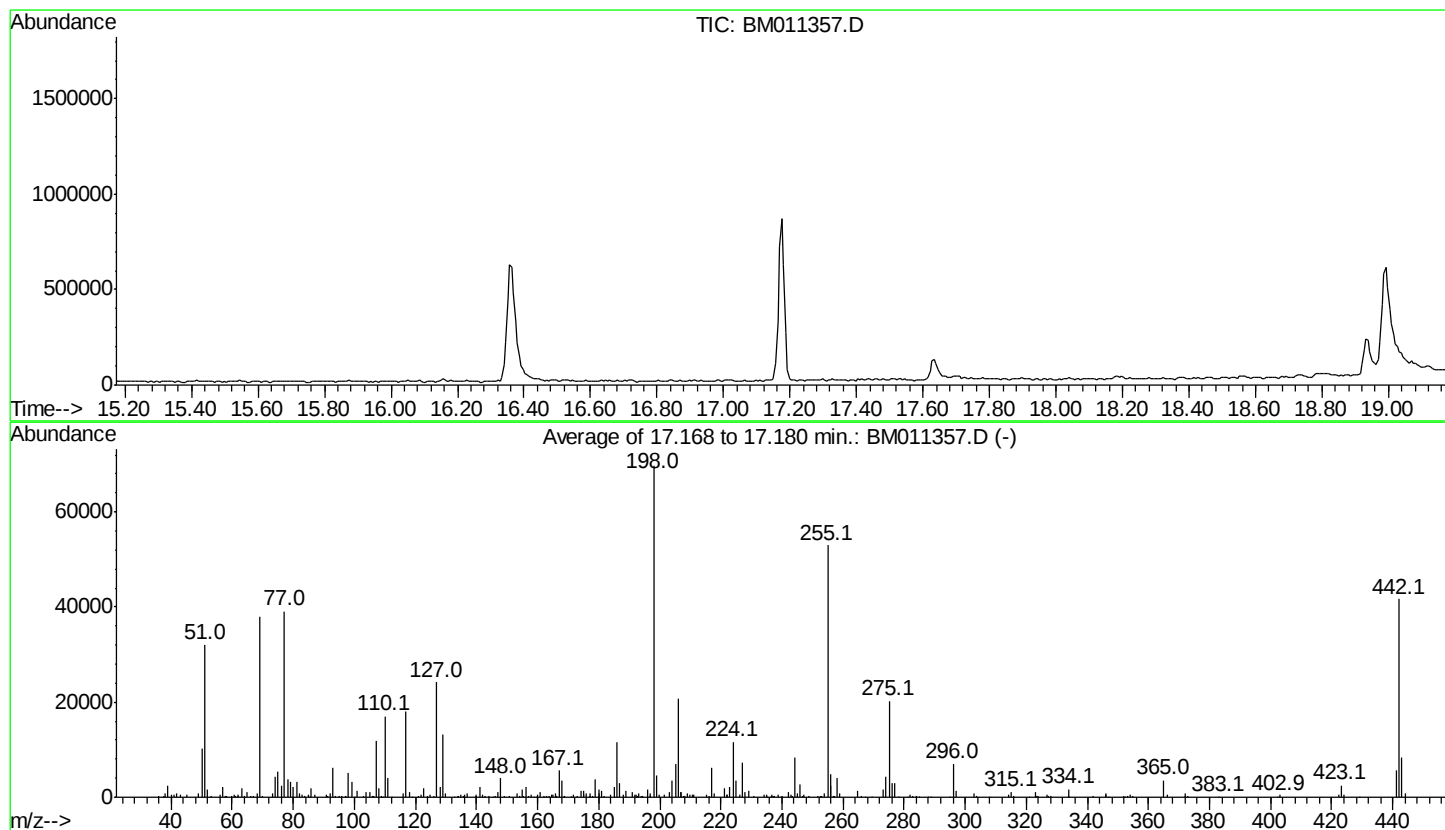

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	32080	PASS
68	69	0.00	2	1.9	728	PASS
69	198	0.00	100	54.5	38040	PASS
70	69	0.00	2	0.9	356	PASS
127	198	10	80	34.7	24224	PASS
197	198	0.00	2	1.0	700	PASS
198	198	100	100	100.0	69741	PASS
199	198	5	9	6.7	4676	PASS
275	198	10	60	29.0	20227	PASS
365	198	1	100	5.1	3573	PASS
441	443	0.01	100	67.3	5571	PASS
442	198	50	100	59.8	41712	PASS
443	442	15	24	19.8	8272	PASS