


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
Data File : BM027286.D
Acq On : 28 Aug 2020 11:51
Operator : JU/CG
Sample : L3695-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG072

Manual Integrations
APPROVED

mohammad
8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:23:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 10:39:41 2020
Response via : Initial Calibration

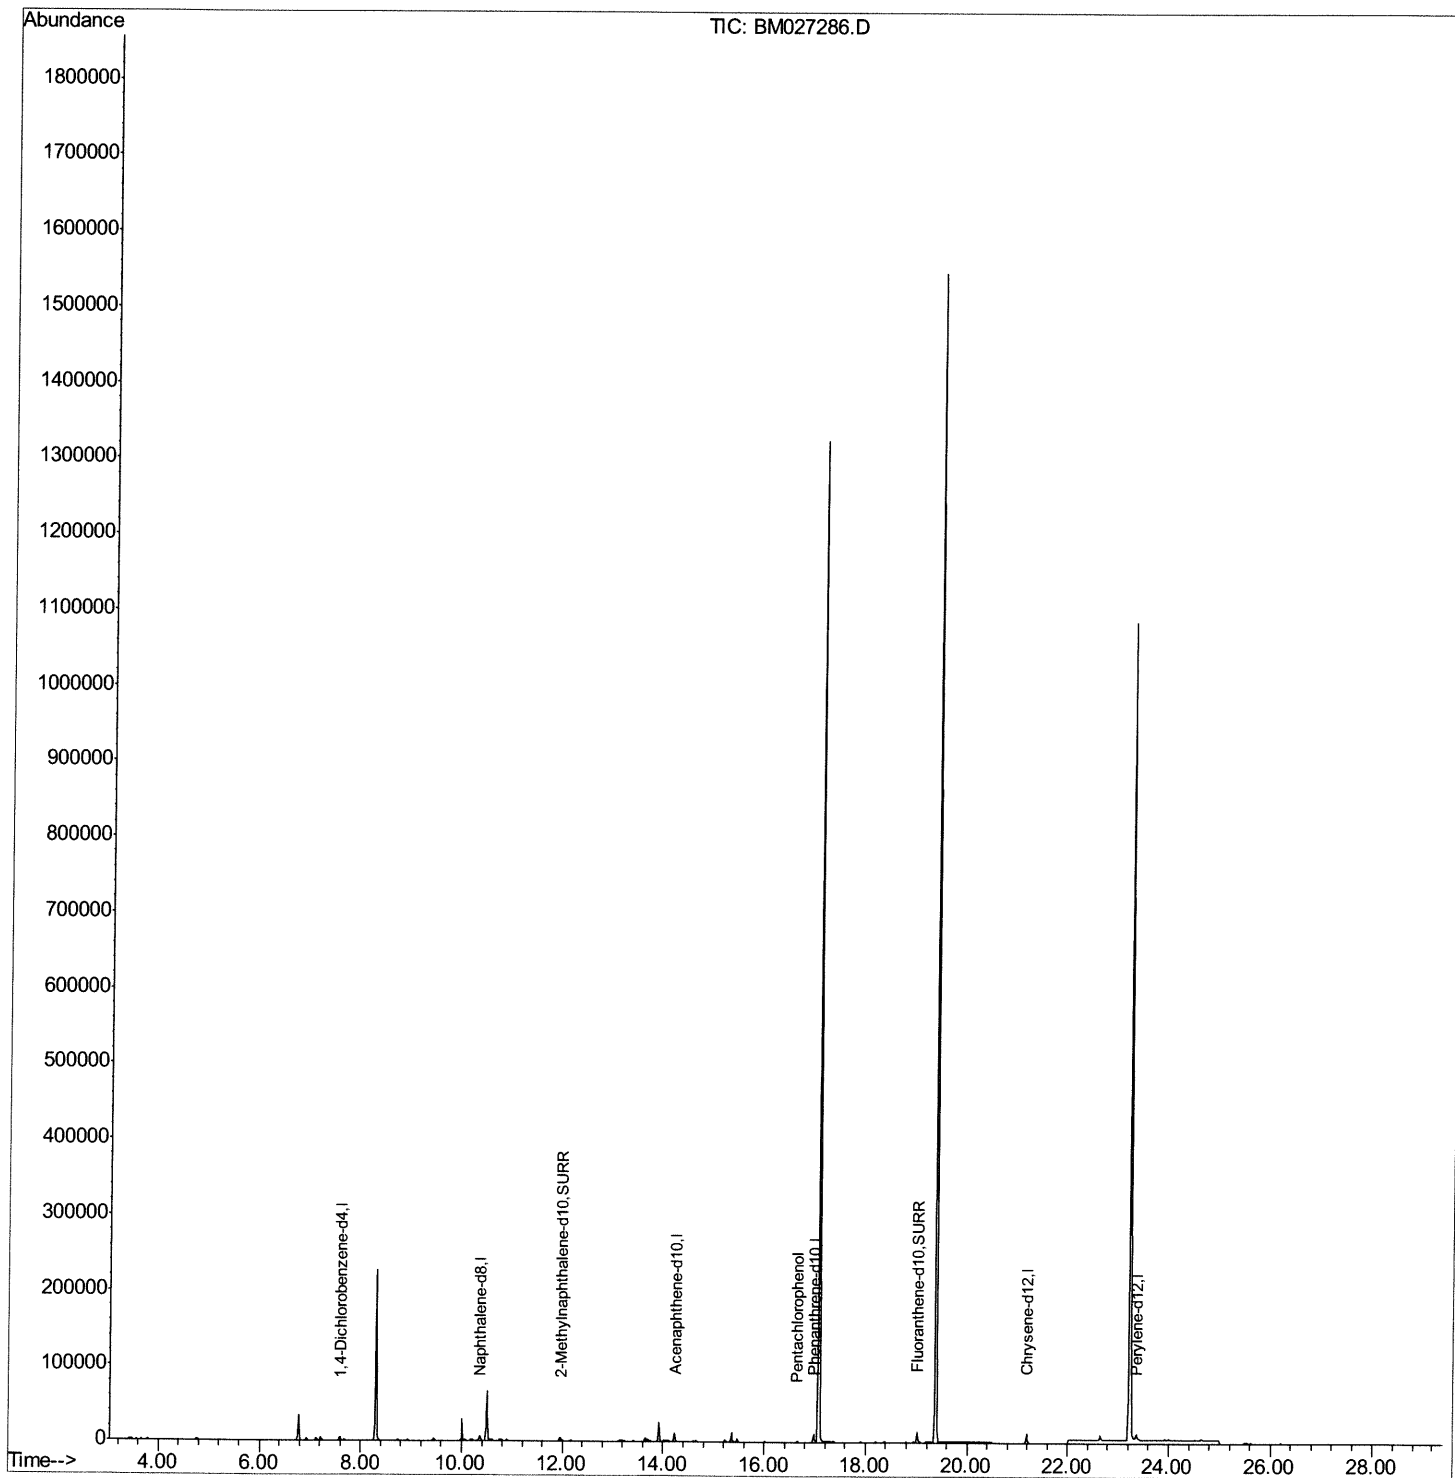

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
 Data File : BM027286.D
 Acq On : 28 Aug 2020 11:51
 Operator : JU/CG
 Sample : L3695-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG072

Manual Integrations
 APPROVED

mohammad
 8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:21:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 10:39:41 2020
 Response via : Initial Calibration

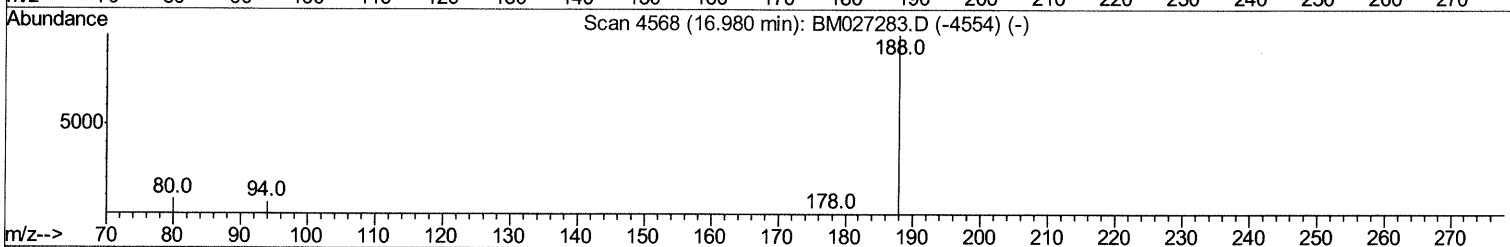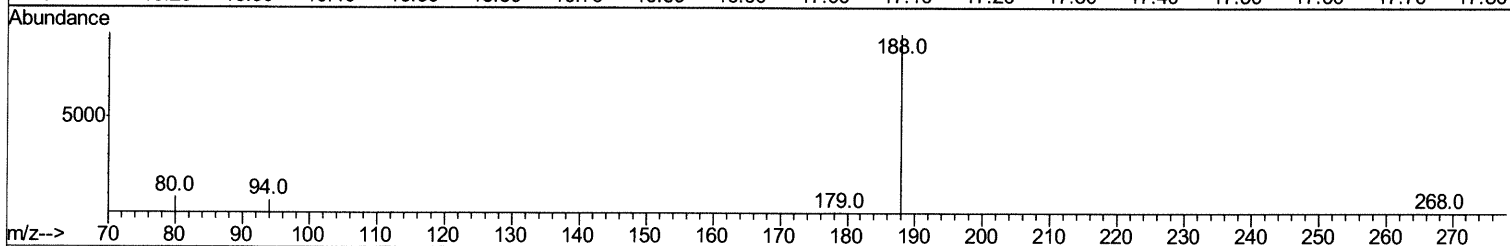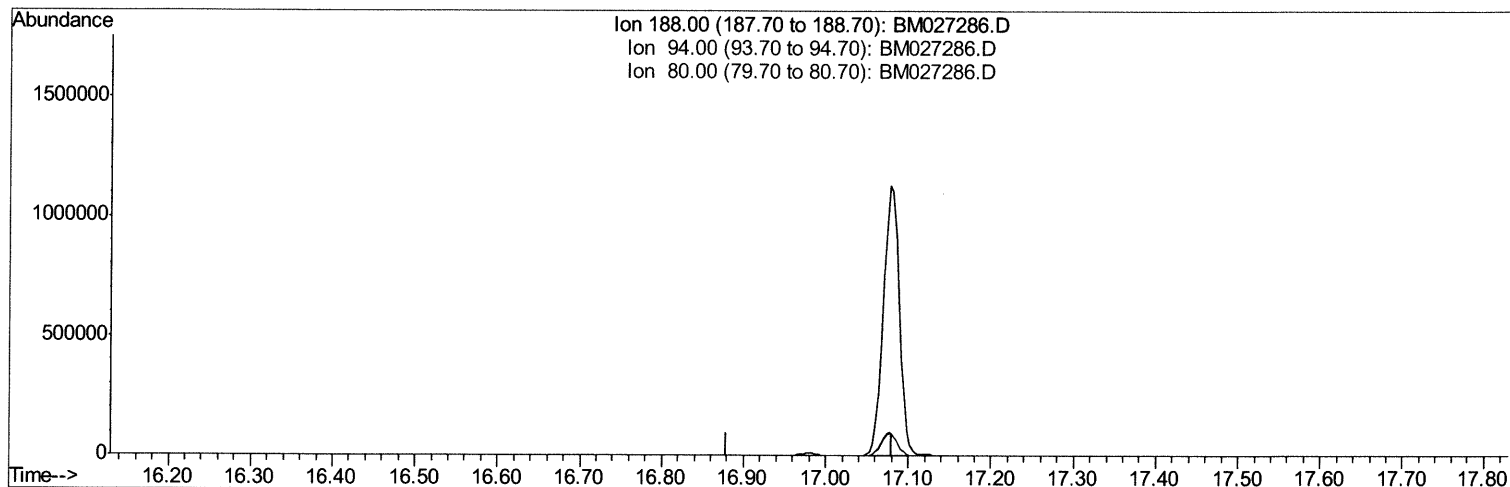

TIC: BM027286.D

(10) Phenanthrene-d10 (I)

16.980min (-16.980) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.80	0.00#
80.00	9.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
Data File : BM027286.D
Acq On : 28 Aug 2020 11:51
Operator : JU/CG
Sample : L3695-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG072

Manual Integrations
APPROVED

mohammad
8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:21:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 10:39:41 2020
Response via : Initial Calibration

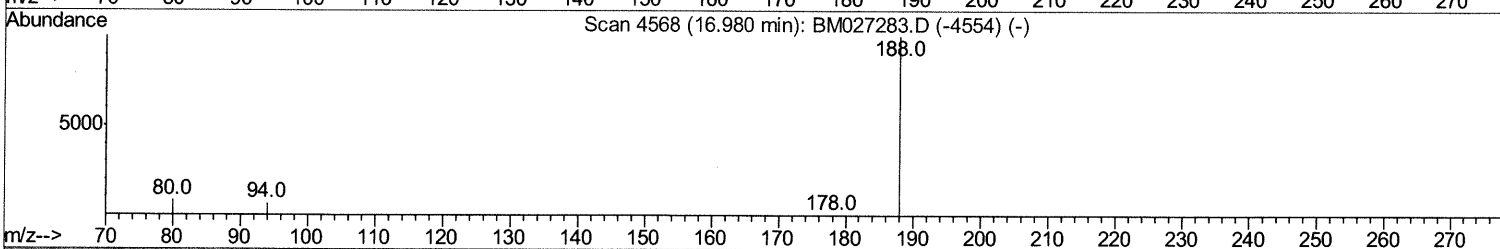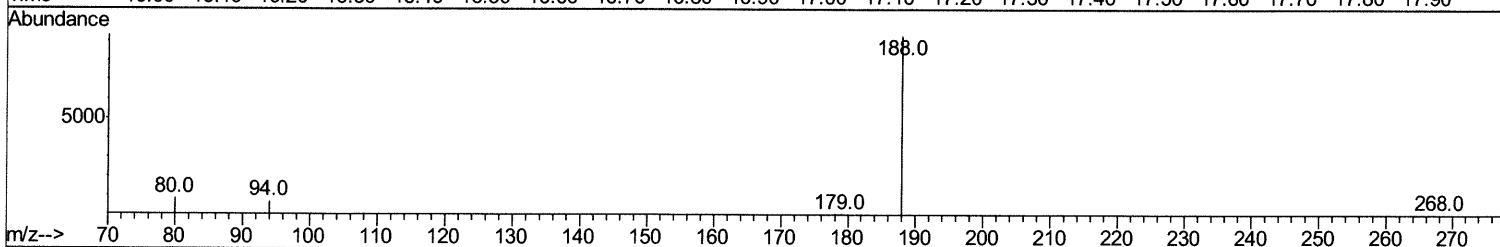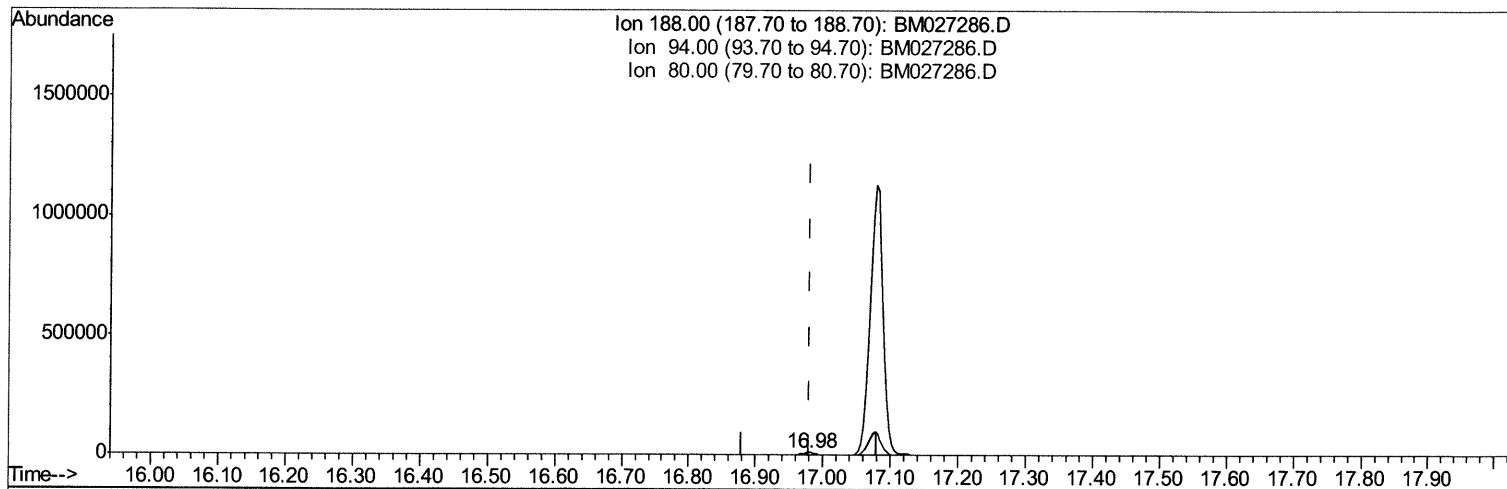

TIC: BM027286.D

(10) Phenanthrene-d10 (I)

16.980min (-0.000) 0.40ng/ul m

08/31/20 JU

response 12903

Ion	Exp%	Act%
188.00	100	100
94.00	7.80	7.56
80.00	9.00	9.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
 Data File : BM027286.D
 Acq On : 28 Aug 2020 11:51
 Operator : JU/CG
 Sample : L3695-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG072

Manual Integrations
 APPROVED

mohammad
 8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:23:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 10:39:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2346	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	8342	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	5858	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	12903m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.19	240	11420	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	10303	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	6717	0.48	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	16593	0.45	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.64	266	512	0.120	ng/ul	Ovalue 95

08/31/20 JU

(#) = qualifier out of range (m) = manual integration (+) = signals summed