

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082820\
 Data File : BM027286.D
 Acq On : 28 Aug 2020 11:51
 Operator : JU/CG
 Sample : L3695-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG072

Manual Integrations
 APPROVED

mohammad
 8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:23:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 10:39:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2346	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	8342	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	5858	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.98	188	12903m	0.40	ng/ul	0.00
16) Chrysene-d12	21.19	240	11420	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	10303	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	6717	0.48	ng/ul	0.00
14) Fluoranthene-d10	19.01	212	16593	0.45	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.64	266	512	0.120	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082820\
Data File : BM027286.D
Acq On : 28 Aug 2020 11:51
Operator : JU/CG
Sample : L3695-02
Misc :
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BG072

Manual Integrations
APPROVED

mohammad
8/31/2020 11:14:30 AM

Quant Time: Aug 28 12:23:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 10:39:41 2020
Response via : Initial Calibration

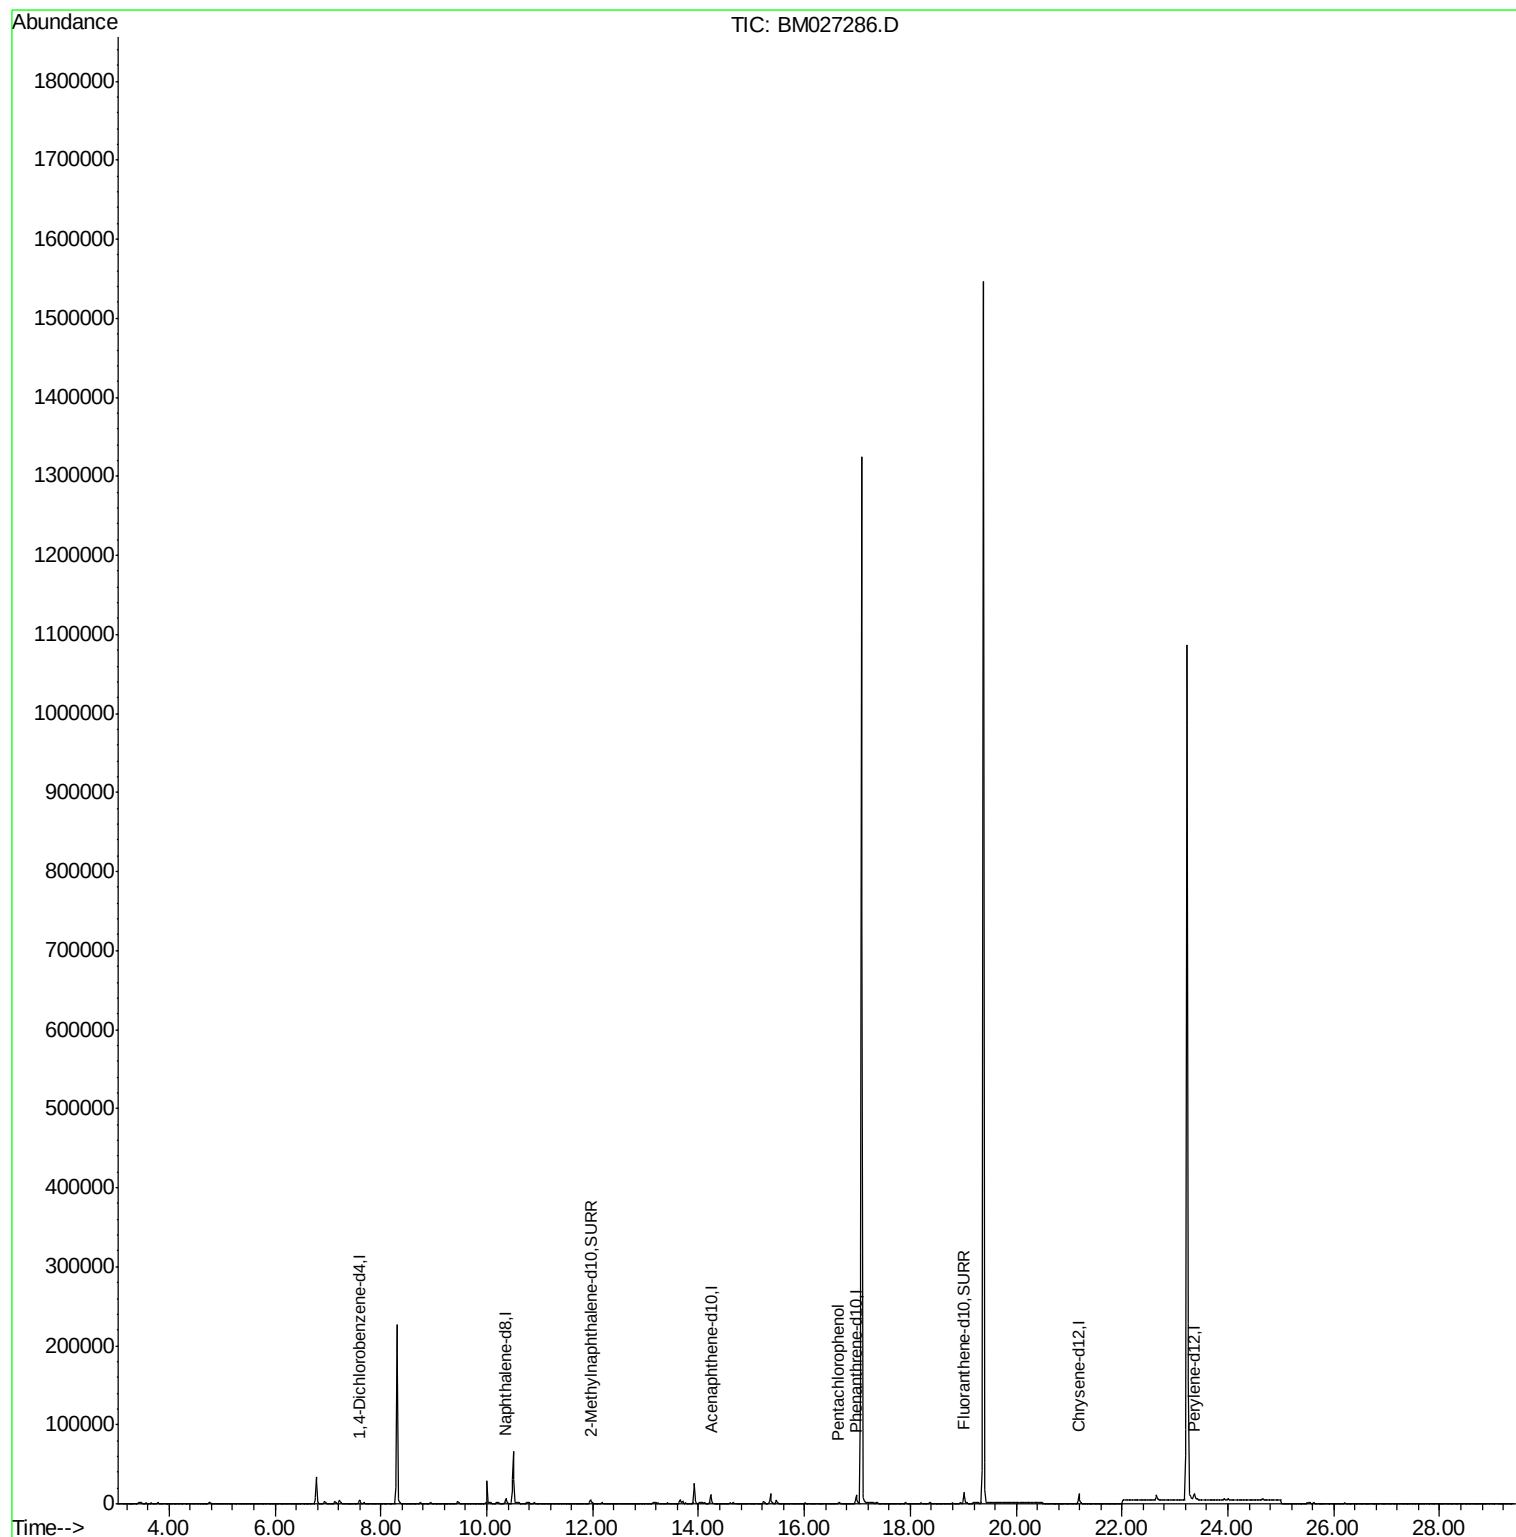

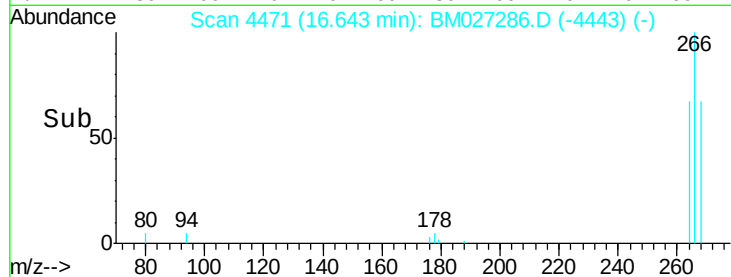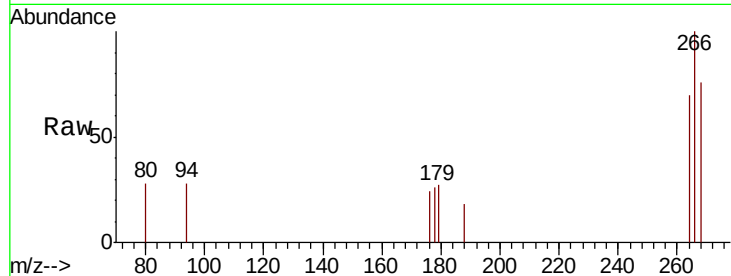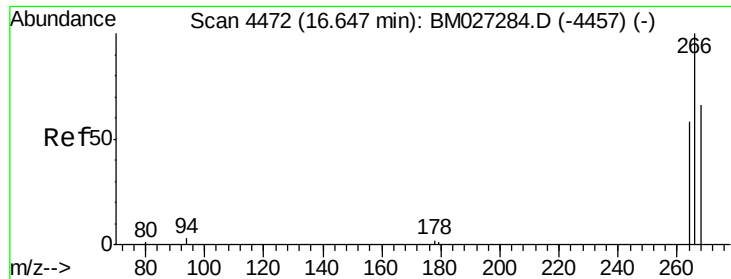

#11
 Pentachlorophenol
 Concen: 0.120 ng/ul
 RT: 16.64 min Scan# 4471
 Delta R.T. -0.00 min
 Lab File: BM027286.D
 Acq: 28 Aug 2020 11:51

Instrument :
 BNA_M
 ClientSampleId :
 BG072

Tot Ion:	266	Resp:	512
Ion Ratio	Lower	Upper	
266	100		
264	62.5	47.8	71.8
268	65.2	48.5	72.7

Manual Integrations
 APPROVED

mohammad
 8/31/2020 11:14:30 AM

