


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082915\
Data File : BM002559.D
Acq On : 29 Aug 2015 11:47
Operator : UM/IZ
Sample : DFTPP08
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP08

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Title : SVOA CALIBRATION
Last Update : Mon Aug 31 14:08:41 2015

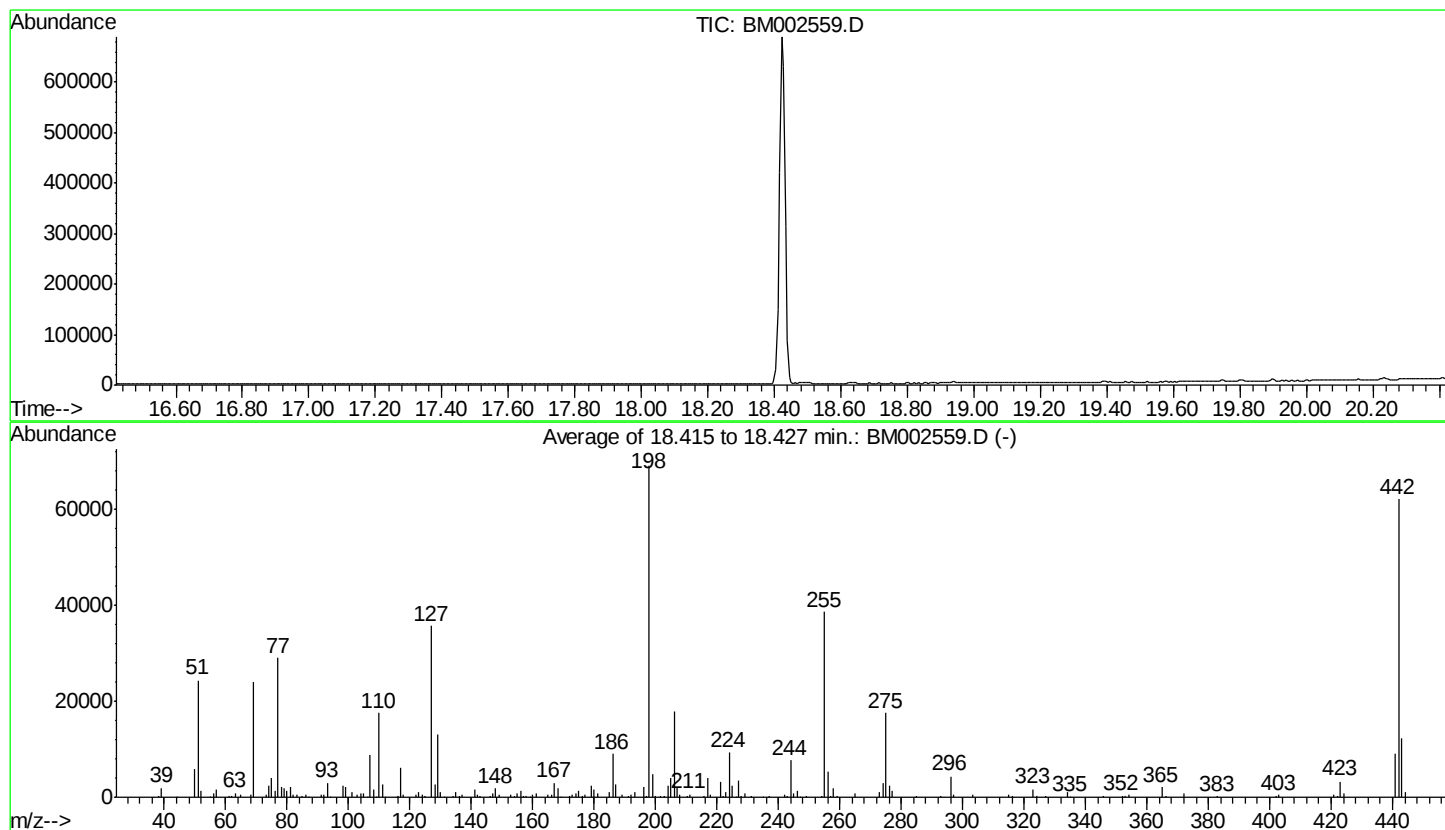

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	24256	PASS
68	69	0.00	2	1.9	467	PASS
69	198	0.00	100	34.8	24000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	35664	PASS
197	198	0.00	2	0.5	363	PASS
198	198	100	100	100.0	69045	PASS
199	198	5	9	6.8	4677	PASS
275	198	10	60	25.4	17534	PASS
365	198	1	100	3.1	2114	PASS
441	443	0.01	100	75.0	9153	PASS
442	198	50	100	89.8	62029	PASS
443	442	15	24	19.7	12207	PASS

m/z	Abundance
38.00	307.0
39.10	1717.0
40.00	692.0
44.00	2194.0
50.00	5166.0
51.10	21008.0
52.00	1061.0
56.00	680.0
57.00	1610.0
62.00	343.0
63.00	767.0
65.00	401.0
68.00	411.0
69.00	20440.0
73.00	405.0
74.00	2097.0
75.00	3330.0
76.10	1118.0
77.10	24000.0
78.00	1893.0
79.00	1558.0
80.00	1201.0
81.00	1829.0
82.00	425.0
83.00	419.0
85.90	482.0
91.00	437.0
92.00	561.0
93.00	2520.0
98.00	1783.0
99.00	1873.0
101.00	965.0
103.00	403.0
104.00	577.0
105.00	641.0
107.00	7416.0
108.00	1343.0
110.00	14228.0
111.00	2439.0
112.00	373.0
115.80	372.0
117.00	4814.0
117.90	458.0
121.90	512.0
122.90	848.0
124.10	306.0
125.10	324.0
127.00	27672.0
128.00	2104.0
129.00	10447.0
130.00	792.0
134.90	819.0
135.90	359.0
137.00	551.0
141.00	1316.0
142.00	413.0
147.00	720.0
148.00	1399.0
149.00	340.0
152.80	355.0
153.90	326.0
155.00	733.0
156.00	1018.0
160.00	518.0
161.00	589.0
165.00	381.0
166.00	302.0
167.00	2354.0
168.00	1699.0
172.90	320.0
174.00	512.0
175.00	1111.0
176.90	447.0
178.90	1716.0
180.00	1289.0
180.90	586.0
185.00	838.0
186.00	6559.0
187.00	1831.0
188.90	386.0
192.00	557.0
193.00	648.0
196.00	1387.0
196.80	368.0
198.00	50736.0
198.90	3606.0
204.00	1768.0
205.00	2780.0
206.00	13133.0
207.00	2357.0
207.90	575.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

211.00	539.0
217.00	2861.0
218.00	372.0
220.90	2336.0
222.00	480.0
223.00	657.0
224.00	6905.0
225.00	1696.0
227.00	2302.0
229.00	616.0
242.00	382.0
244.00	5352.0
245.00	591.0
245.90	822.0
255.00	26672.0
256.00	3927.0
258.00	1399.0
264.90	452.0
273.00	802.0
274.00	2211.0
275.00	11674.0
276.00	1583.0
276.90	949.0
296.00	3053.0
297.00	430.0
303.00	361.0
315.00	401.0
323.00	1107.0
334.00	767.0
354.10	347.0
364.90	1288.0
372.00	574.0
402.90	315.0
423.00	1793.0
424.00	516.0
441.00	5007.0
442.00	33944.0
443.00	6704.0
444.00	561.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

m/z	Abundance
37.90	431.0
39.00	2426.0
40.00	668.0
44.00	2199.0
50.00	7157.0
51.00	28776.0
52.00	1440.0
55.00	313.0
56.00	823.0
57.00	2031.0
60.90	313.0
62.00	441.0
63.00	1083.0
65.00	663.0
68.00	566.0
69.00	28432.0
73.10	409.0
74.00	2943.0
75.00	4864.0
76.00	1620.0
77.10	34560.0
78.00	2725.0
79.00	2095.0
80.00	1458.0
81.00	2318.0
82.00	528.0
83.00	671.0
85.00	476.0
86.00	678.0
86.90	353.0
91.00	628.0
91.90	645.0
93.00	3433.0
94.00	312.0
98.00	2874.0
99.00	2509.0
101.00	1398.0
102.90	459.0
104.00	830.0
105.00	831.0
107.00	10713.0
108.00	1754.0
109.20	315.0
110.00	21064.0
111.00	3185.0
116.00	633.0
117.00	7164.0
118.00	571.0
122.00	709.0
123.00	1099.0
124.00	536.0
124.90	429.0
127.00	42944.0
128.00	3337.0
129.00	15595.0
130.00	1357.0
131.00	306.0
133.90	398.0
135.00	1376.0
135.90	450.0
136.90	813.0
141.00	2036.0
142.00	606.0
142.80	397.0
145.90	393.0
147.00	1192.0
147.90	2082.0
149.00	549.0
152.90	596.0
153.90	473.0
155.00	1148.0
156.00	1630.0
157.00	446.0
157.80	344.0
159.10	334.0
159.90	656.0
161.00	945.0
165.00	888.0
166.00	535.0
167.00	3817.0
168.00	2183.0
169.00	373.0
171.90	393.0
173.00	445.0
174.00	830.0
175.00	1696.0
176.00	498.0
177.00	629.0
179.00	2804.0
180.00	1839.0
181.00	1033.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

185.00	1340.0
186.00	10797.0
187.00	3345.0
188.90	740.0
191.00	365.0
192.00	732.0
193.00	1129.0
196.00	2624.0
197.00	554.0
197.90	81280.0
198.90	5541.0
200.00	455.0
201.60	354.0
203.00	520.0
204.00	2666.0
205.00	4724.0
206.00	20952.0
207.00	3172.0
207.90	750.0
210.30	484.0
210.90	750.0
215.90	386.0
217.00	4871.0
218.00	769.0
221.00	3827.0
221.80	691.0
223.00	1198.0
224.00	10777.0
225.00	2708.0
226.10	366.0
227.00	4327.0
228.00	610.0
229.00	1016.0
231.00	435.0
235.00	354.0
237.00	392.0
242.00	597.0
243.00	631.0
244.10	9022.0
245.00	1136.0
245.90	1519.0
247.00	359.0
248.90	411.0
254.10	406.0
255.00	45424.0
256.00	6467.0
256.90	603.0
258.00	2174.0
259.00	363.0
265.00	937.0
273.00	1305.0
274.00	3378.0
275.00	20488.0
276.00	2766.0
276.90	1553.0
285.00	301.0
293.00	359.0
296.00	5132.0
296.90	692.0
303.00	680.0
315.00	587.0
316.00	385.0
323.00	2022.0
324.00	356.0
326.90	338.0
334.00	1042.0
346.00	350.0
351.90	430.0
352.90	301.0
354.00	655.0
364.90	2362.0
366.00	337.0
372.00	877.0
383.00	313.0
402.00	391.0
402.90	657.0
421.00	625.0
422.00	527.0
423.00	3966.0
424.00	989.0
441.00	10425.0
442.00	70128.0
443.00	13888.0
444.00	1144.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

m/z	Abundance
39.00	1765.0
39.90	628.0
44.00	2126.0
50.00	5413.0
51.00	22984.0
52.00	1133.0
56.00	696.0
57.00	1569.0
60.90	328.0
63.00	842.0
65.00	471.0
68.00	424.0
69.00	23128.0
73.00	515.0
74.00	2077.0
75.00	3631.0
76.10	1335.0
77.10	28296.0
78.00	1897.0
79.00	1900.0
79.90	1429.0
81.00	1949.0
82.00	527.0
83.00	475.0
85.00	355.0
86.00	567.0
90.90	521.0
92.00	503.0
93.00	3085.0
98.00	2191.0
99.00	1941.0
101.00	1113.0
103.00	380.0
103.90	638.0
104.90	689.0
105.90	311.0
107.00	8584.0
108.00	1509.0
110.00	17392.0
111.00	2620.0
116.00	551.0
117.00	6050.0
117.90	375.0
121.90	734.0
123.00	993.0
124.00	440.0
124.90	327.0
127.00	36376.0
128.00	2660.0
129.00	12791.0
129.90	972.0
133.90	416.0
135.00	1208.0
136.00	424.0
136.90	542.0
141.00	1556.0
142.00	549.0
142.90	377.0
146.00	300.0
147.00	776.0
148.00	1847.0
148.90	431.0
152.90	538.0
153.90	419.0
155.00	874.0
156.00	1534.0
157.00	363.0
157.90	308.0
159.90	489.0
161.00	827.0
165.00	661.0
165.80	424.0
167.00	2853.0
168.00	1964.0
171.90	302.0
172.90	488.0
174.00	727.0
174.90	1313.0
175.90	469.0
176.90	595.0
179.00	2558.0
180.00	1785.0
180.90	836.0
185.00	1161.0
186.00	9696.0
187.00	2499.0
188.90	700.0
190.90	390.0
192.00	710.0
193.10	1100.0
196.00	2508.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

197.10	536.0
197.90	75120.0
198.90	4886.0
199.90	391.0
201.40	389.0
203.00	393.0
203.90	2521.0
205.00	4272.0
206.00	19248.0
207.00	2913.0
208.00	603.0
211.10	724.0
215.90	339.0
217.00	4304.0
217.90	547.0
221.00	3466.0
223.00	1043.0
224.00	9956.0
225.00	2545.0
227.00	4025.0
227.90	497.0
229.00	902.0
231.10	399.0
237.00	357.0
241.90	578.0
242.90	570.0
244.00	8455.0
245.00	1096.0
246.00	1520.0
248.90	324.0
254.10	394.0
255.00	43584.0
256.00	5898.0
257.00	493.0
258.00	2317.0
259.00	339.0
265.00	888.0
273.00	1412.0
274.00	3446.0
275.00	20440.0
276.00	2503.0
277.00	1554.0
285.00	300.0
292.90	416.0
296.00	4931.0
297.00	644.0
303.10	666.0
314.90	633.0
316.00	345.0
323.00	2100.0
323.90	316.0
326.90	308.0
334.00	1236.0
335.00	307.0
345.90	367.0
351.90	585.0
353.00	438.0
354.00	782.0
365.00	2693.0
366.00	440.0
372.00	1230.0
383.00	374.0
402.00	543.0
403.00	632.0
420.90	672.0
422.00	691.0
423.00	4069.0
424.00	1074.0
441.00	12027.0
442.00	82016.0
443.00	16031.0
444.00	1289.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

Scan 2601 (18.386 min): BM002559.D
DFTPP08

m/z	Abundance
39.90	679.0
44.00	2124.0
207.00	645.0


Instrument :
BNA_M
ClientSampleId :
DFTPP08

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082915\
 Data File : BM002559.D
 Acq On : 29 Aug 2015 11:47
 Operator : UM/IZ
 Sample : DFTPP08
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP08

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Title : SVOA CALIBRATION
 Last Update : Mon Aug 31 14:08:41 2015

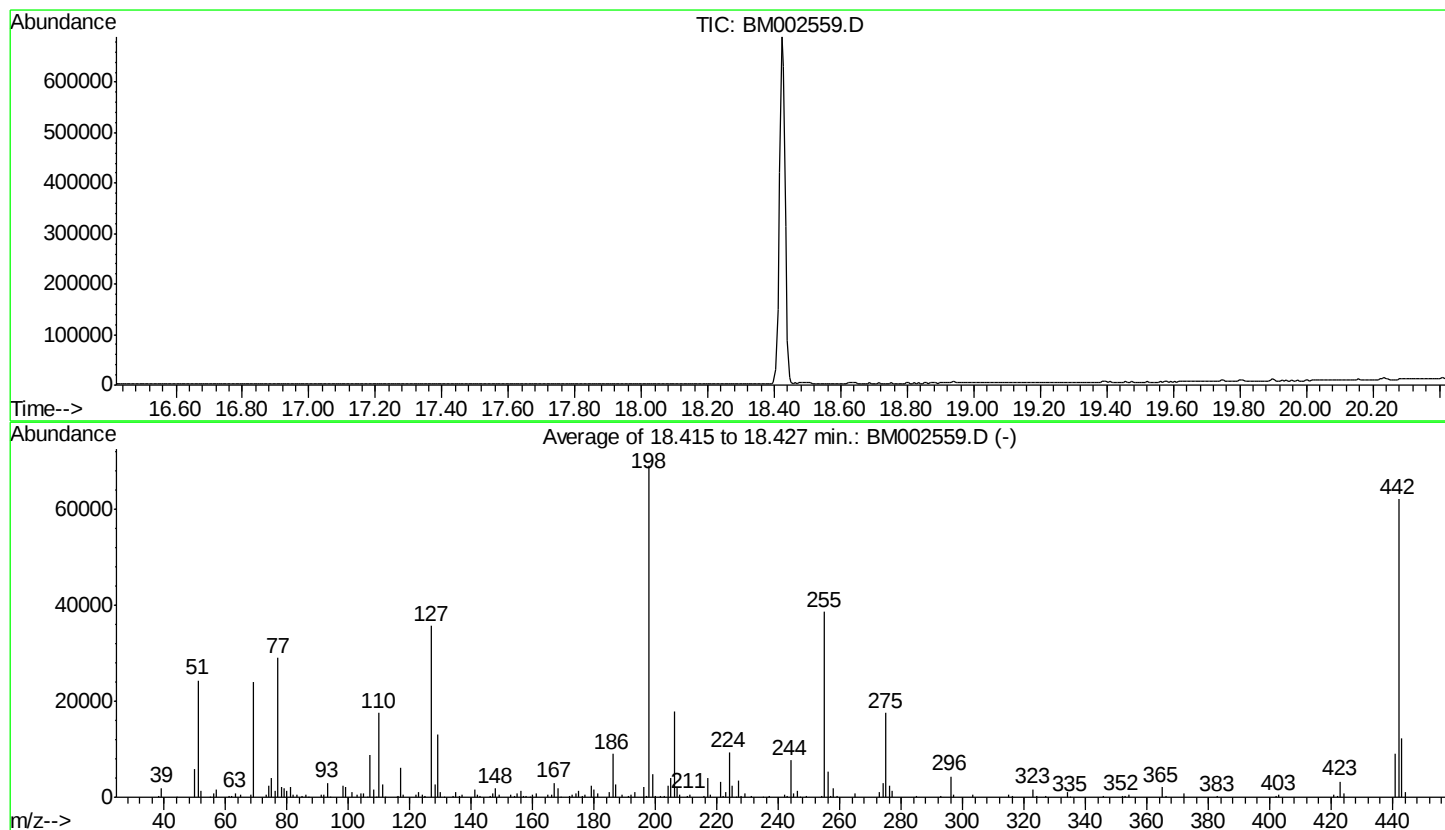

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	24256	PASS
68	69	0.00	2	1.9	467	PASS
69	198	0.00	100	34.8	24000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	35664	PASS
197	198	0.00	2	0.5	363	PASS
198	198	100	100	100.0	69045	PASS
199	198	5	9	6.8	4677	PASS
275	198	10	60	25.4	17534	PASS
365	198	1	100	3.1	2114	PASS
441	443	0.01	100	75.0	9153	PASS
442	198	50	100	89.8	62029	PASS
443	442	15	24	19.7	12207	PASS