

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007312.D
 Acq On : 29 Aug 2016 17:09
 Operator : UM/SJ
 Sample : H4575-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA277

Quant Time: Aug 30 02:26:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 30 02:26:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	127581	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	614173	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	458622	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1315871	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2052853	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2305888	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	7259	2.91	ng/uL	0.00
5) Phenol-d5	6.96	99	154926	12.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	96692	15.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	125725	14.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	137899	13.12	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	66121	14.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	76074	14.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	141906	13.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	133855	10.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	636052	16.08	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	708917	15.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	94222	12.61	ng/ul	0.00
57) Fluorene-d10	15.42	176	559038	16.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	92285	11.15	ng/ul	0.00
70) Anthracene-d10	17.27	188	983971	16.01	ng/ul	0.00
76) Pyrene-d10	19.56	212	1309908	15.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	1682685	15.84	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	478179	12.13	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007312.D
Acq On : 29 Aug 2016 17:09
Operator : UM/SJ
Sample : H4575-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA277

Quant Time: Aug 30 02:26:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 30 02:26:11 2016
Response via : Initial Calibration

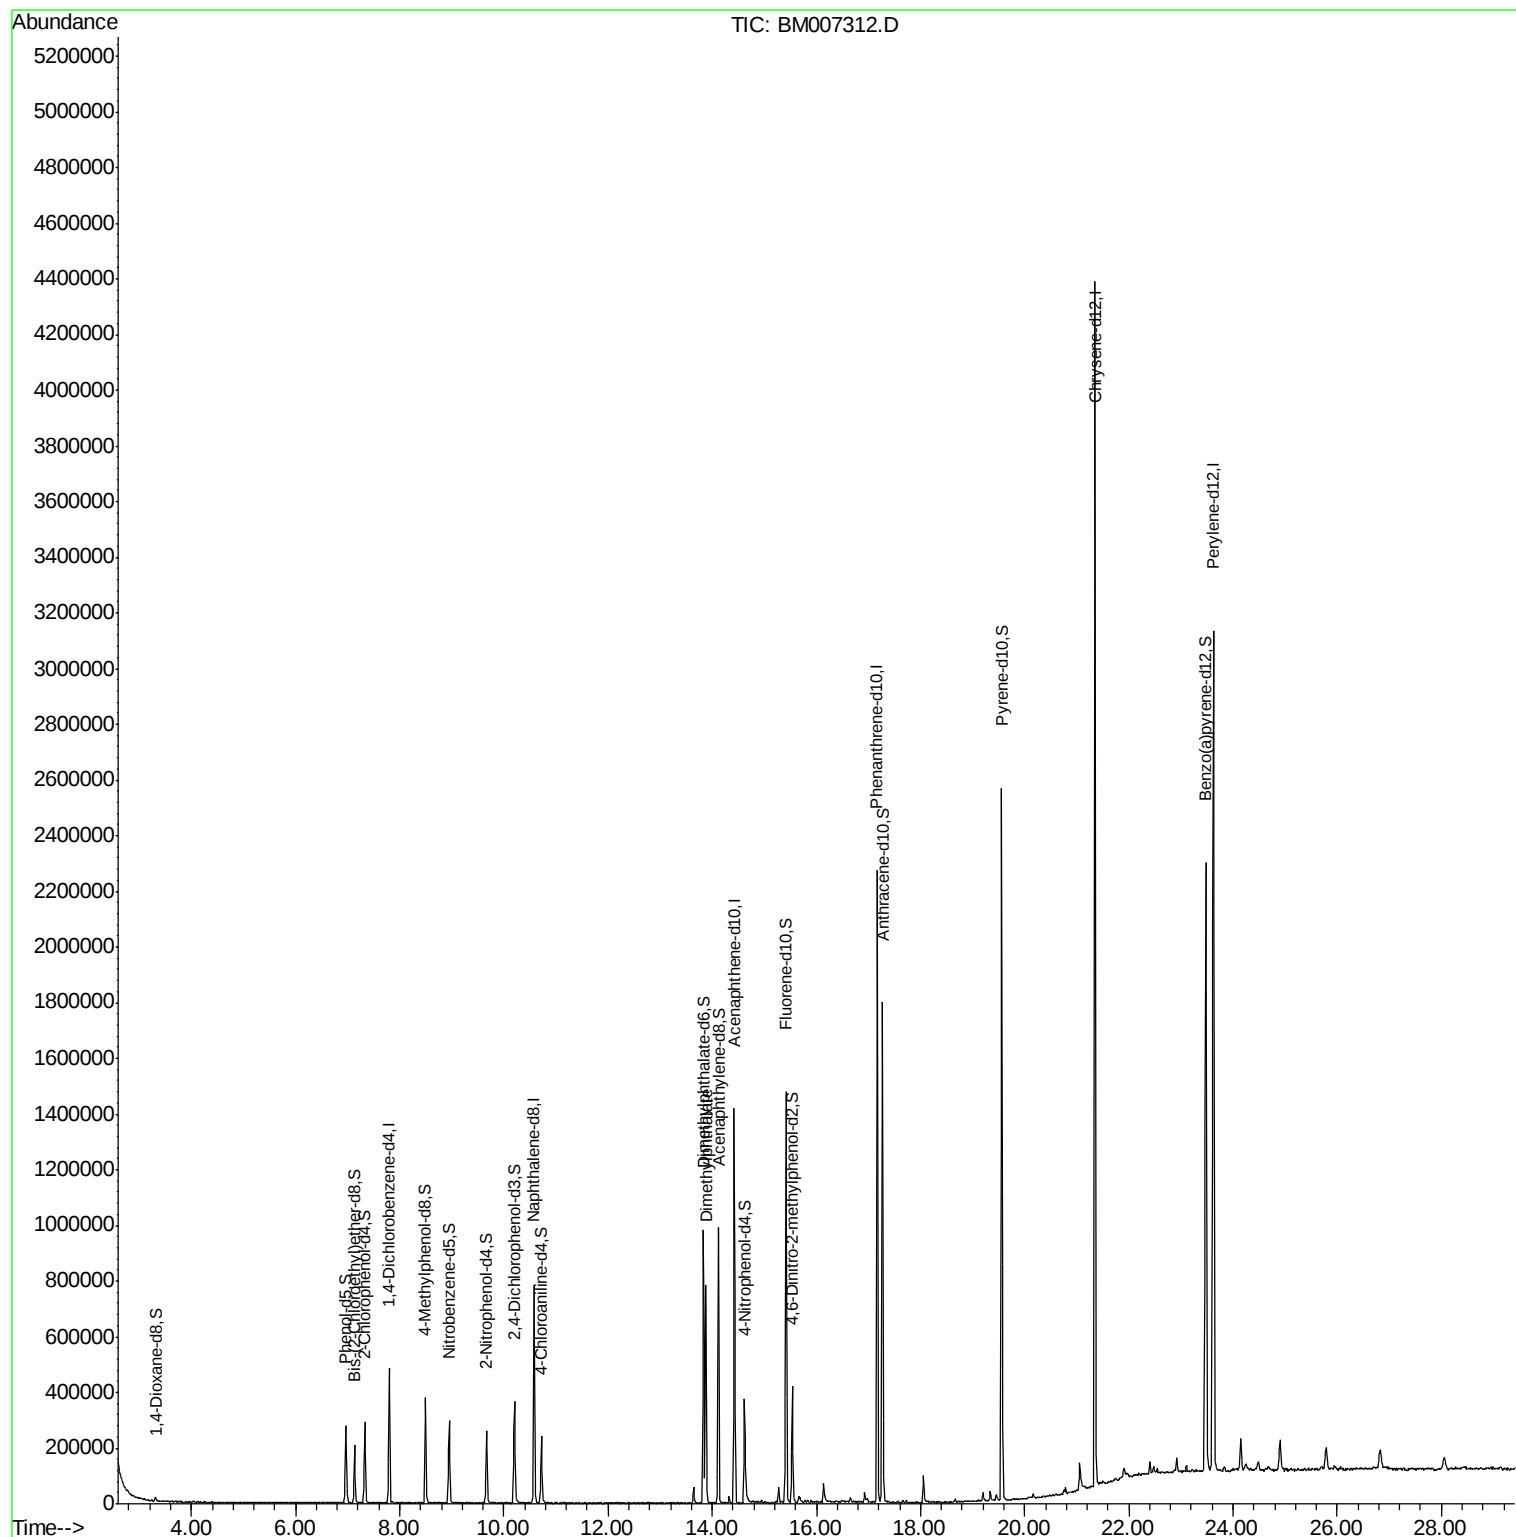

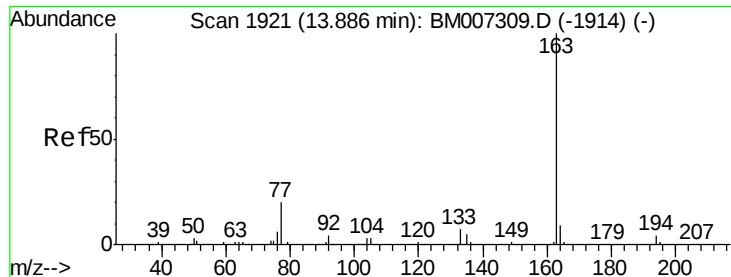

#44
 Dimethylphthalate
 Concen: 12.13 ng/ul
 RT: 13.88 min Scan# 1920
 Delta R.T. -0.01 min
 Lab File: BM007312.D
 Acq: 29 Aug 2016 17:09

Instrument :
 BNA_M
 ClientSampleId :
 DA277

Tgt Ion:163 Resp: 478179
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.2
 164 10.2 7.8 11.8

