

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007334.D
 Acq On : 30 Aug 2016 06:57
 Operator : UM/SJ
 Sample : H4575-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA275

Quant Time: Aug 30 08:46:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 30 04:03:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	206794	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	1029104	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	741786	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1957842	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2642927	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2621638	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	8969	2.22	ng/uL	0.00
5) Phenol-d5	6.96	99	246206	12.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	126107	12.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	186925	12.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	171330	10.06	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	92750	12.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	107399	12.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	242234	13.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	210772	9.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	834362	13.04	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1007414	13.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	144508	11.96	ng/ul	0.00
57) Fluorene-d10	15.42	176	793465	14.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	113654	9.23	ng/ul	0.00
70) Anthracene-d10	17.27	188	1312398	14.35	ng/ul	0.00
76) Pyrene-d10	19.56	212	1717505	15.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	1761611	14.59	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	536979	8.42	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007334.D
Acq On : 30 Aug 2016 06:57
Operator : UM/SJ
Sample : H4575-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA275

Quant Time: Aug 30 08:46:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 30 04:03:42 2016
Response via : Initial Calibration

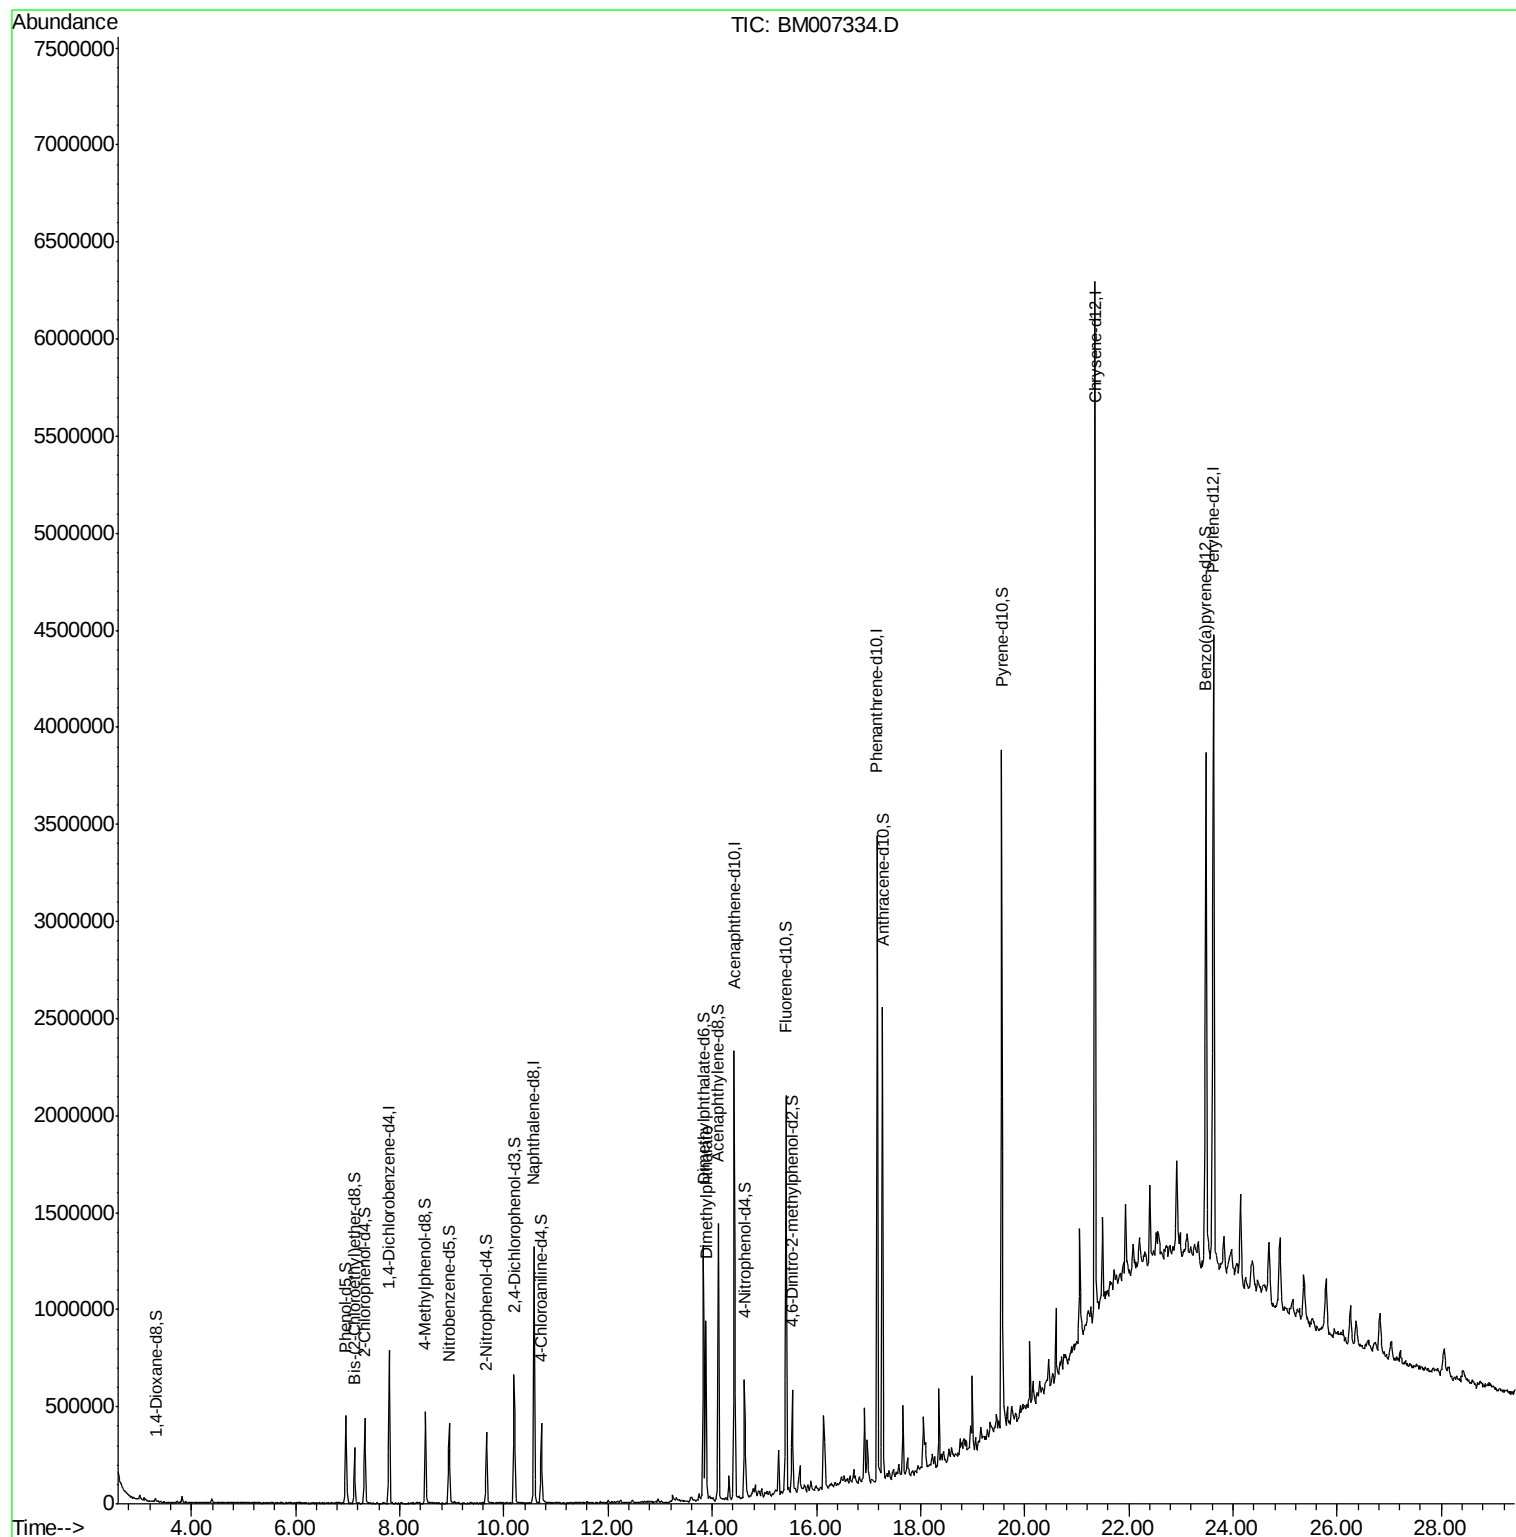

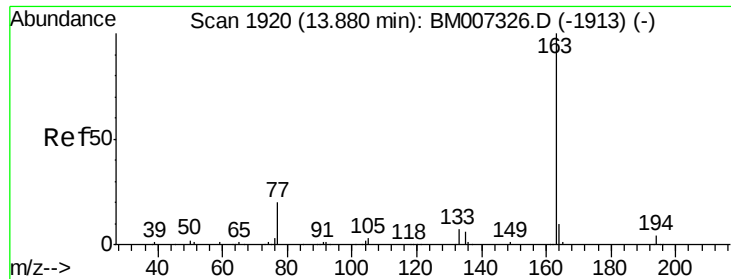

#44

Dimethylphthalate

Concen: 8.42 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. -0.00 min

Lab File: BM007334.D


Acq: 30 Aug 2016 06:57

Instrument :

BNA_M

ClientSampleId :

DA275

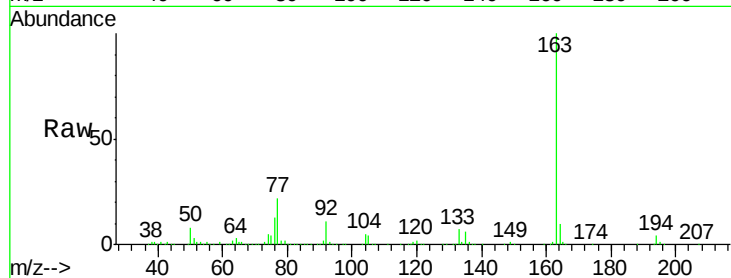


Tgt Ion:163 Resp: 536979

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.9 7.8 11.8

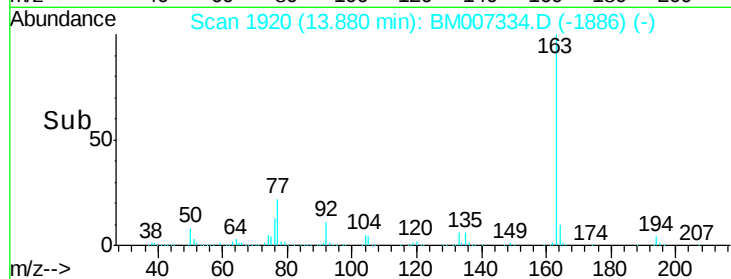

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

