

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007335.D
 Acq On : 30 Aug 2016 08:09
 Operator : UM/SJ
 Sample : H4575-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA286

Quant Time: Aug 30 08:43:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 30 04:03:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	178843	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	903992	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	686289	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1853593	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	2507375	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2556061	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	8344	2.38	ng/uL	0.00
5) Phenol-d5	6.96	99	204401	12.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	116993	13.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	160380	12.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	146468	9.94	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	85945	12.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	96533	12.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	192140	12.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	199402	10.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	751609	12.69	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	894305	13.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	114089	10.21	ng/ul	0.00
57) Fluorene-d10	15.42	176	706419	13.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	99370	8.53	ng/ul	0.00
70) Anthracene-d10	17.27	188	1192166	13.77	ng/ul	0.00
76) Pyrene-d10	19.56	212	1598046	15.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	1667295	14.16	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.88	163	535230	9.08	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007335.D
Acq On : 30 Aug 2016 08:09
Operator : UM/SJ
Sample : H4575-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA286

Quant Time: Aug 30 08:43:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 30 04:03:42 2016
Response via : Initial Calibration

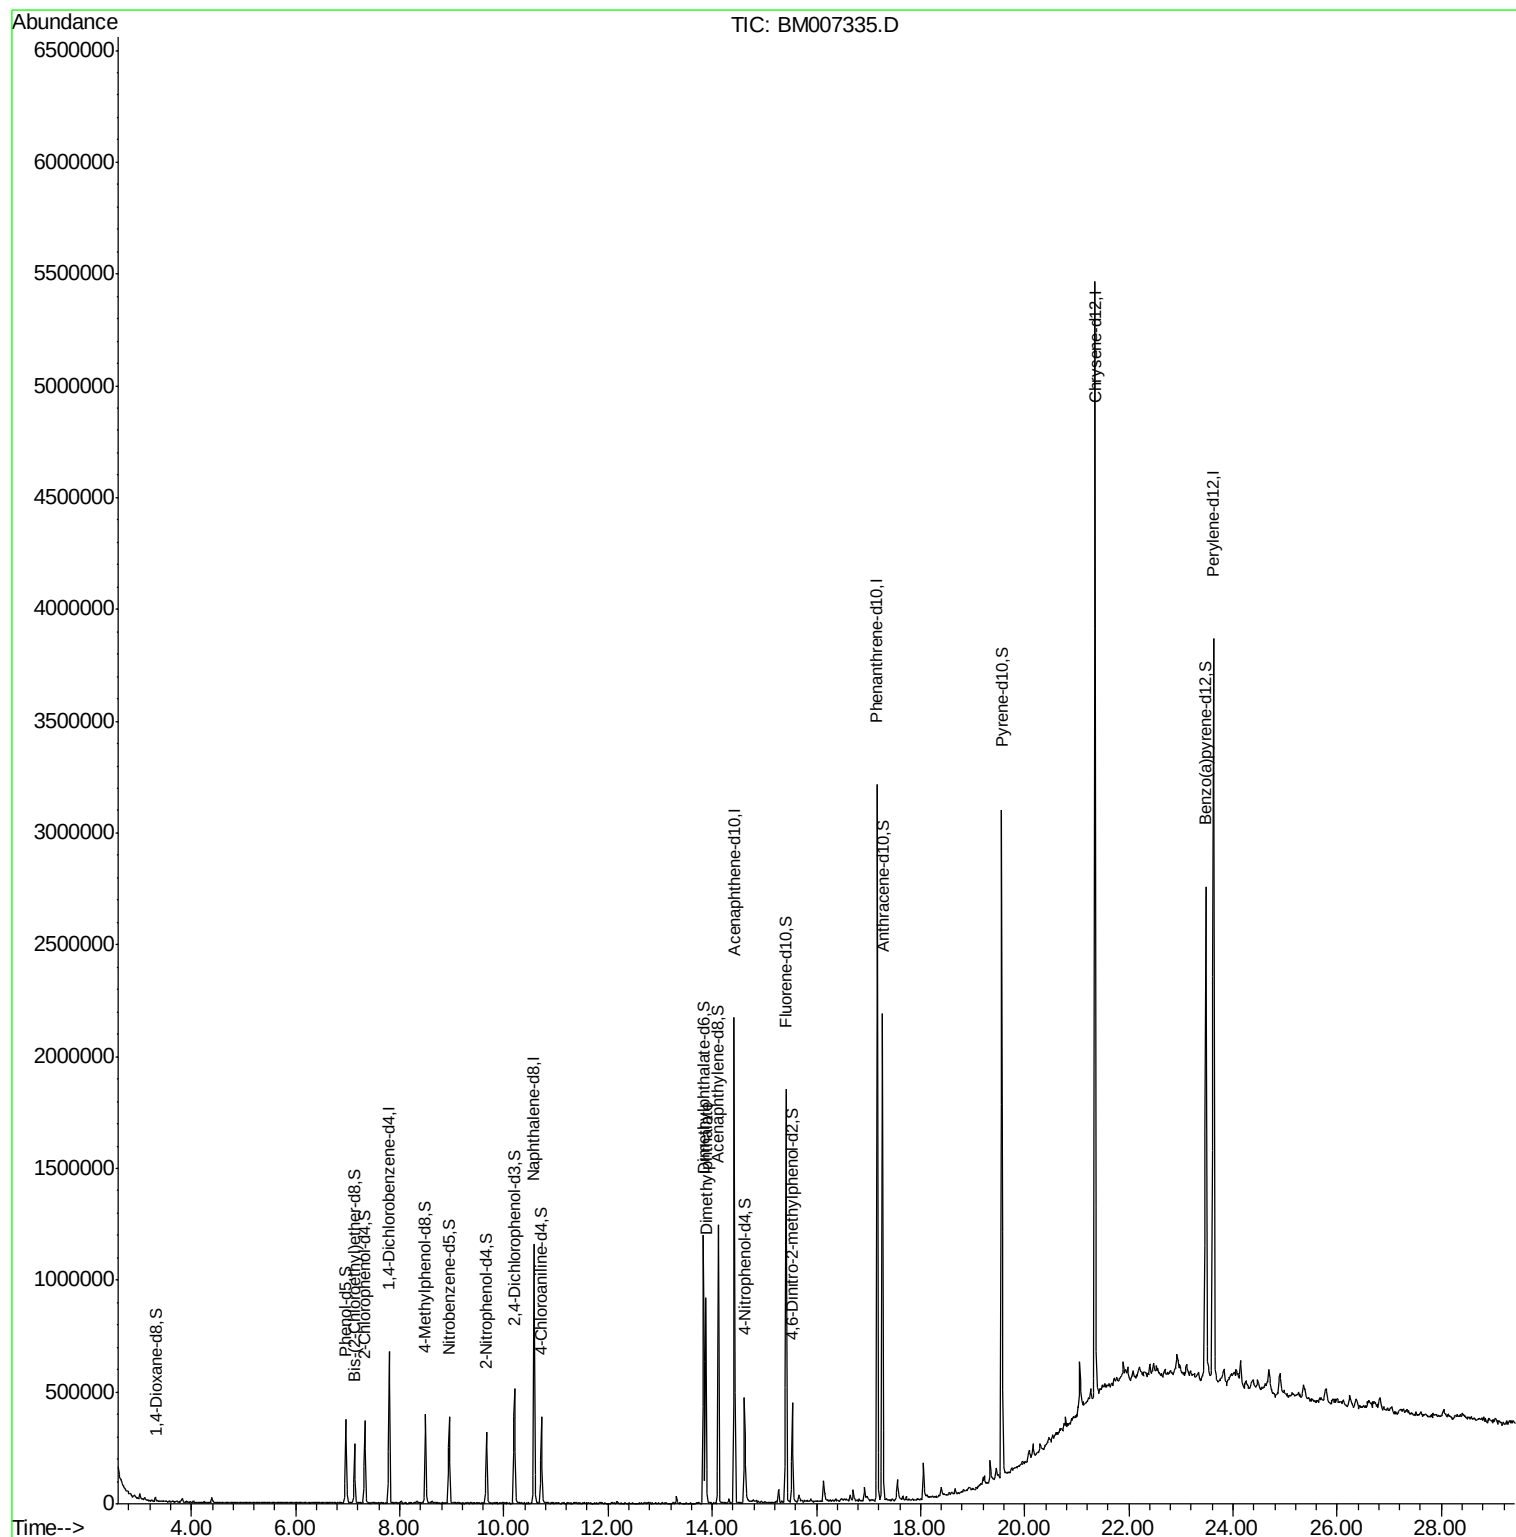

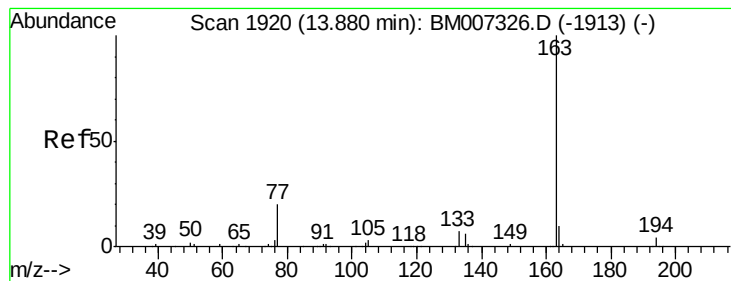

#44
 Dimethylphthalate
 Concen: 9.08 ng/ul
 RT: 13.88 min Scan# 1920
 Delta R.T. -0.00 min
 Lab File: BM007335.D
 Acq: 30 Aug 2016 08:09

Instrument :
 BNA_M
 ClientSampleId :
 DA286

Tgt Ion:	163	Resp:	535230
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.2
164	10.2	7.8	11.8

