

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007307.D
 Acq On : 29 Aug 2016 11:55
 Operator : UM/SJ
 Sample : PB93087BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	737	744	755	rBV	476850	764020	11.13%	1.411%
2	7.134	765	773	783	rBV	364779	581910	8.48%	1.074%
3	7.328	800	806	815	rBV	486812	796421	11.60%	1.471%
4	7.798	879	886	899	rBV	513785	831434	12.12%	1.535%
5	8.492	998	1004	1016	rBV	626889	1042749	15.19%	1.925%
6	8.951	1075	1082	1093	rBV	489077	827150	12.05%	1.527%
7	9.669	1197	1204	1214	rBV	429349	719537	10.48%	1.329%
8	10.204	1288	1295	1308	rBV	615833	1095603	15.96%	2.023%
9	10.581	1352	1359	1367	rBV	794864	1352360	19.71%	2.497%
10	10.716	1375	1382	1398	rBV	681180	1219390	17.77%	2.251%
11	13.839	1906	1913	1925	rBV	1685649	2439752	35.55%	4.505%
12	14.122	1954	1961	1972	rBV	1602104	2457633	35.81%	4.538%
13	14.427	2006	2013	2022	rBV2	1482560	2314757	33.73%	4.274%
14	14.621	2040	2046	2064	rBV	744074	1202819	17.53%	2.221%
15	15.421	2175	2182	2188	rBV	2379271	3449287	50.26%	6.369%
16	15.539	2197	2202	2214	rBV	760345	1107034	16.13%	2.044%
17	17.168	2472	2479	2490	rBV2	2360943	3435705	50.06%	6.344%
18	17.268	2490	2496	2513	rVB2	2881185	4218810	61.47%	7.790%
19	19.562	2879	2886	2901	rVV	4195011	5726371	83.44%	10.573%
20	21.350	3184	3190	3200	rBV	4301079	5527157	80.54%	10.205%
21	22.921	3454	3457	3464	rVB7	43538	72428	1.06%	0.134%
22	23.480	3544	3552	3566	rVB2	3561820	6862830	100.00%	12.672%
23	23.621	3568	3576	3587	rVB	2922427	5695601	82.99%	10.516%
24	24.150	3661	3666	3672	rVB	72198	135887	1.98%	0.251%
25	24.903	3790	3794	3803	rVB4	77163	164627	2.40%	0.304%
26	25.791	3941	3945	3955	rVB5	52999	118106	1.72%	0.218%


Sum of corrected areas: 54159378

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007307.D
Acq On : 29 Aug 2016 11:55
Operator : UM/SJ
Sample : PB93087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

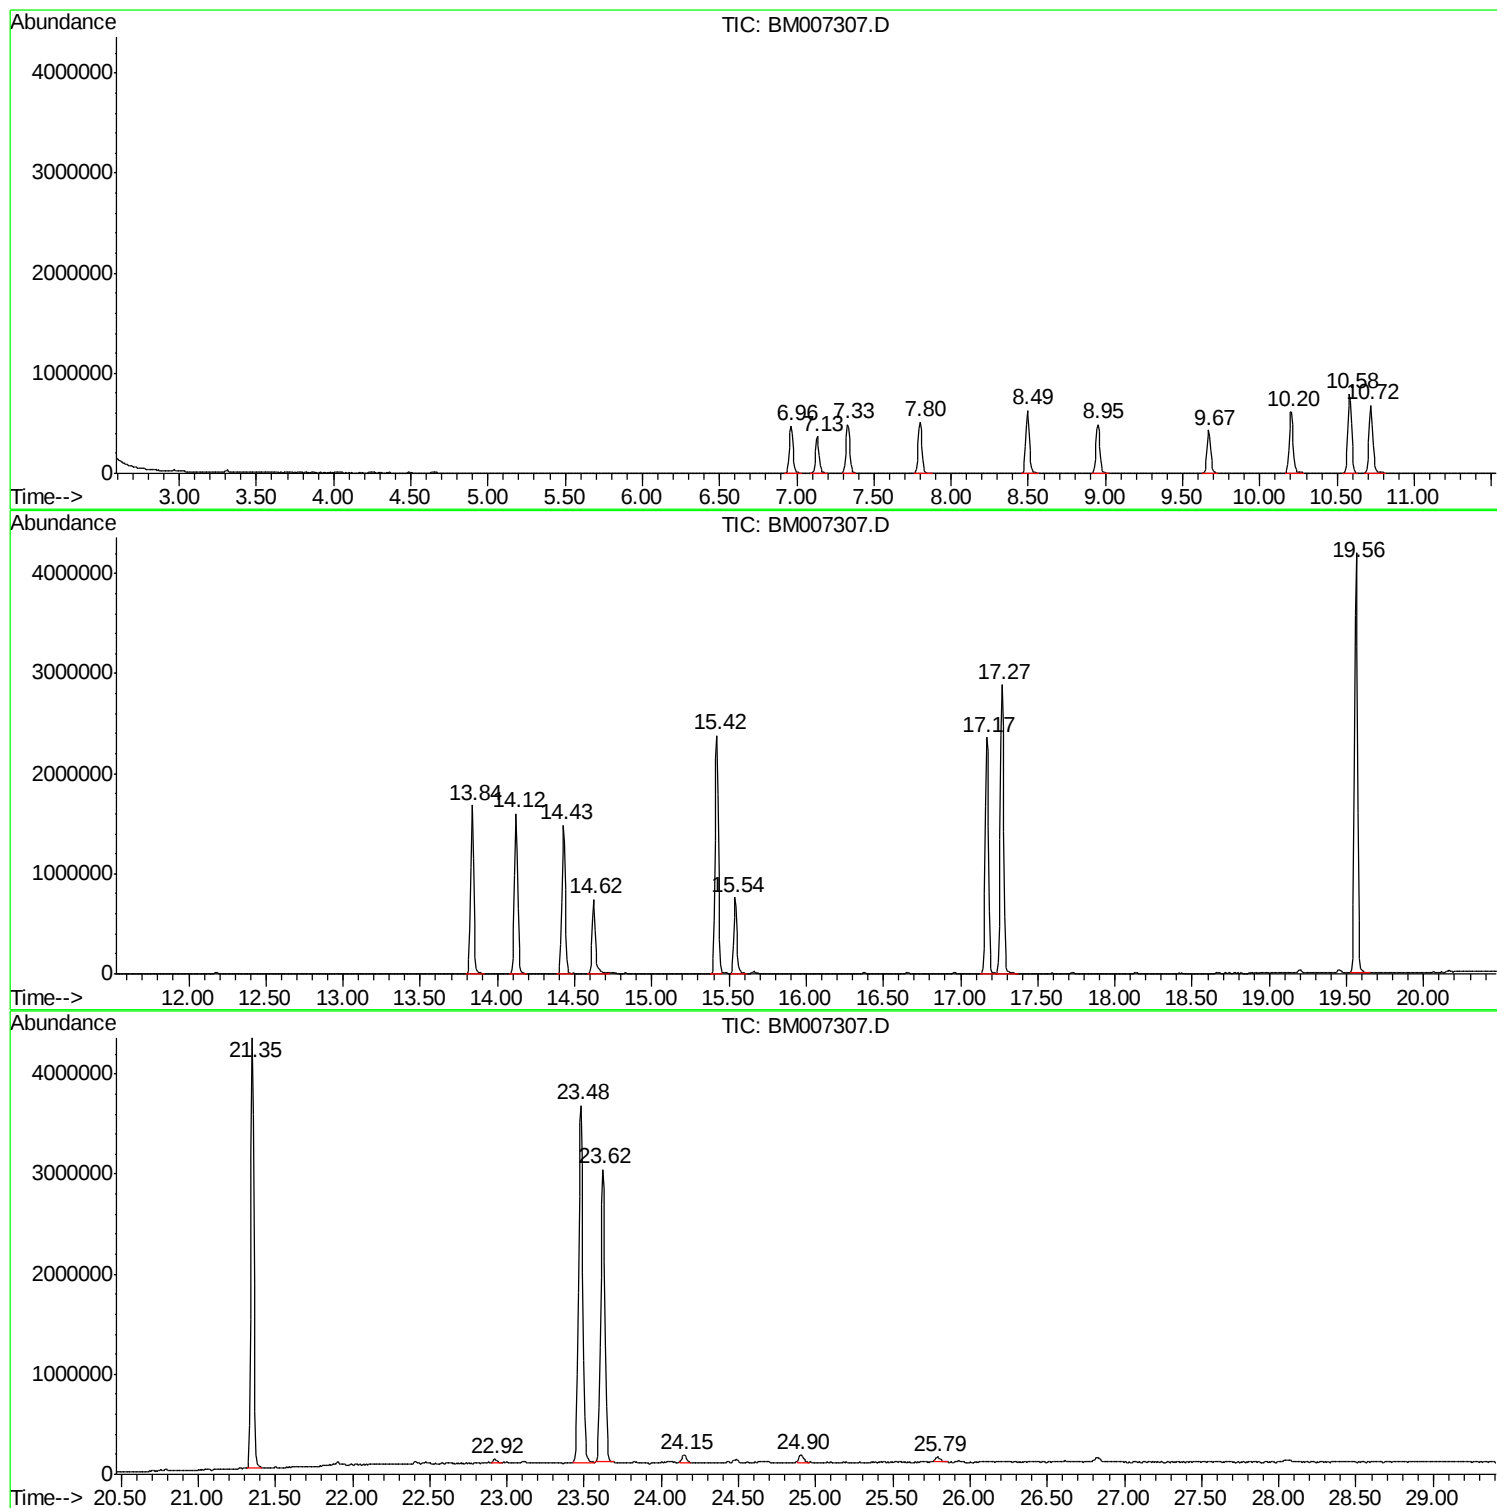

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007307.D
Acq On : 29 Aug 2016 11:55
Operator : UM/SJ
Sample : PB93087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007307.D
Acq On : 29 Aug 2016 11:55
Operator : UM/SJ
Sample : PB93087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc