

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007312.D
 Acq On : 29 Aug 2016 17:09
 Operator : UM/SJ
 Sample : H4575-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA277

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	736	744	753	rBV	278286	496915	8.49%	1.182%
2	7.134	766	773	785	rVB	210190	350788	5.99%	0.835%
3	7.328	800	806	816	rBV	293900	481490	8.23%	1.145%
4	7.798	879	886	893	rBV	485629	801055	13.69%	1.906%
5	8.492	997	1004	1016	rBV	379828	638312	10.91%	1.519%
6	8.951	1074	1082	1092	rBV	296703	508421	8.69%	1.210%
7	9.669	1197	1204	1215	rBV	259052	431677	7.38%	1.027%
8	10.204	1285	1295	1305	rBV	365915	664881	11.36%	1.582%
9	10.581	1352	1359	1367	rBV	784735	1309113	22.37%	3.114%
10	10.716	1375	1382	1395	rBV	242035	463745	7.92%	1.103%
11	13.645	1873	1880	1887	rBV	55634	77253	1.32%	0.184%
12	13.833	1906	1912	1916	rBV	982592	1412946	24.14%	3.361%
13	13.880	1916	1920	1930	rVB	784710	1098920	18.78%	2.614%
14	14.121	1953	1961	1973	rBV	990249	1510765	25.81%	3.594%
15	14.427	2005	2013	2024	rBV2	1417427	2197312	37.54%	5.227%
16	14.621	2038	2046	2063	rBV	376177	676004	11.55%	1.608%
17	15.280	2153	2158	2163	rVB	53785	67362	1.15%	0.160%
18	15.421	2175	2182	2196	rVV	1473687	2118776	36.20%	5.040%
19	15.539	2196	2202	2214	rVB	417422	595309	10.17%	1.416%
20	16.139	2300	2304	2308	rBV2	64927	93826	1.60%	0.223%
21	17.168	2473	2479	2489	rBV2	2269172	3261028	55.72%	7.758%
22	17.268	2489	2496	2508	rVB	1795482	2547958	43.53%	6.061%
23	18.056	2624	2630	2639	rBV3	97996	139119	2.38%	0.331%
24	19.562	2880	2886	2892	rBV	2558223	3443783	58.84%	8.193%
25	21.062	3136	3141	3149	rBV3	96748	191607	3.27%	0.456%
26	21.350	3184	3190	3203	rBV	4329320	5515870	94.24%	13.122%
27	22.921	3454	3457	3461	rVB3	48817	66233	1.13%	0.158%
28	23.474	3544	3551	3561	rBV2	2176839	4409785	75.34%	10.491%
29	23.621	3568	3576	3590	rVB	3014259	5853008	100.00%	13.924%
30	24.150	3661	3666	3674	rVB	112049	203968	3.48%	0.485%
31	24.909	3789	3795	3802	rVB2	104293	216441	3.70%	0.515%
32	25.785	3940	3944	3953	rVB3	79422	191892	3.28%	0.456%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007312.D
Acq On : 29 Aug 2016 17:09
Operator : UM/SJ
Sample : H4575-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA277

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Title : SVOA CALIBRATION


Sum of corrected areas: 42035562

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007312.D
Acq On : 29 Aug 2016 17:09
Operator : UM/SJ
Sample : H4575-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA277

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

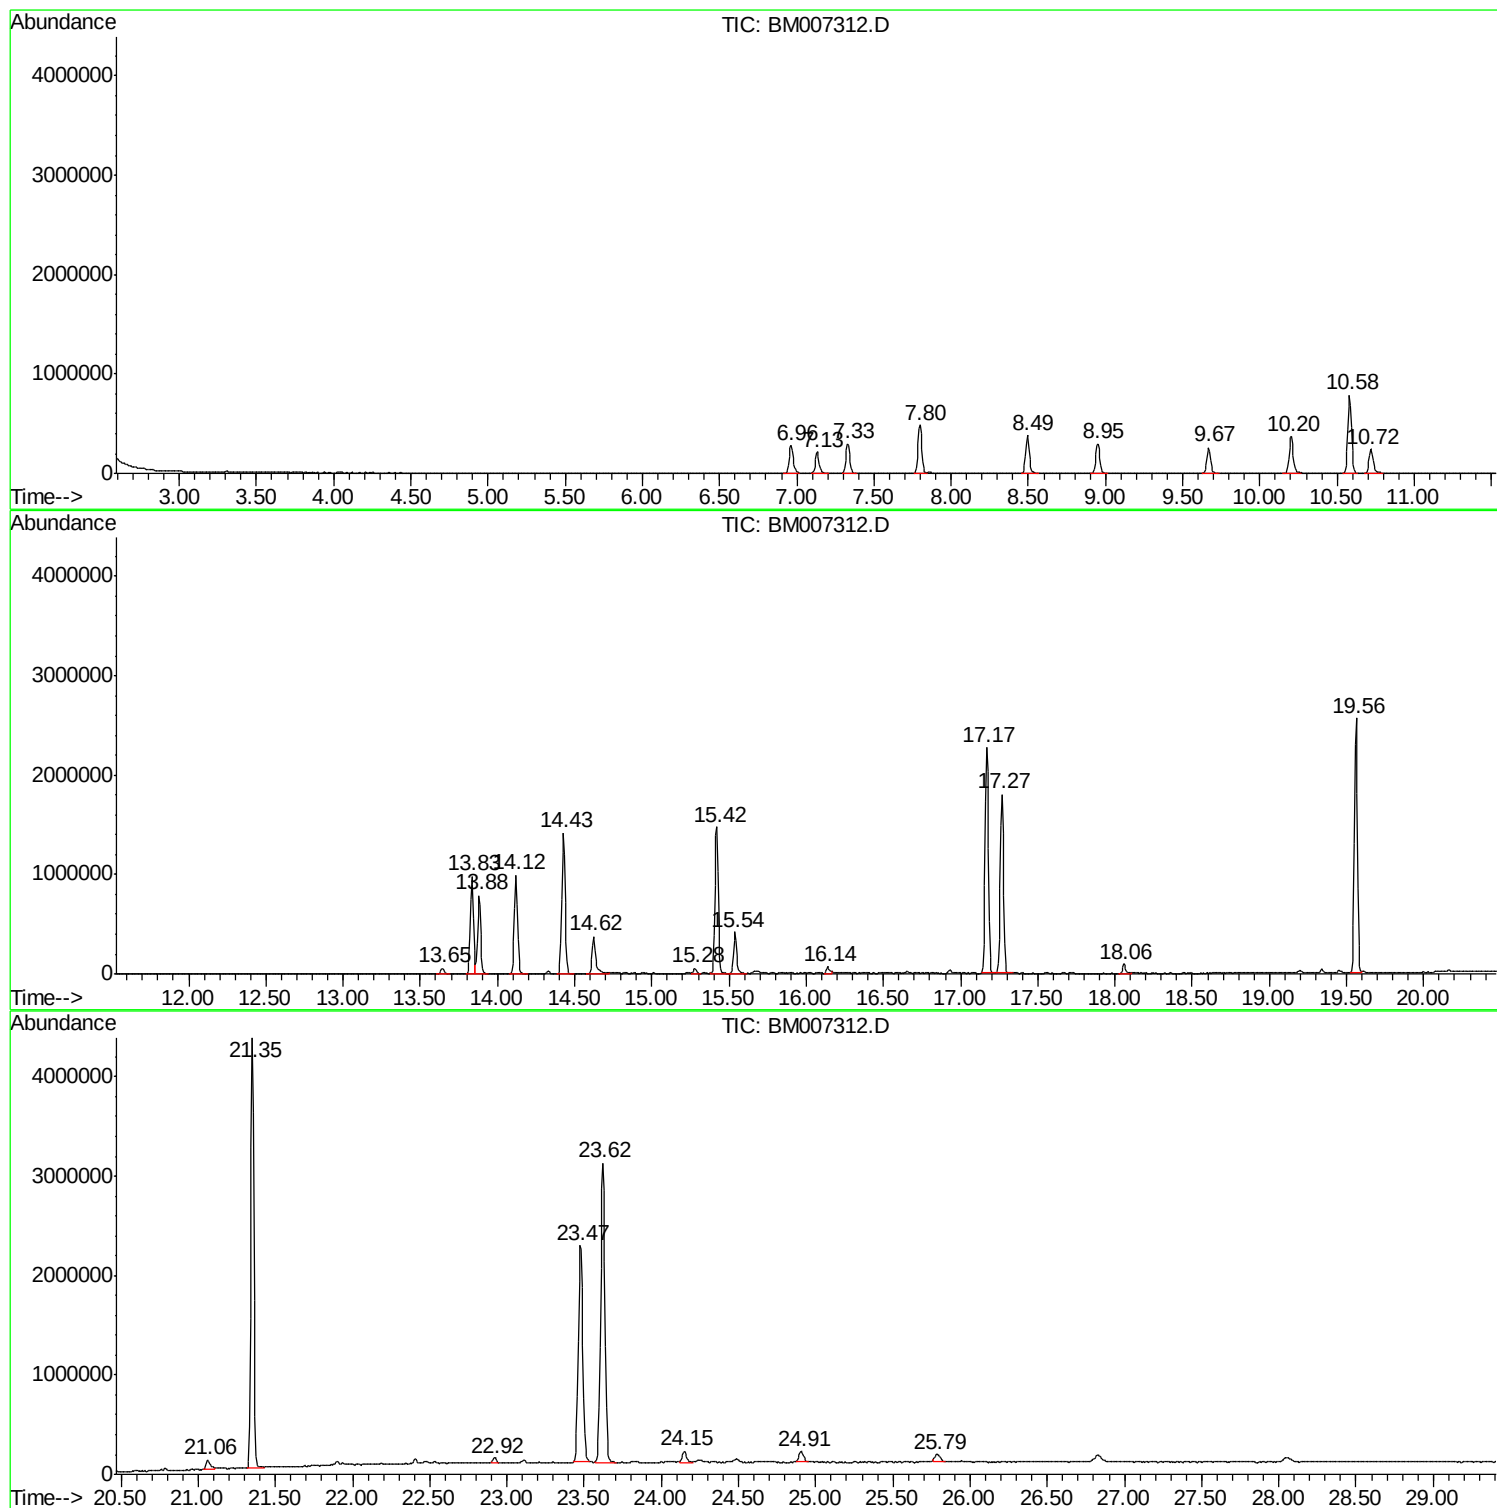

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007312.D
Acq On : 29 Aug 2016 17:09
Operator : UM/SJ
Sample : H4575-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA277

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007312.D
Acq On : 29 Aug 2016 17:09
Operator : UM/SJ
Sample : H4575-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA277

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc