

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007325.D
 Acq On : 30 Aug 2016 00:58
 Operator : UM/SJ
 Sample : H4587-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA289

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	738	744	753	rVB	120044	190432	2.32%	0.295%
2	7.134	766	773	782	rBV	382802	628144	7.66%	0.973%
3	7.328	799	806	815	rBV	444886	725299	8.84%	1.123%
4	7.798	878	886	893	rBV	676657	1099381	13.40%	1.703%
5	8.492	995	1004	1016	rBV	401104	671112	8.18%	1.040%
6	8.951	1075	1082	1092	rBV	577334	978553	11.93%	1.516%
7	9.669	1197	1204	1215	rBV	524119	881642	10.74%	1.366%
8	10.198	1287	1294	1306	rBV	741693	1342914	16.37%	2.080%
9	10.581	1349	1359	1367	rBV	1077363	1829331	22.29%	2.834%
10	11.369	1487	1493	1505	rBV2	53335	102921	1.25%	0.159%
11	12.698	1712	1719	1728	rBV2	56297	96227	1.17%	0.149%
12	13.027	1770	1775	1785	rBV	71921	113694	1.39%	0.176%
13	13.833	1905	1912	1922	rBV	2008577	2858266	34.83%	4.427%
14	14.121	1951	1961	1974	rVB	2065224	3089400	37.65%	4.785%
15	14.427	2006	2013	2022	rVB2	2024354	3110177	37.90%	4.817%
16	14.627	2041	2047	2056	rBV	165129	293937	3.58%	0.455%
17	15.221	2143	2148	2159	rVB2	46520	86740	1.06%	0.134%
18	15.421	2175	2182	2191	rBV	2914612	4258368	51.90%	6.596%
19	15.539	2195	2202	2212	rBV	1096095	1519988	18.52%	2.354%
20	17.168	2473	2479	2489	rBV2	3155255	4570110	55.70%	7.079%
21	17.268	2489	2496	2506	rVV2	3624077	5164672	62.94%	8.000%
22	19.562	2879	2886	2900	rBV	4871889	6959547	84.82%	10.780%
23	21.350	3184	3190	3199	rBV	5731755	7332184	89.36%	11.357%
24	22.921	3453	3457	3465	rVB2	74726	113816	1.39%	0.176%
25	23.480	3543	3552	3567	rVV2	4147462	8205560	100.00%	12.710%
26	23.621	3568	3576	3590	rVB	3727085	7455434	90.86%	11.548%
27	24.144	3660	3665	3670	rVB2	127469	238171	2.90%	0.369%
28	24.480	3718	3722	3730	rVB2	60533	122424	1.49%	0.190%
29	24.903	3788	3794	3800	rVB3	130803	287818	3.51%	0.446%
30	25.780	3939	3943	3955	rVB4	99140	233741	2.85%	0.362%


Sum of corrected areas: 64560003

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007325.D
Acq On : 30 Aug 2016 00:58
Operator : UM/SJ
Sample : H4587-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA289

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

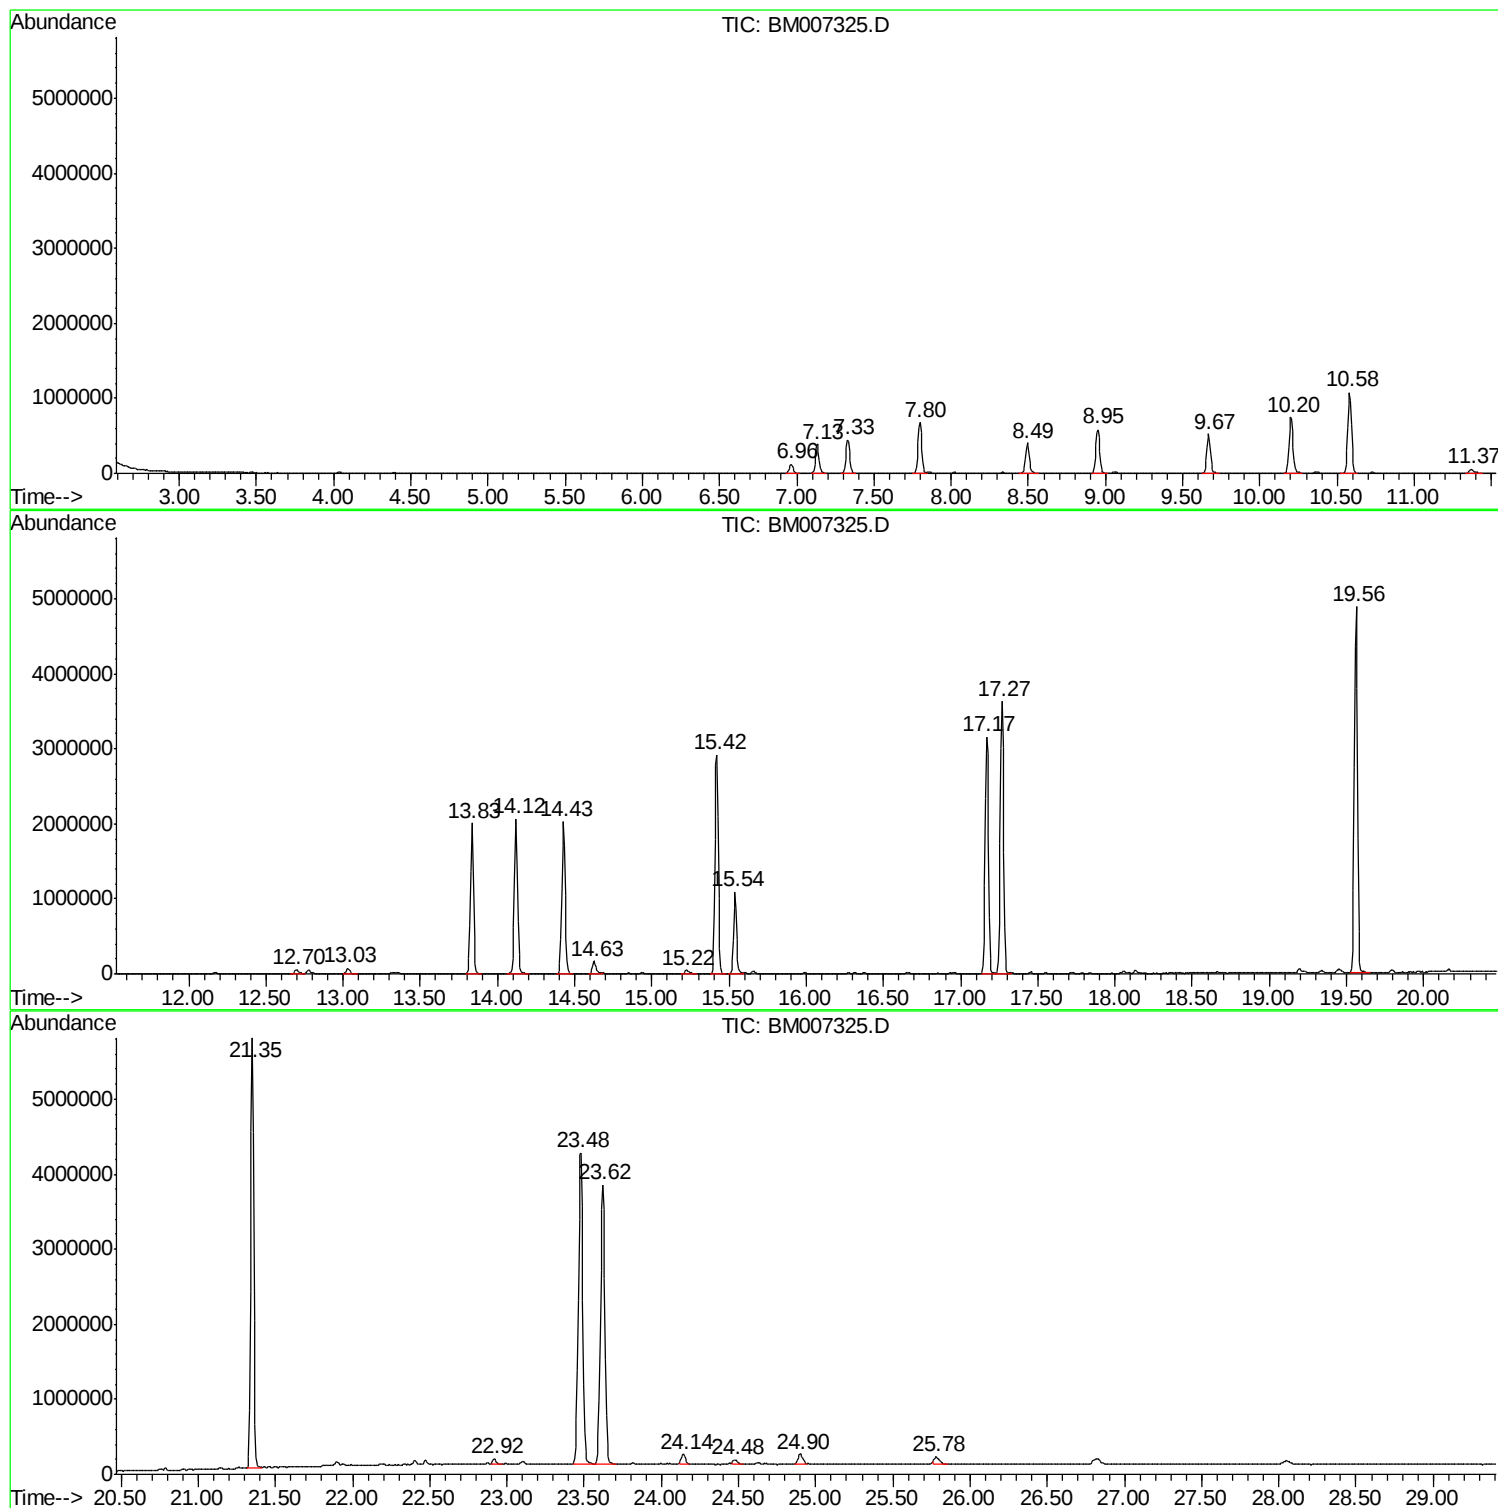

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007325.D
Acq On : 30 Aug 2016 00:58
Operator : UM/SJ
Sample : H4587-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA289

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007325.D
Acq On : 30 Aug 2016 00:58
Operator : UM/SJ
Sample : H4587-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA289

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc