

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007331.D
 Acq On : 30 Aug 2016 04:34
 Operator : UM/SJ
 Sample : PB93088BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	737	744	754	rBV	729046	1186861	11.79%	1.506%
2	7.134	766	773	785	rBV	536232	864103	8.58%	1.096%
3	7.328	800	806	817	rBV	730215	1207681	11.99%	1.532%
4	7.798	879	886	894	rBV	724072	1170526	11.62%	1.485%
5	8.492	997	1004	1016	rBV	1009934	1634420	16.23%	2.074%
6	8.951	1072	1082	1090	rBV	777372	1307806	12.99%	1.659%
7	9.669	1196	1204	1215	rBV	708956	1180555	11.72%	1.498%
8	10.198	1287	1294	1310	rBV	1030583	1766184	17.54%	2.241%
9	10.580	1351	1359	1367	rBV	1157401	1944495	19.31%	2.467%
10	10.716	1375	1382	1398	rBV	1060145	1849662	18.37%	2.347%
11	13.833	1904	1912	1924	rBV	2583162	3553281	35.29%	4.509%
12	14.121	1953	1961	1973	rBV	2470421	3745153	37.19%	4.752%
13	14.427	2006	2013	2022	rVB2	2156889	3219060	31.97%	4.085%
14	14.621	2040	2046	2064	rBV	1303794	1978976	19.65%	2.511%
15	15.421	2175	2182	2189	rBV	3388719	5067796	50.33%	6.430%
16	15.539	2196	2202	2216	rBV	1322470	1855089	18.42%	2.354%
17	17.168	2472	2479	2489	rBV2	3287124	4733091	47.01%	6.006%
18	17.268	2489	2496	2508	rVV2	4379807	6226797	61.84%	7.901%
19	19.562	2879	2886	2897	rBV	5974240	8193912	81.37%	10.397%
20	21.350	3184	3190	3200	rBV	5950731	7613725	75.61%	9.661%
21	23.480	3543	3552	3566	rVB2	5151055	10069324	100.00%	12.777%
22	23.621	3568	3576	3587	rVB2	4049937	7988212	79.33%	10.136%
23	24.138	3660	3664	3671	rVB	109658	199898	1.99%	0.254%
24	24.897	3787	3793	3803	rVB3	110566	253741	2.52%	0.322%


Sum of corrected areas: 78810348

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007331.D
Acq On : 30 Aug 2016 04:34
Operator : UM/SJ
Sample : PB93088BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

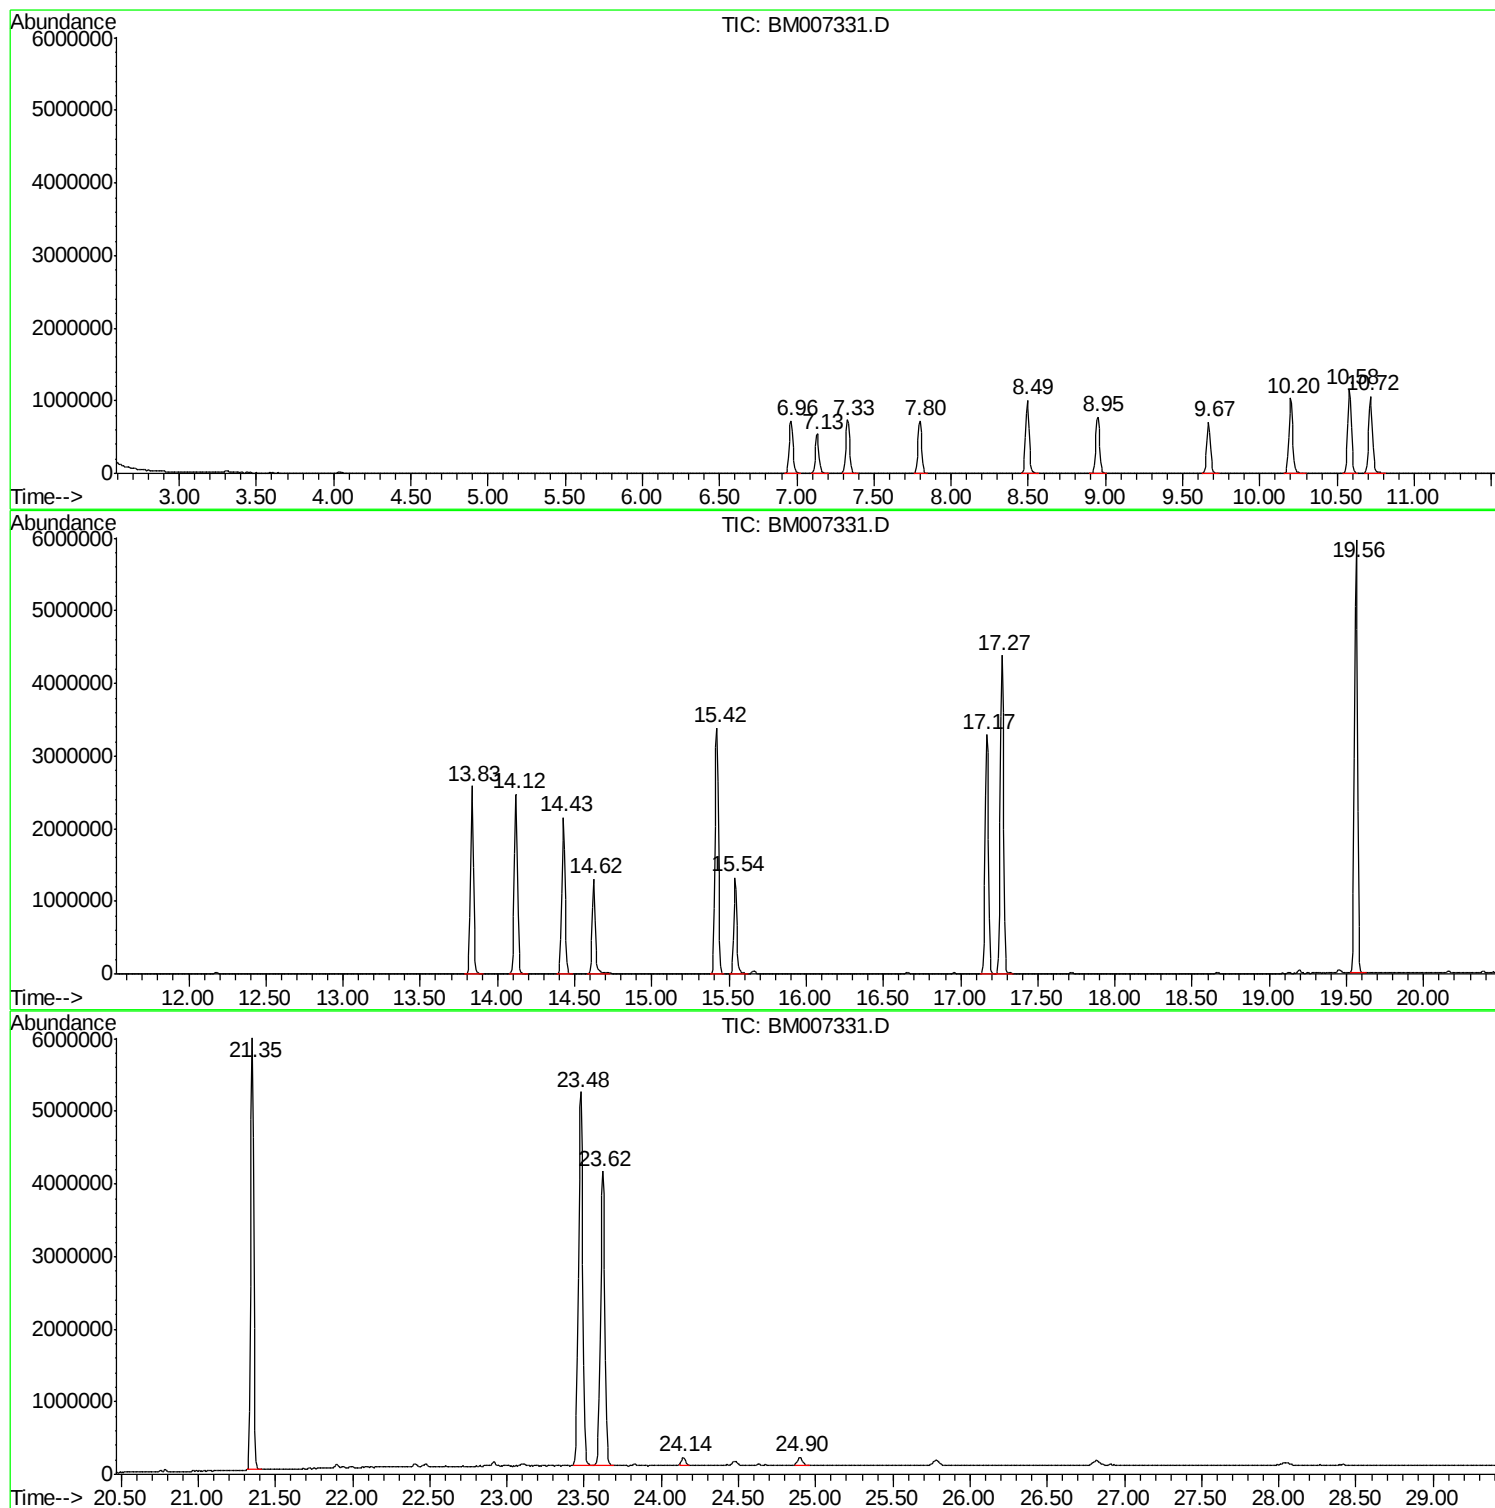

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007331.D
Acq On : 30 Aug 2016 04:34
Operator : UM/SJ
Sample : PB93088BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007331.D
Acq On : 30 Aug 2016 04:34
Operator : UM/SJ
Sample : PB93088BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK88

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc