

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007336.D
 Acq On : 30 Aug 2016 08:45
 Operator : UM/SJ
 Sample : H4575-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA273

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	738	744	754	rBV	356232	625232	11.04%	1.393%
2	7.128	766	772	781	rBV	229619	375076	6.63%	0.836%
3	7.328	800	806	814	rBV	340696	565799	9.99%	1.261%
4	7.798	878	886	893	rBV	668895	1075824	19.00%	2.398%
5	8.492	995	1004	1019	rBV	393959	665217	11.75%	1.483%
6	8.951	1074	1082	1090	rBV	343711	588501	10.40%	1.312%
7	9.669	1197	1204	1211	rBV	310465	522805	9.24%	1.165%
8	10.204	1288	1295	1304	rBV	509511	901426	15.92%	2.009%
9	10.580	1351	1359	1367	rBV	1087672	1814507	32.05%	4.044%
10	10.716	1376	1382	1394	rBV	304388	575175	10.16%	1.282%
11	13.833	1906	1912	1916	rBV	1084261	1530247	27.03%	3.410%
12	13.880	1916	1920	1928	rVB	812730	1131488	19.99%	2.522%
13	14.116	1954	1960	1969	rVB	1142191	1745871	30.84%	3.891%
14	14.427	2003	2013	2022	rBV2	1880098	2939247	51.92%	6.551%
15	14.621	2039	2046	2063	rBV	469515	825501	14.58%	1.840%
16	15.280	2153	2158	2162	rVB	61961	76721	1.36%	0.171%
17	15.421	2175	2182	2189	rBV	1665330	2464409	43.53%	5.492%
18	15.539	2197	2202	2214	rVB	400817	587681	10.38%	1.310%
19	16.139	2299	2304	2307	rBV	75371	107237	1.89%	0.239%
20	16.927	2433	2438	2441	rBV	46160	58297	1.03%	0.130%
21	17.168	2473	2479	2488	rBV2	2747932	4073588	71.96%	9.079%
22	17.268	2489	2496	2504	rVB	1969937	2826214	49.92%	6.299%
23	18.056	2625	2630	2641	rBV	169312	284285	5.02%	0.634%
24	19.339	2845	2848	2853	rBV4	59967	84839	1.50%	0.189%
25	19.562	2880	2886	2892	rBV	2688509	3739778	66.06%	8.335%
26	21.062	3138	3141	3147	rBV	187098	304176	5.37%	0.678%
27	21.350	3185	3190	3196	rVB	4414088	5660970	100.00%	12.617%
28	23.474	3545	3551	3559	rBV2	1779121	3612144	63.81%	8.050%
29	23.621	3569	3576	3586	rVB	2666395	5106451	90.20%	11.381%


Sum of corrected areas: 44868706

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007336.D
Acq On : 30 Aug 2016 08:45
Operator : UM/SJ
Sample : H4575-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA273

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

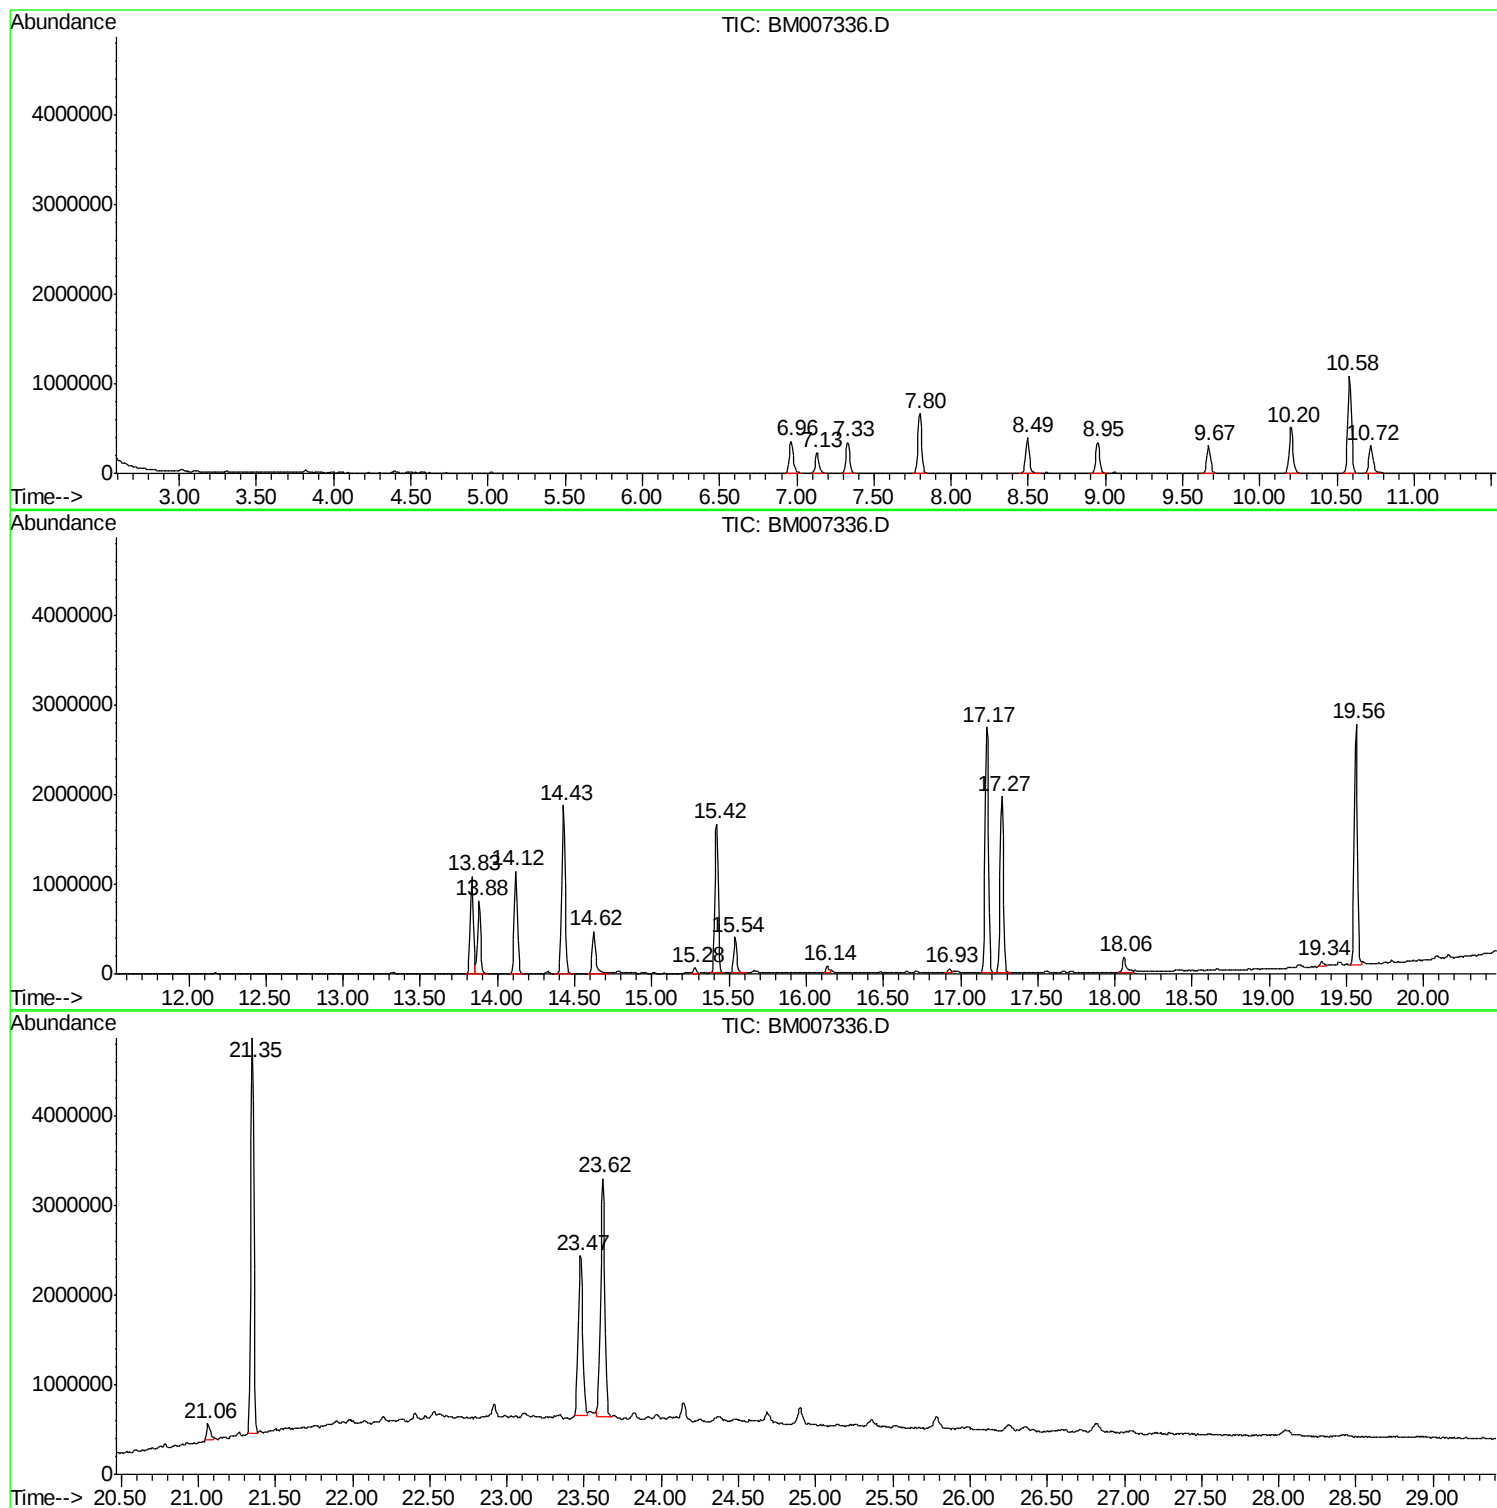

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007336.D
Acq On : 30 Aug 2016 08:45
Operator : UM/SJ
Sample : H4575-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA273

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007336.D
Acq On : 30 Aug 2016 08:45
Operator : UM/SJ
Sample : H4575-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA273

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc