

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
 Data File : BM007337.D
 Acq On : 30 Aug 2016 09:21
 Operator : UM/SJ
 Sample : H4575-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA276

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	734	744	756	rBV	369302	655619	10.65%	1.369%
2	7.134	765	773	781	rBV	256212	416225	6.76%	0.869%
3	7.328	800	806	818	rVB	371140	609082	9.90%	1.272%
4	7.798	878	886	894	rBV	689257	1141485	18.55%	2.384%
5	8.492	995	1004	1013	rBV	392379	668614	10.86%	1.397%
6	8.951	1074	1082	1089	rBV	369570	632144	10.27%	1.320%
7	9.669	1197	1204	1214	rBV	318864	545293	8.86%	1.139%
8	10.198	1287	1294	1306	rBV	522541	925582	15.04%	1.933%
9	10.581	1352	1359	1367	rBV	1135060	1896571	30.81%	3.962%
10	10.716	1375	1382	1396	rBV	386310	703836	11.44%	1.470%
11	13.833	1906	1912	1916	rBV	1119025	1586667	25.78%	3.314%
12	13.880	1916	1920	1929	rVB	739863	1039120	16.88%	2.171%
13	14.116	1950	1960	1968	rBV	1226956	1849965	30.06%	3.864%
14	14.427	2002	2013	2022	rBV2	2081365	3140198	51.02%	6.559%
15	14.621	2040	2046	2060	rBV	442986	788467	12.81%	1.647%
16	15.274	2153	2157	2162	rVB	71602	89724	1.46%	0.187%
17	15.421	2175	2182	2189	rBV	1697493	2529447	41.10%	5.284%
18	15.539	2197	2202	2213	rVB	360305	528059	8.58%	1.103%
19	15.663	2218	2223	2230	rBV6	34109	81947	1.33%	0.171%
20	16.139	2299	2304	2313	rBV	95135	166592	2.71%	0.348%
21	16.715	2396	2402	2410	rBV2	46524	76910	1.25%	0.161%
22	16.927	2433	2438	2441	rBV	61339	76425	1.24%	0.160%
23	17.168	2473	2479	2485	rBV	3055588	4355063	70.76%	9.097%
24	17.268	2490	2496	2505	rVB	1973389	2817320	45.77%	5.885%
25	18.057	2626	2630	2634	rBV2	104064	151073	2.45%	0.316%
26	18.398	2684	2688	2692	rBV3	44643	66712	1.08%	0.139%
27	19.227	2825	2829	2833	rVB	149792	198536	3.23%	0.415%
28	19.462	2863	2869	2873	rBV6	53410	96381	1.57%	0.201%
29	19.562	2880	2886	2899	rBV	2798779	4124534	67.01%	8.615%
30	20.086	2972	2975	2980	rBV3	71620	96416	1.57%	0.201%
31	21.062	3138	3141	3148	rBV5	123555	213520	3.47%	0.446%
32	21.350	3185	3190	3202	rVB	4704256	6155047	100.00%	12.857%
33	23.480	3545	3552	3566	rVB2	1866306	3884176	63.11%	8.113%
34	23.627	3569	3577	3592	rVB	2813419	5567689	90.46%	11.630%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007337.D
Acq On : 30 Aug 2016 09:21
Operator : UM/SJ
Sample : H4575-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA276

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Title : SVOA CALIBRATION


Sum of corrected areas: 47874439

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007337.D
Acq On : 30 Aug 2016 09:21
Operator : UM/SJ
Sample : H4575-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA276

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

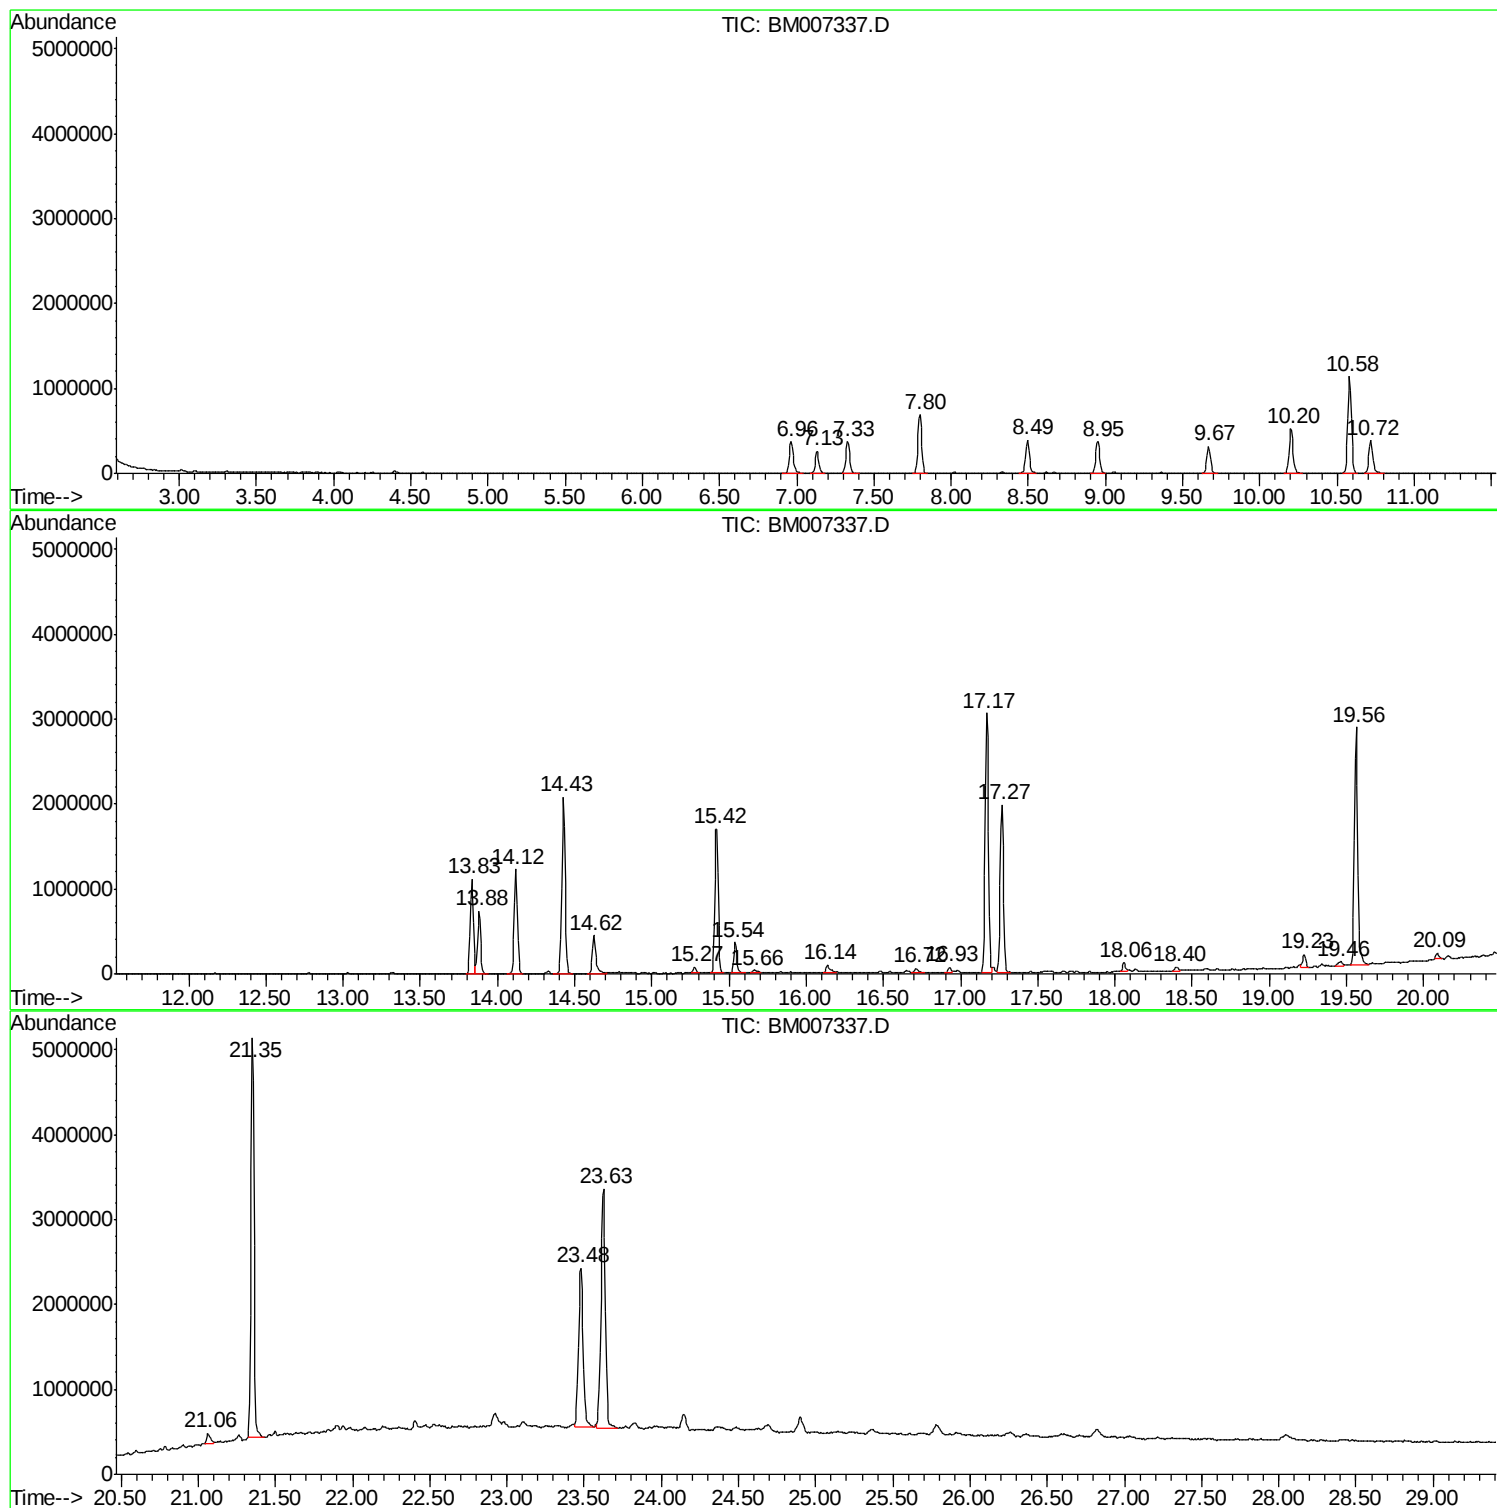

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007337.D
Acq On : 30 Aug 2016 09:21
Operator : UM/SJ
Sample : H4575-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA276

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM082916\
Data File : BM007337.D
Acq On : 30 Aug 2016 09:21
Operator : UM/SJ
Sample : H4575-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA276

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc