
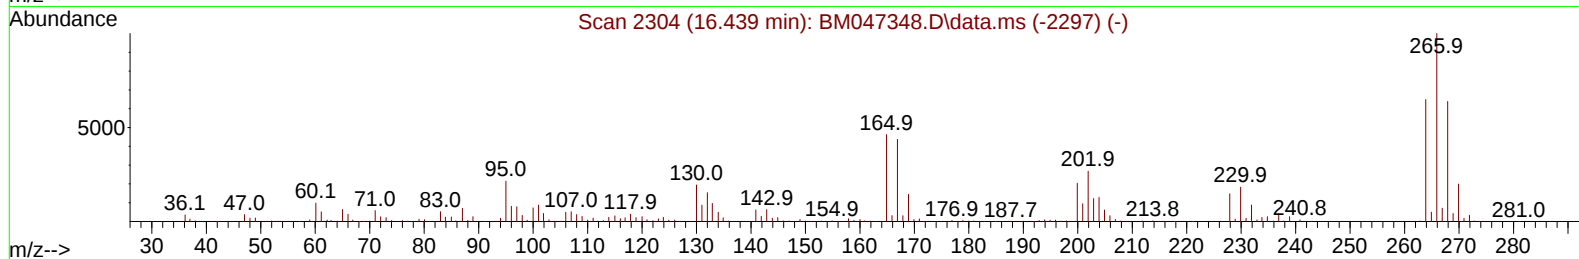
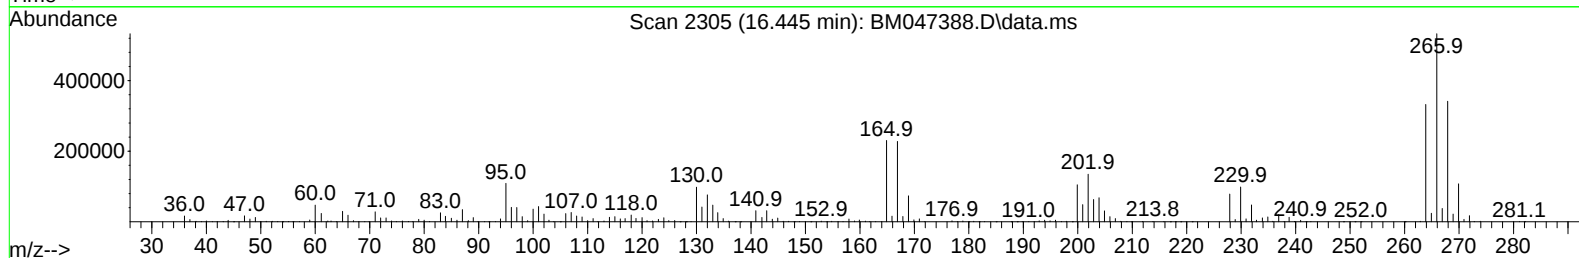


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082924\
Data File : BM047388.D
Acq On : 29 Aug 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 11:16:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

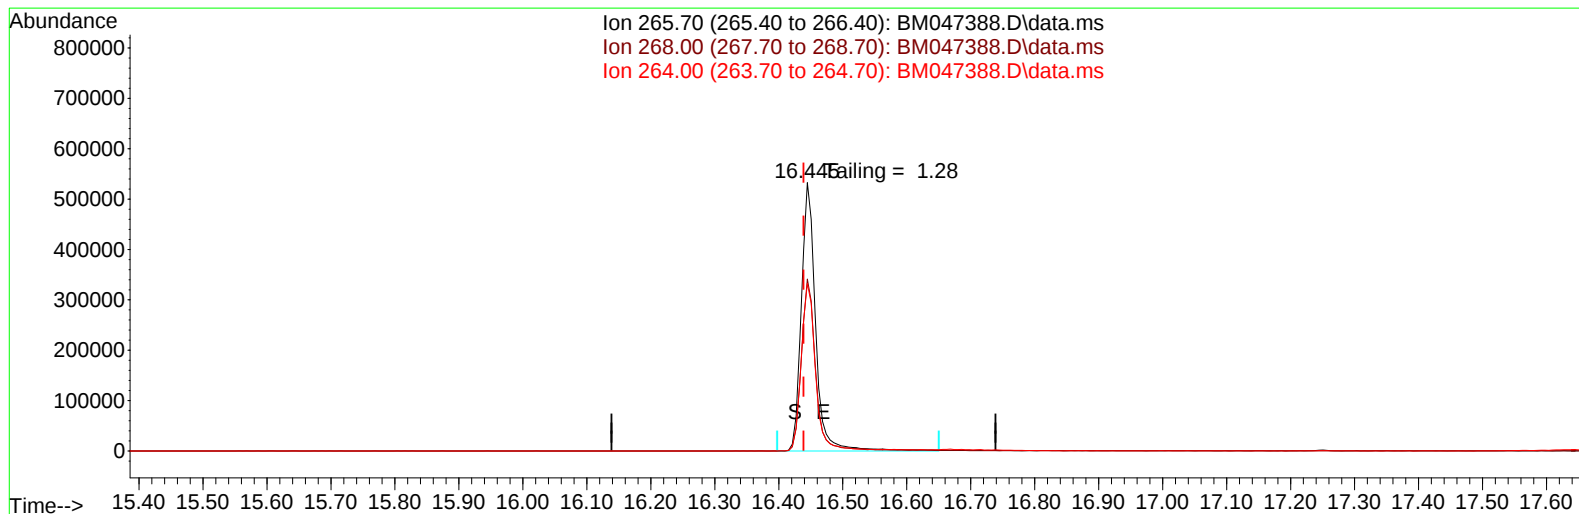

TIC: BM047388.D\data.ms

(70) Pentachlorophenol (C)




16.445min (+ 0.006) 106487.81 ng

response 829653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.08
264.00	64.90	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082924\
Data File : BM047388.D
Acq On : 29 Aug 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 11:16:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM082624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 26 18:11:40 2024
Response via : Initial Calibration

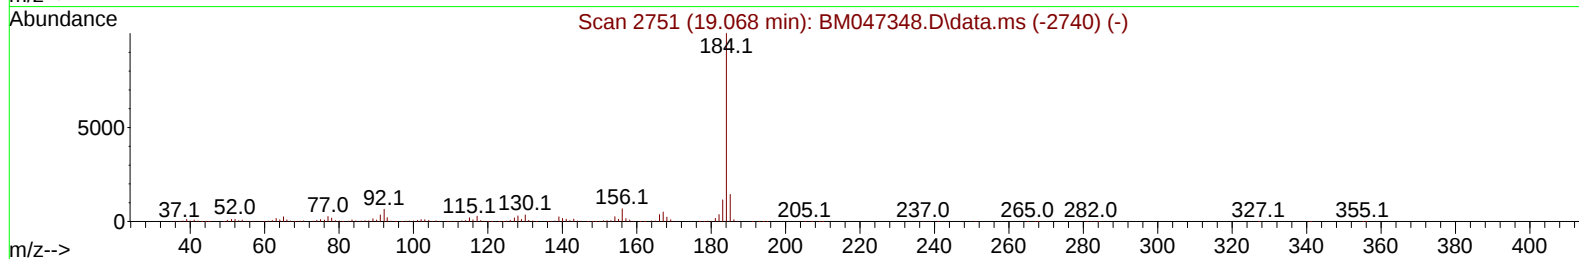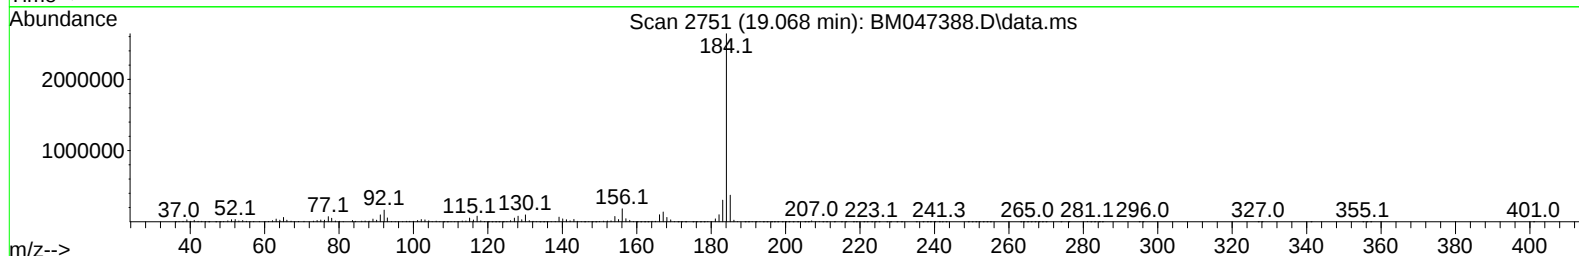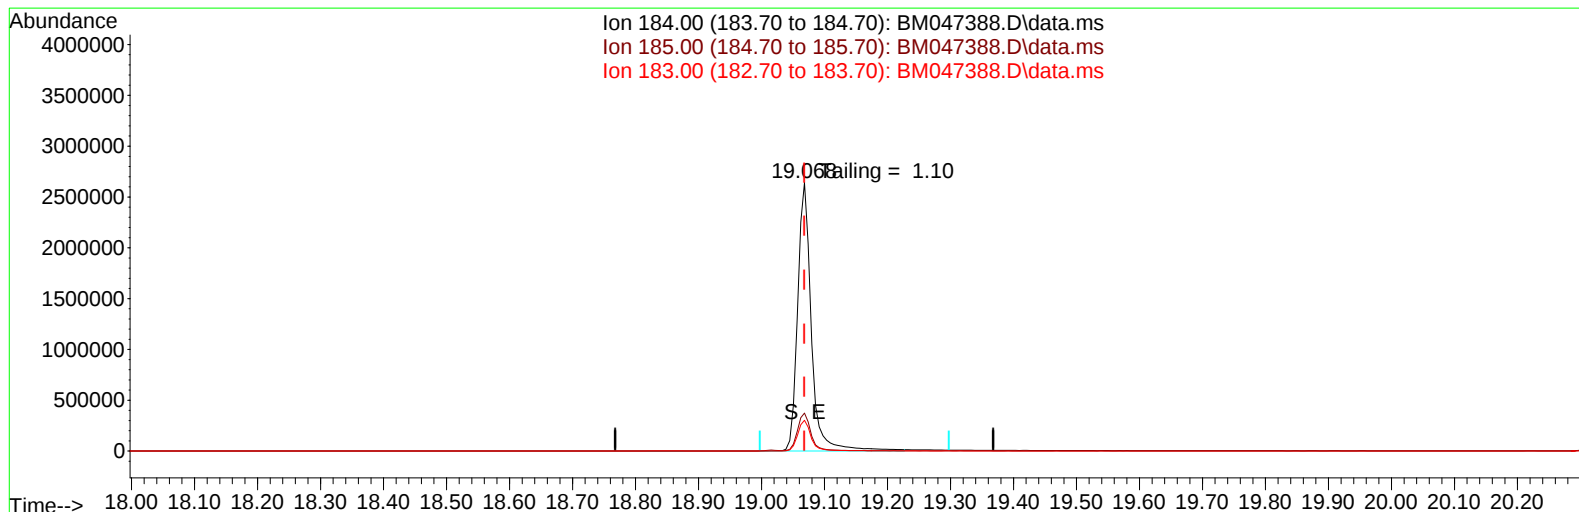

TIC: BM047388.D\data.ms

(77) Benzidine**19.068min (+ 0.000) 105128.63 ng****response 4071227**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.50	11.49
0.00	0.00	0.00